

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091422AL\
 Data File : FC061507.D
 Signal(s) : FID1A.ch
 Acq On : 14 Sep 2022 12:33
 Operator : YP/AJ
 Sample : N4591-01DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 14 12:59:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 31 11:58:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.571	1071025	6.050 ug/ml
Spiked Amount 50.000		Recovery =	12.10%
12) S 1-chlorooctadecane (S...	13.010	879683	6.281 ug/ml
Spiked Amount 50.000		Recovery =	12.56%
Target Compounds			
10) T n-Eicosane (C20)	12.620	206703	1.330 ug/ml
14) T n-Tetracosane (C24)	14.834	82181	0.531 ug/ml
16) T n-Octacosane (C28)	16.832	90989	0.616 ug/ml
17) T n-Tricontane (C30)	17.723	103385	0.749 ug/ml
18) T n-Dotriacontane (C32)	18.556	67900	0.619 ug/ml
19) T n-Tetratriacontane (C34)	19.343	14842	0.192 ug/ml
21) T n-Octatriacontane (C38)	20.814	361129	7.784 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091422AL\
Data File : FC061507.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2022 12:33
Operator : YP/AJ
Sample : N4591-01DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 14 12:59:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 082222.M
Quant Title : GC Extractables
QLast Update : Wed Aug 31 11:58:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

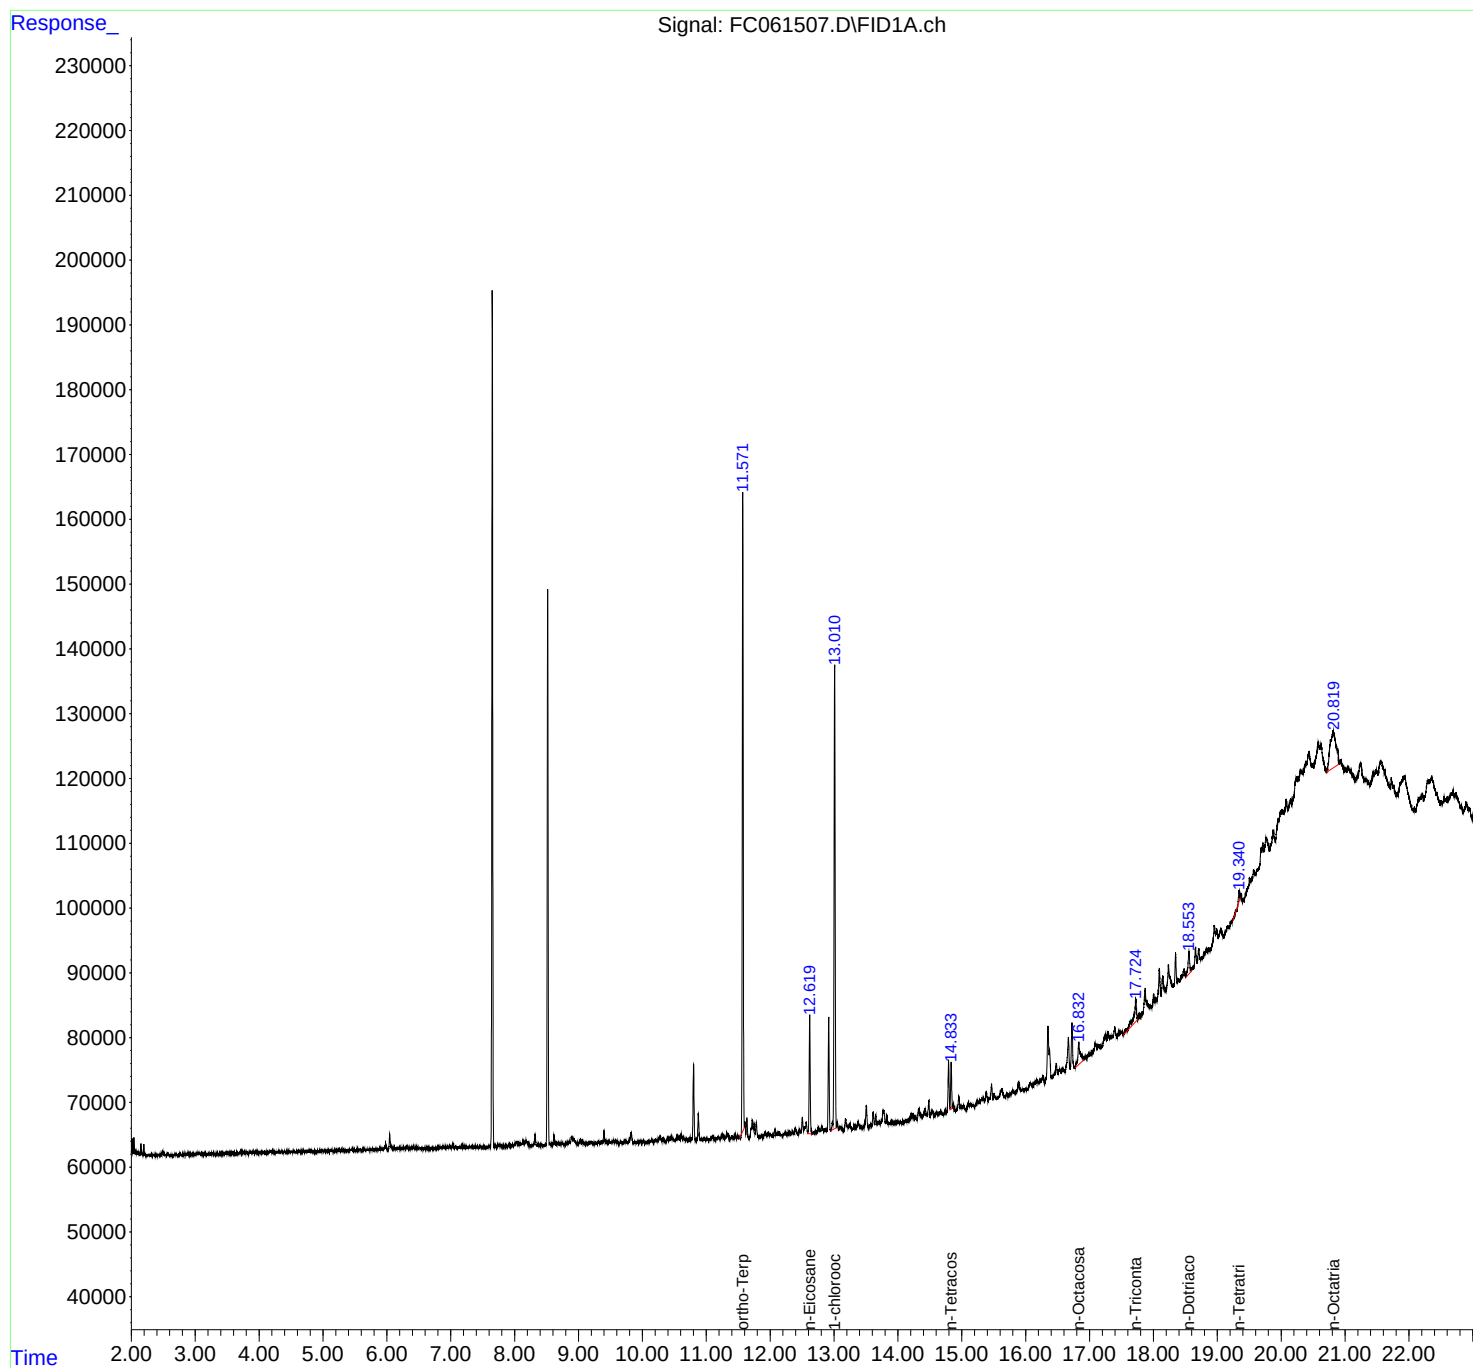


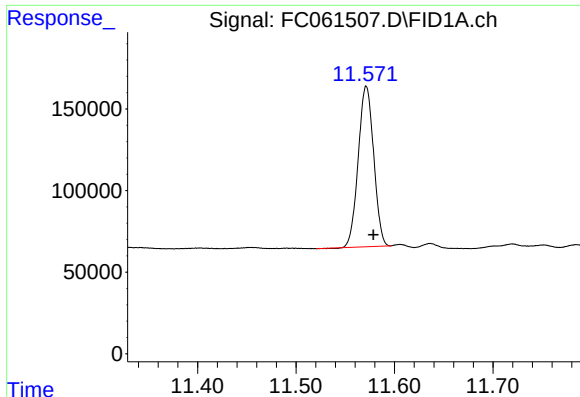

#9 ortho-Terphenyl (SURR)


R.T.: 11.571 min
Delta R.T.: -0.007 min
Response: 1071025
Conc: 6.05 ug/ml

Instrument :
FID_C
ClientSampleId :

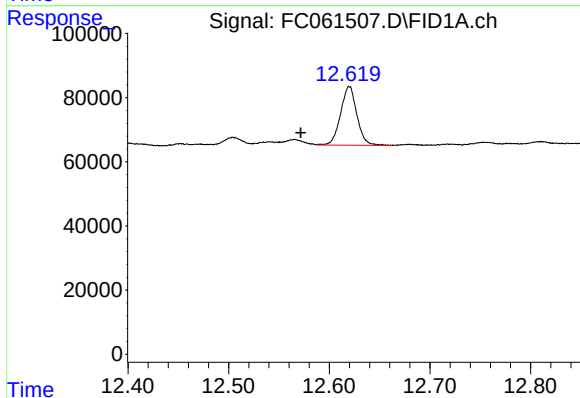


#10 n-Eicosane (C20)

R.T.: 12.620 min
Delta R.T.: 0.048 min
Response: 206703
Conc: 1.33 ug/ml

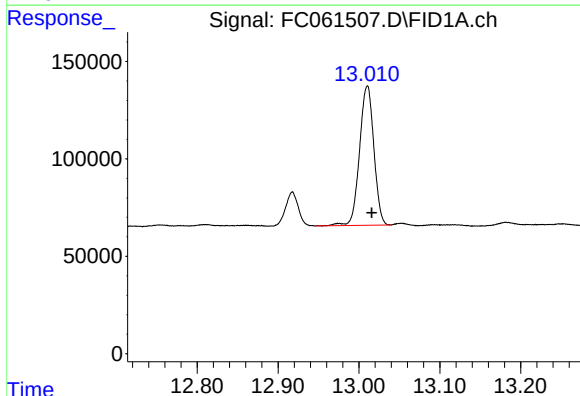


#12 1-chlorooctadecane (SURR)

R.T.: 13.010 min
Delta R.T.: -0.006 min
Response: 879683
Conc: 6.28 ug/ml

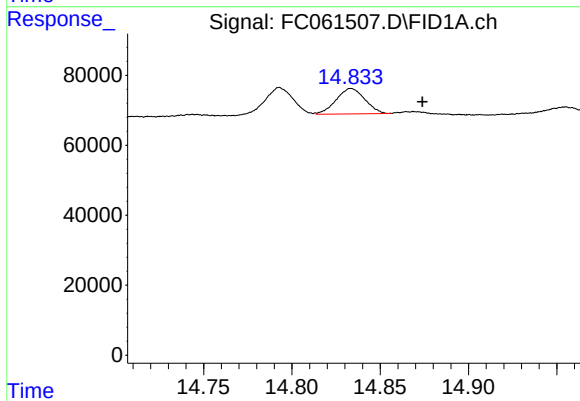

#14 n-Tetracosane (C24)


R.T.: 14.834 min
Delta R.T.: -0.040 min
Response: 82181
Conc: 0.53 ug/ml

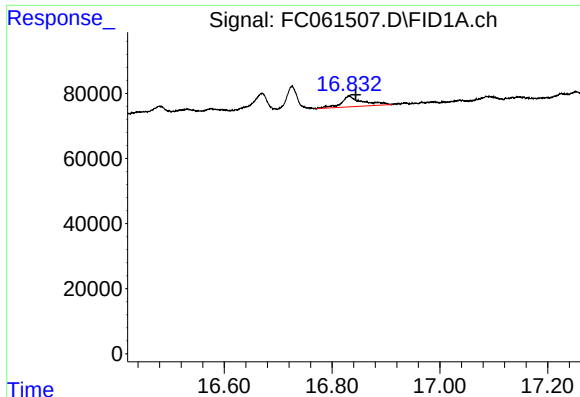

#16 n-Octacosane (C28)


R.T.: 16.832 min
Delta R.T.: -0.012 min
Response: 90989
Conc: 0.62 ug/ml

Instrument :
FID_C
ClientSampleId :

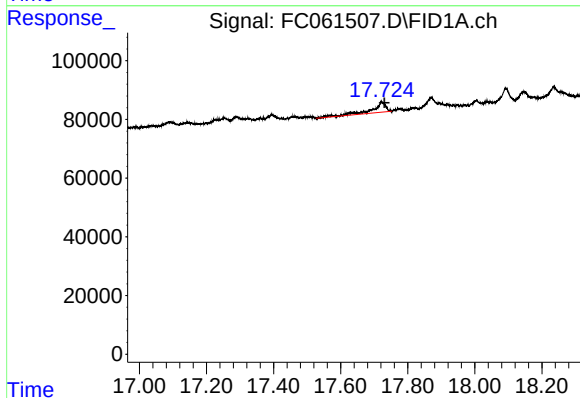


#17 n-Tricontane (C30)

R.T.: 17.723 min
Delta R.T.: -0.008 min
Response: 103385
Conc: 0.75 ug/ml

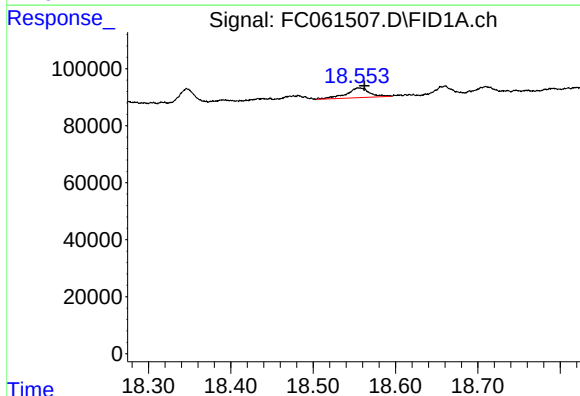


#18 n-Dotriacontane (C32)

R.T.: 18.556 min
Delta R.T.: -0.006 min
Response: 67900
Conc: 0.62 ug/ml

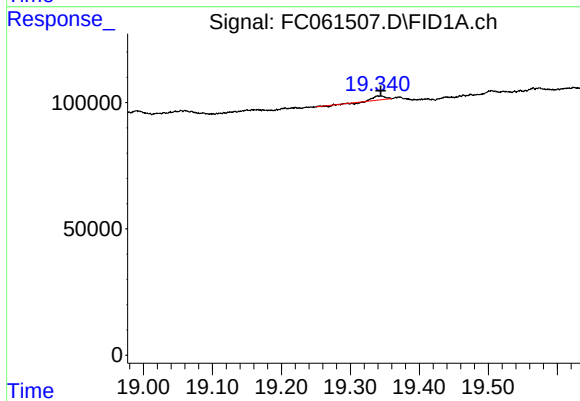

#19 n-Tetratriacontane (C34)

R.T.: 19.343 min
Delta R.T.: -0.001 min
Response: 14842
Conc: 0.19 ug/ml

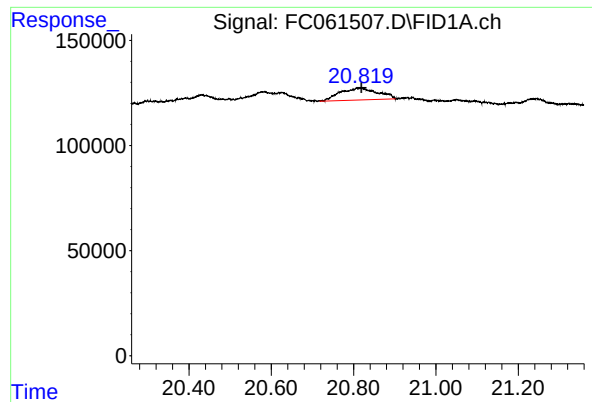

#21 n-Octatriacontane (C38)

R.T.: 20.814 min
Delta R.T.: -0.005 min
Response: 361129
Conc: 7.78 ug/ml

Instrument :

FID_C

ClientSampleId :