

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091623AL\
 Data File : FC064592.D
 Signal(s) : FID1A.ch
 Acq On : 15 Sep 2023 16:07
 Operator : YP/AJ
 Sample : 04416-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 A591

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/18/2023
 Supervised By :Ankita Jodhani 09/18/2023

Integration File: autoint1.e
 Quant Time: Sep 16 00:27:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:25:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.944	5479660	37.620 ug/mlm
Spiked Amount	50.000	Recovery	= 75.24%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC091623AL\
Data File : FC064592.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2023 16:07
Operator : YP/AJ
Sample : 04416-01
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
A591


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/18/2023
Supervised By :Ankita Jodhani 09/18/2023

Integration File: autoint1.e
Quant Time: Sep 16 00:27:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

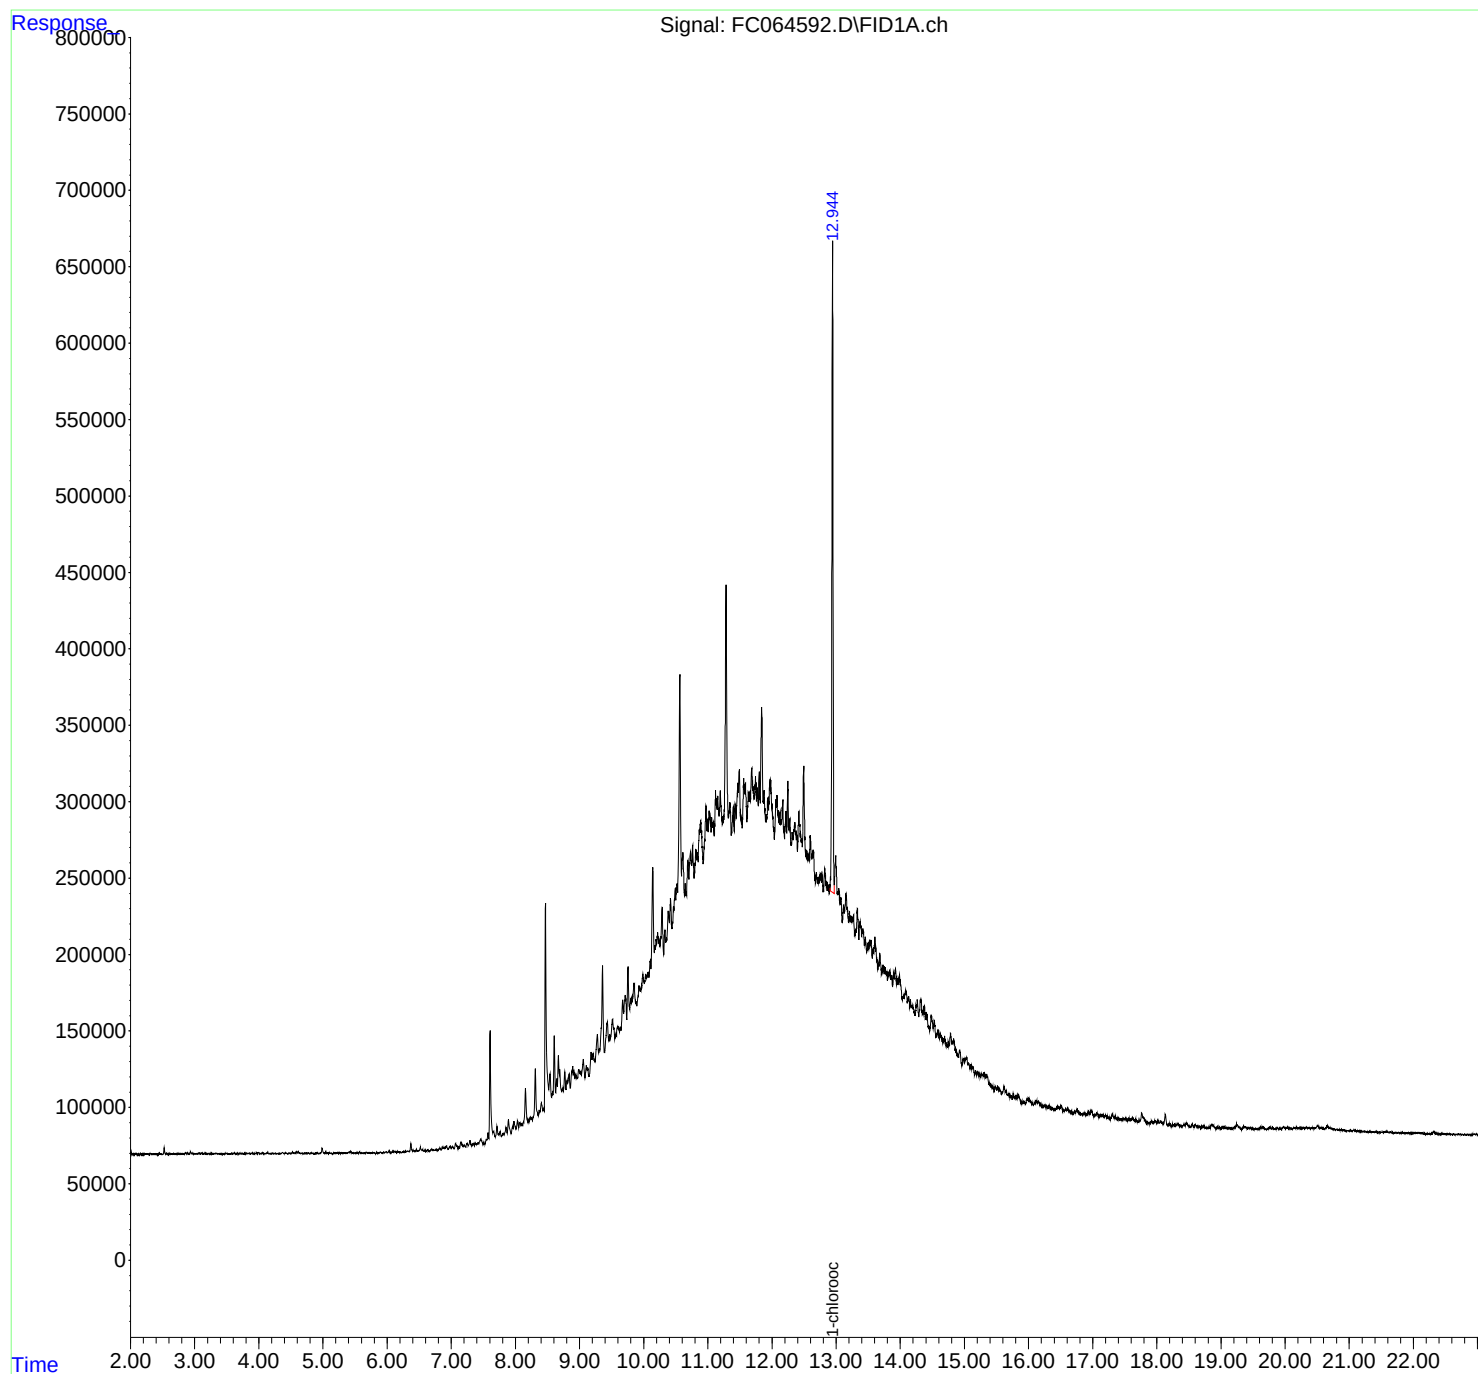

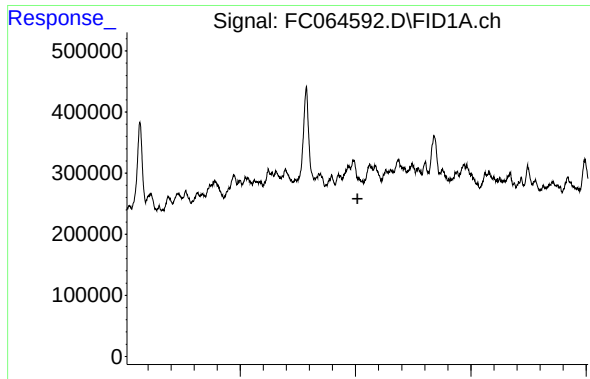


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
A591

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/18/2023
Supervised By :Ankita Jodhani 09/18/2023

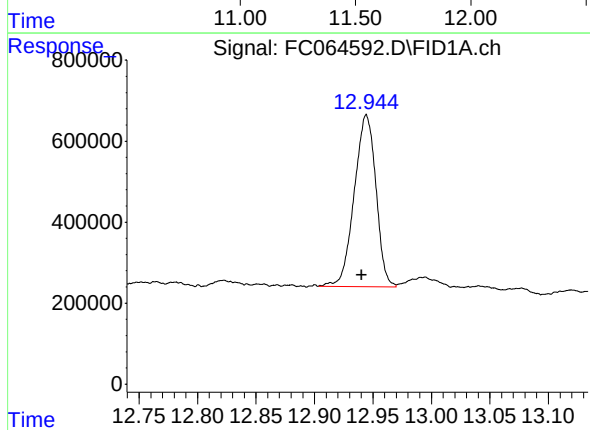

#12 1-chlorooctadecane (SURR)

R.T.: 12.944 min
Delta R.T.: 0.004 min
Response: 5479660
Conc: 37.62 ug/ml m