

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC091924AL\  
Data File : FC067183.D  
Signal(s) : FID1A.ch  
Acq On : 19 Sep 2024 23:09  
Operator : YP/AJ  
Sample : P4103-16D  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
WC-23

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/20/2024  
Supervised By :Ankita Jodhani 09/20/2024

Integration File: autoint1.e  
Quant Time: Sep 20 03:53:24 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Wed Sep 11 02:55:44 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units    |
|--------------------------------|--------|----------|---------------|
| -----                          |        |          |               |
| System Monitoring Compounds    |        |          |               |
| 12) S 1-chlorooctadecane (S... | 12.945 | 4036642  | 41.323 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 82.65%      |

Target Compounds

-----

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC091924AL\  
Data File : FC067183.D  
Signal(s) : FID1A.ch  
Acq On : 19 Sep 2024 23:09  
Operator : YP/AJ  
Sample : P4103-16D  
Misc :  
ALS Vial : 23 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
WC-23


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/20/2024  
Supervised By :Ankita Jodhani 09/20/2024

Integration File: autoint1.e  
Quant Time: Sep 20 03:53:24 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 091024.M  
Quant Title : GC Extractables  
QLast Update : Wed Sep 11 02:55:44 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

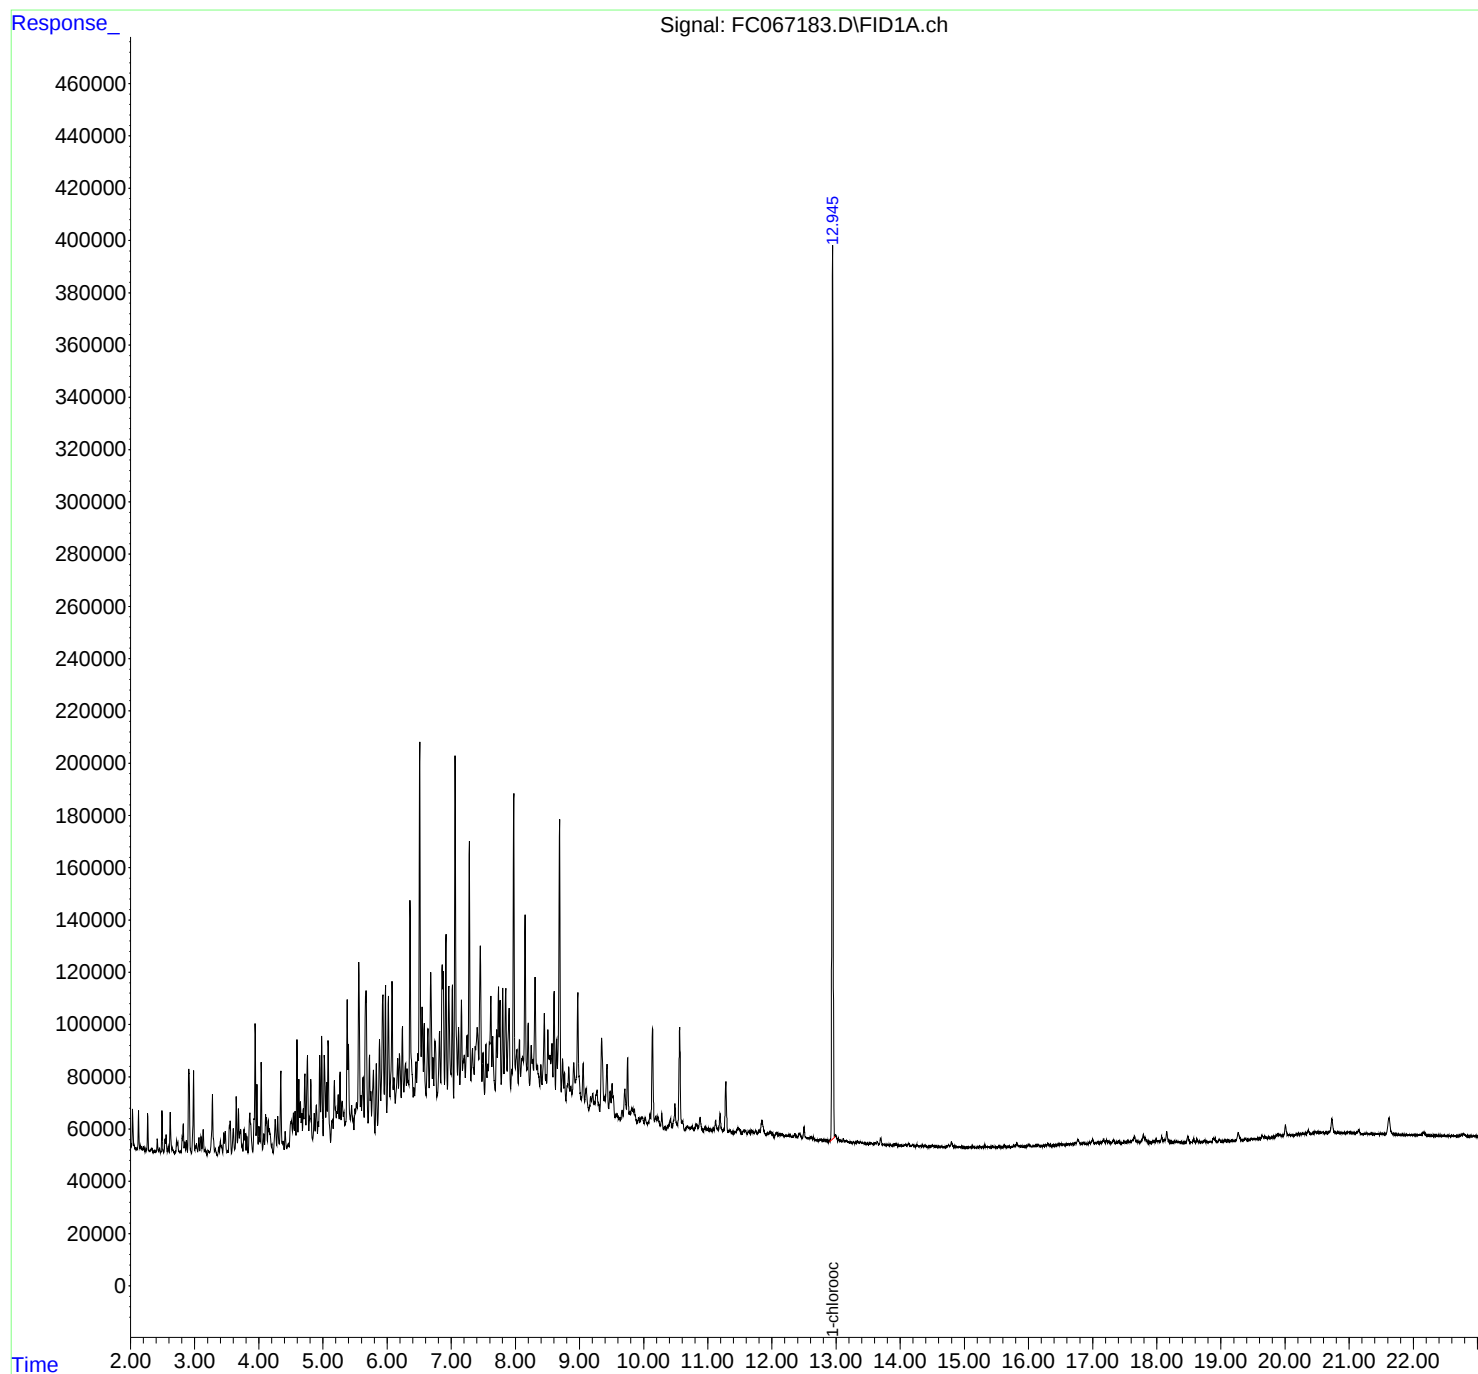

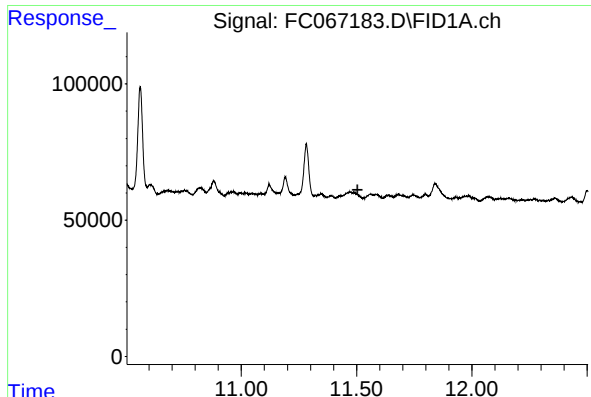


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.504 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :  
WC-23

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 09/20/2024  
Supervised By :Ankita Jodhani 09/20/2024

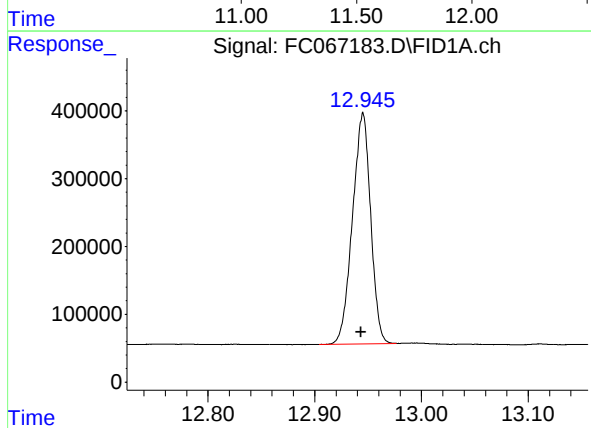

#12 1-chlorooctadecane (SURR)

R.T.: 12.945 min  
Delta R.T.: 0.001 min  
Response: 4036642  
Conc: 41.32 ug/ml m