

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC092023AL\  
Data File : FC064623.D  
Signal(s) : FID1A.ch  
Acq On : 20 Sep 2023 07:55  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 20 10:57:43 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 091523.M  
Quant Title : GC Extractables  
QLast Update : Fri Sep 15 01:25:53 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                          | R.T.   | Response | Conc Units  |
|-----------------------------|--------------------------|--------|----------|-------------|
| -----                       |                          |        |          |             |
| System Monitoring Compounds |                          |        |          |             |
| Target Compounds            |                          |        |          |             |
| 14) T                       | n-Tetracosane (C24)      | 14.768 | 50011    | 0.315 ug/ml |
| 15) T                       | n-Hexacosane (C26)       | 15.817 | 55937    | 0.366 ug/ml |
| 19) T                       | n-Tetratriacontane (C34) | 19.250 | 33399    | 0.235 ug/ml |
| 22) T                       | n-Tetracontane (C40)     | 21.558 | 69019    | 0.507 ug/ml |
| -----                       |                          |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC092023AL\  
Data File : FC064623.D  
Signal(s) : FID1A.ch  
Acq On : 20 Sep 2023 07:55  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 20 10:57:43 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 091523.M  
Quant Title : GC Extractables  
QLast Update : Fri Sep 15 01:25:53 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 u1  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

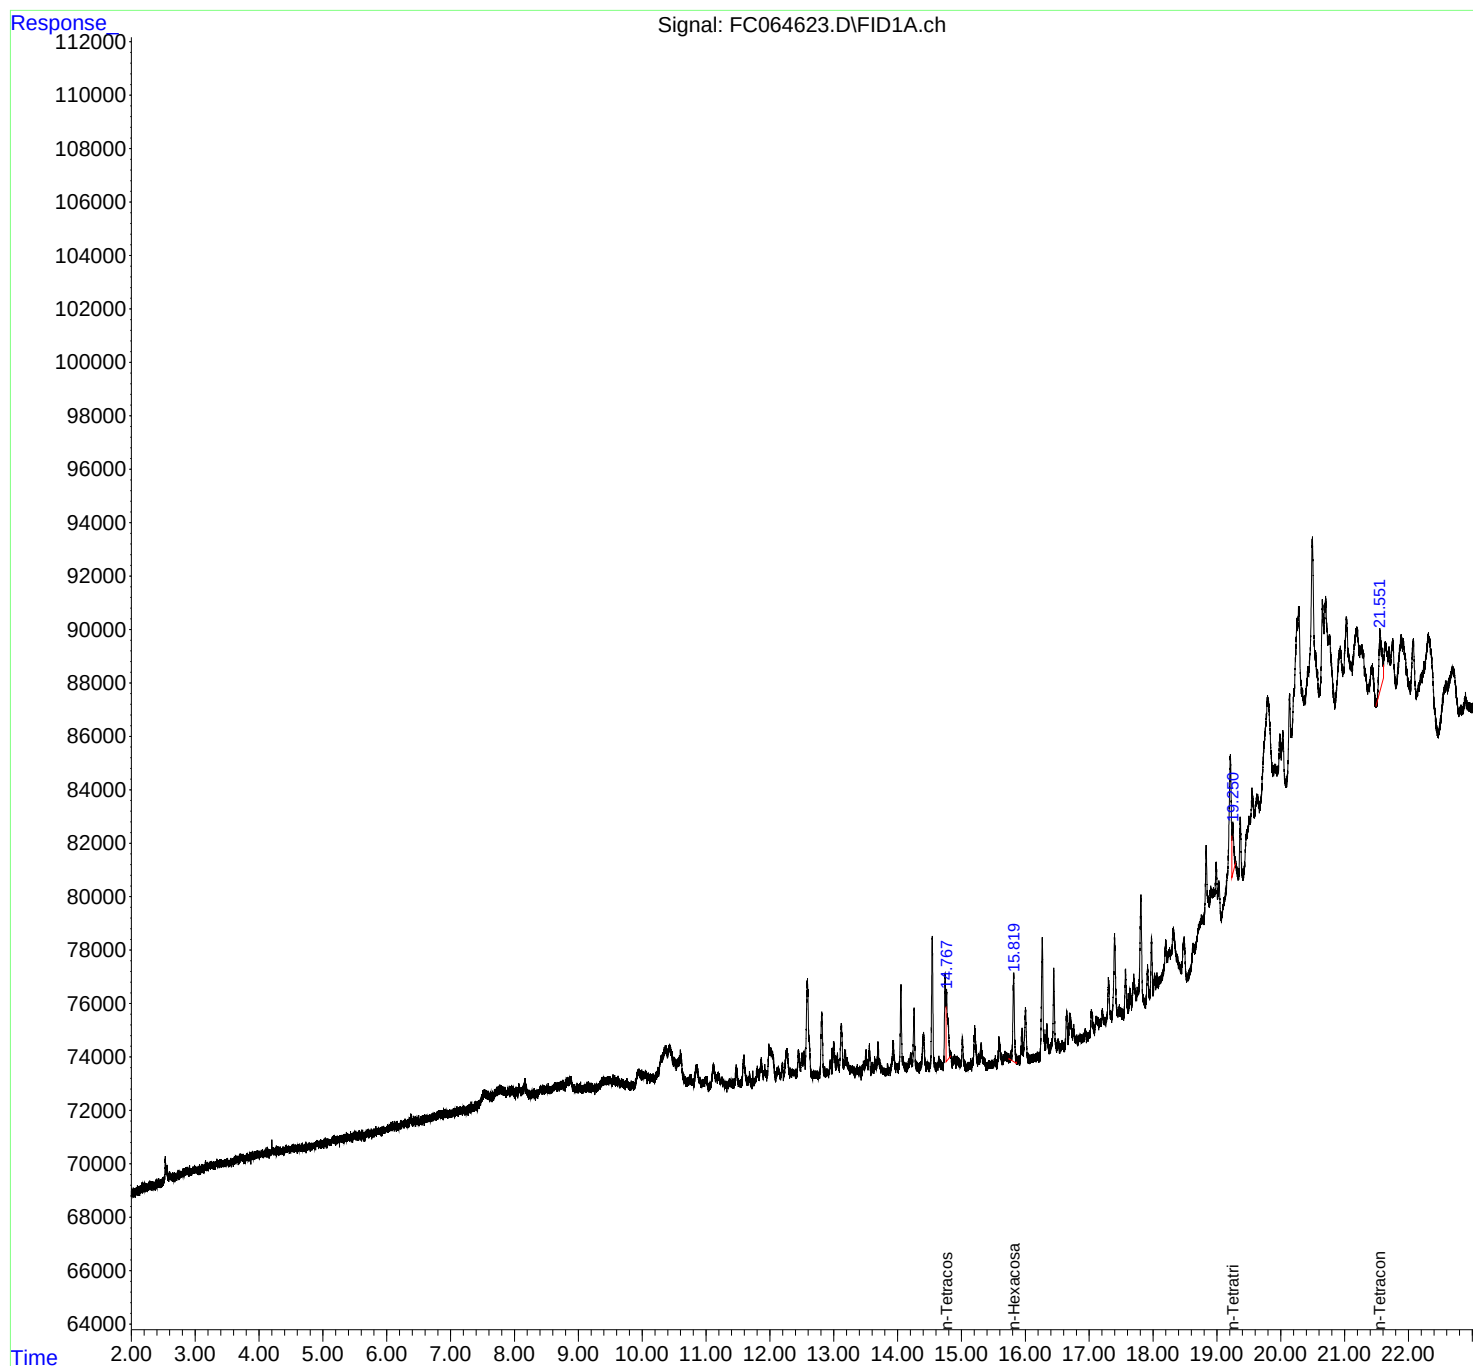


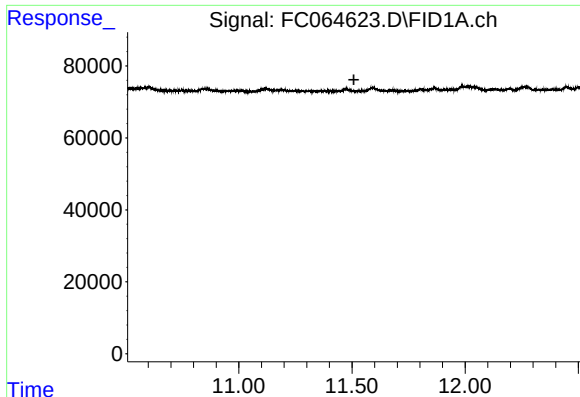

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 11.508 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :

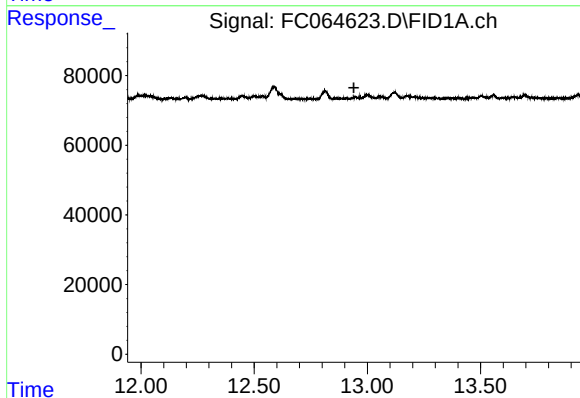


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T.: 12.940 min  
Response: 0  
Conc: N.D.

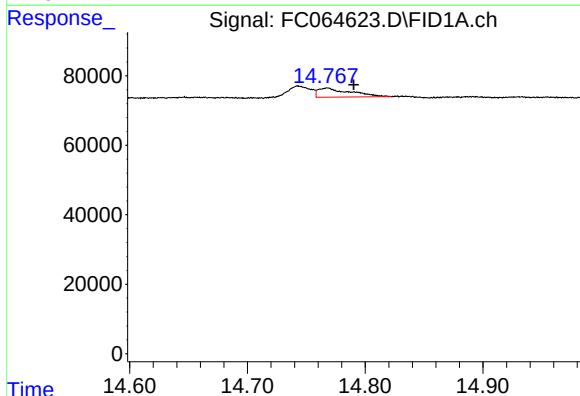


#14 n-Tetracosane (C24)

R.T.: 14.768 min  
Delta R.T.: -0.022 min  
Response: 50011  
Conc: 0.32 ug/ml

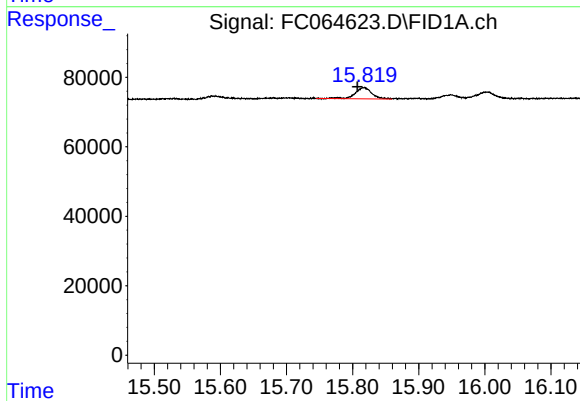

#15 n-Hexacosane (C26)


R.T.: 15.817 min  
Delta R.T.: 0.010 min  
Response: 55937  
Conc: 0.37 ug/ml

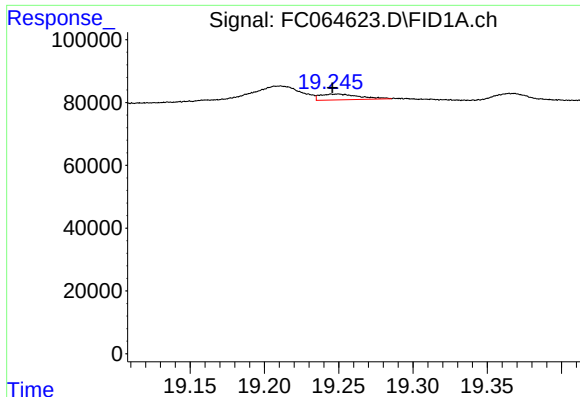

#19 n-Tetratriacontane (C34)

R.T.: 19.250 min  
Delta R.T.: 0.004 min  
Response: 33399  
Conc: 0.23 ug/ml

Instrument :  
FID\_C  
ClientSampleId :

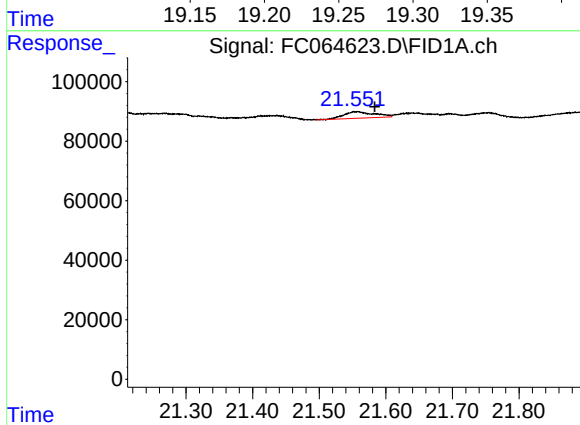

#22 n-Tetracontane (C40)

R.T.: 21.558 min  
Delta R.T.: -0.025 min  
Response: 69019  
Conc: 0.51 ug/ml