

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092023AL\
Data File : FC064626.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2023 09:49
Operator : YP/AJ
Sample : 04434-01DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
DIRTY-PILE-3DL

Integration File: autoint1.e
Quant Time: Sep 20 10:58:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092023AL\
Data File : FC064626.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2023 09:49
Operator : YP/AJ
Sample : 04434-01DL 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
DIRTY-PILE-3DL

Integration File: autoint1.e
Quant Time: Sep 20 10:58:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

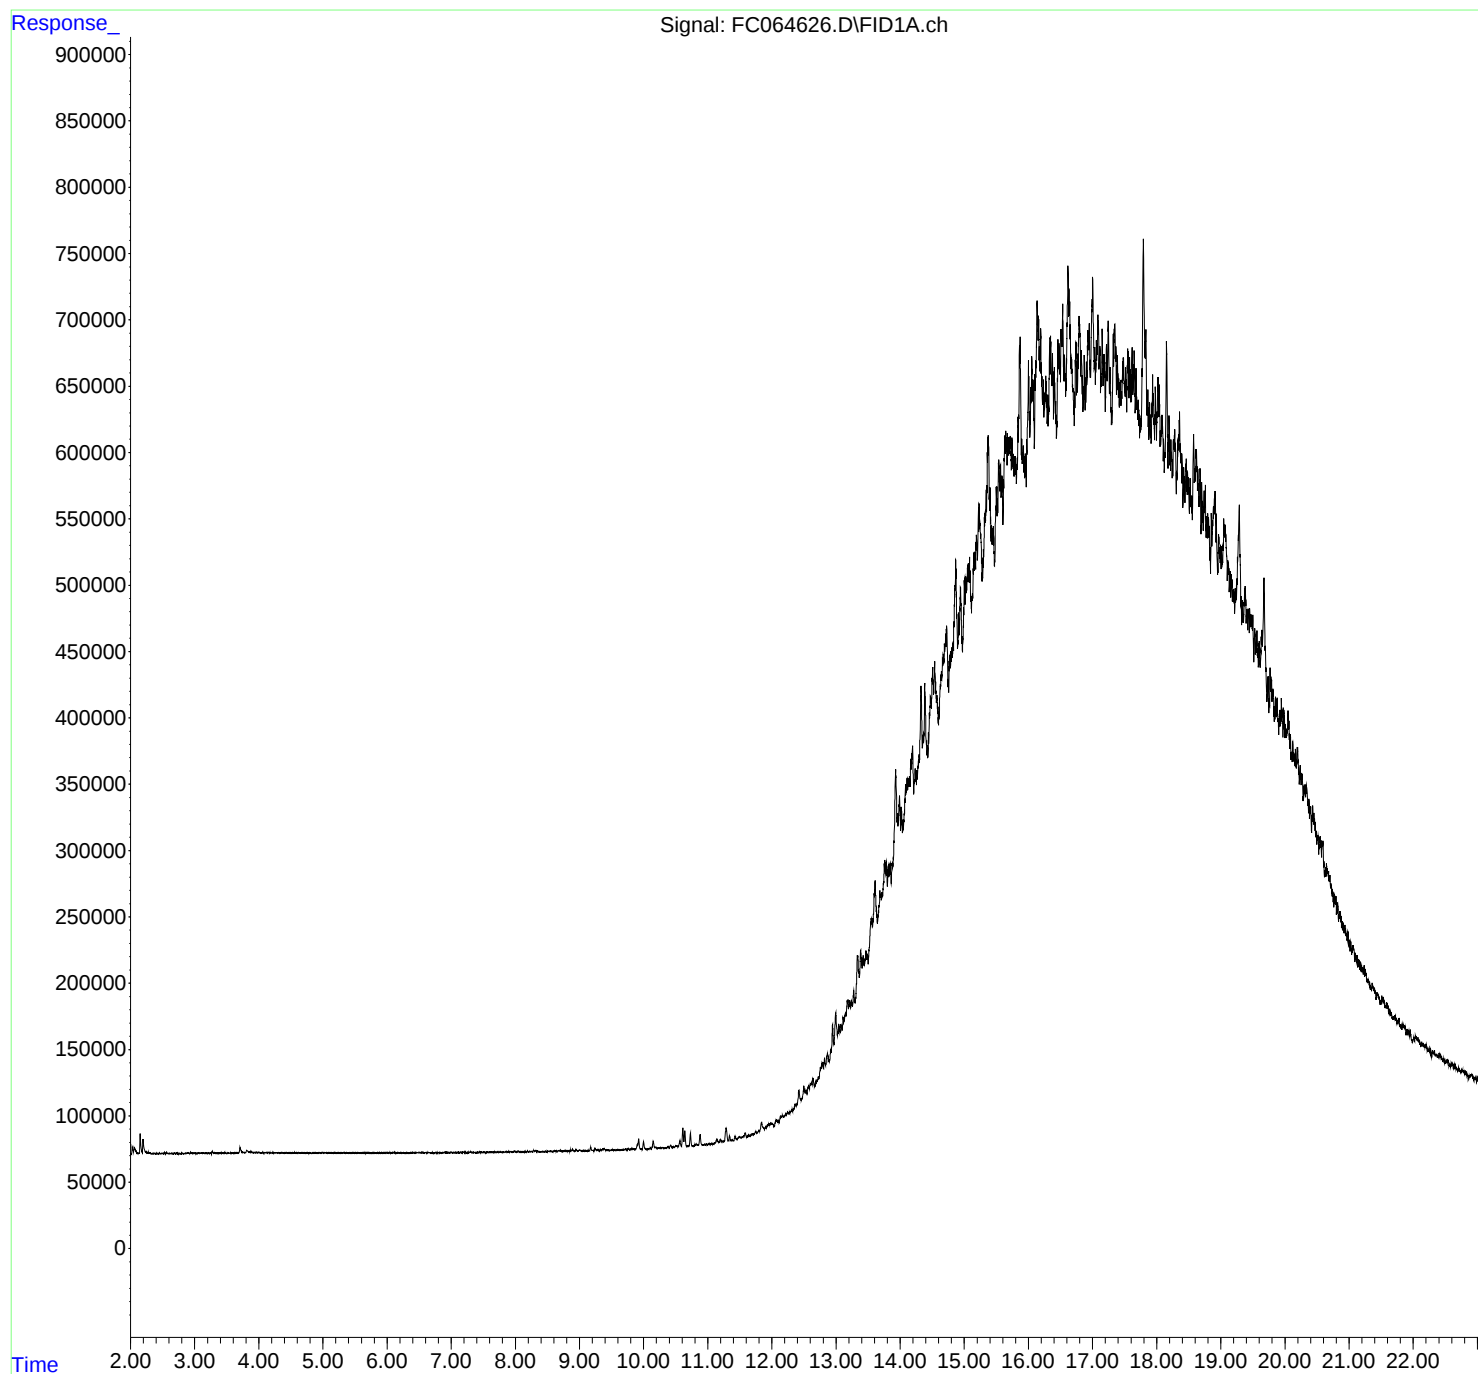


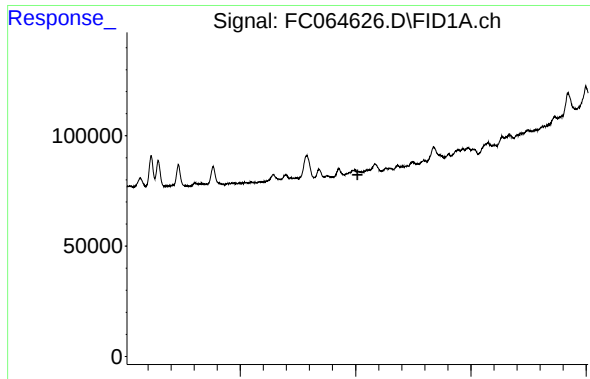

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
DIRTY-PILE-3DL

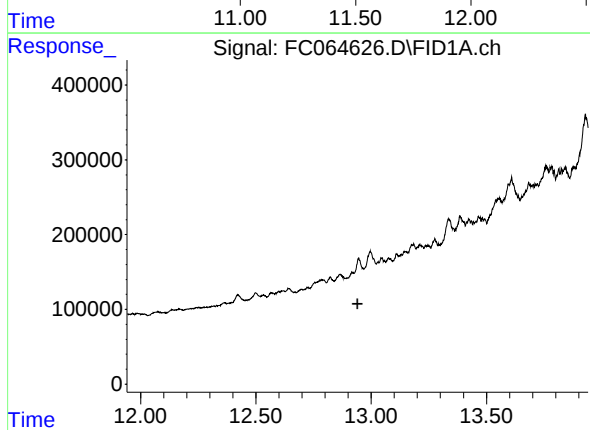

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.940 min
Response: 0
Conc: N.D.