

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092123AL\
 Data File : FC064639.D
 Signal(s) : FID1A.ch
 Acq On : 21 Sep 2023 21:04
 Operator : YP/AJ
 Sample : 04540-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TRANSCO-M-R-HEATER

Integration File: autoint1.e
 Quant Time: Sep 22 00:38:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:25:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.945	3896604	26.752 ug/ml
Spiked Amount	50.000	Recovery	= 53.50%

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092123AL\
Data File : FC064639.D
Signal(s) : FID1A.ch
Acq On : 21 Sep 2023 21:04
Operator : YP/AJ
Sample : 04540-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
TRANSCO-M-R-HEATER

Integration File: autoint1.e
Quant Time: Sep 22 00:38:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

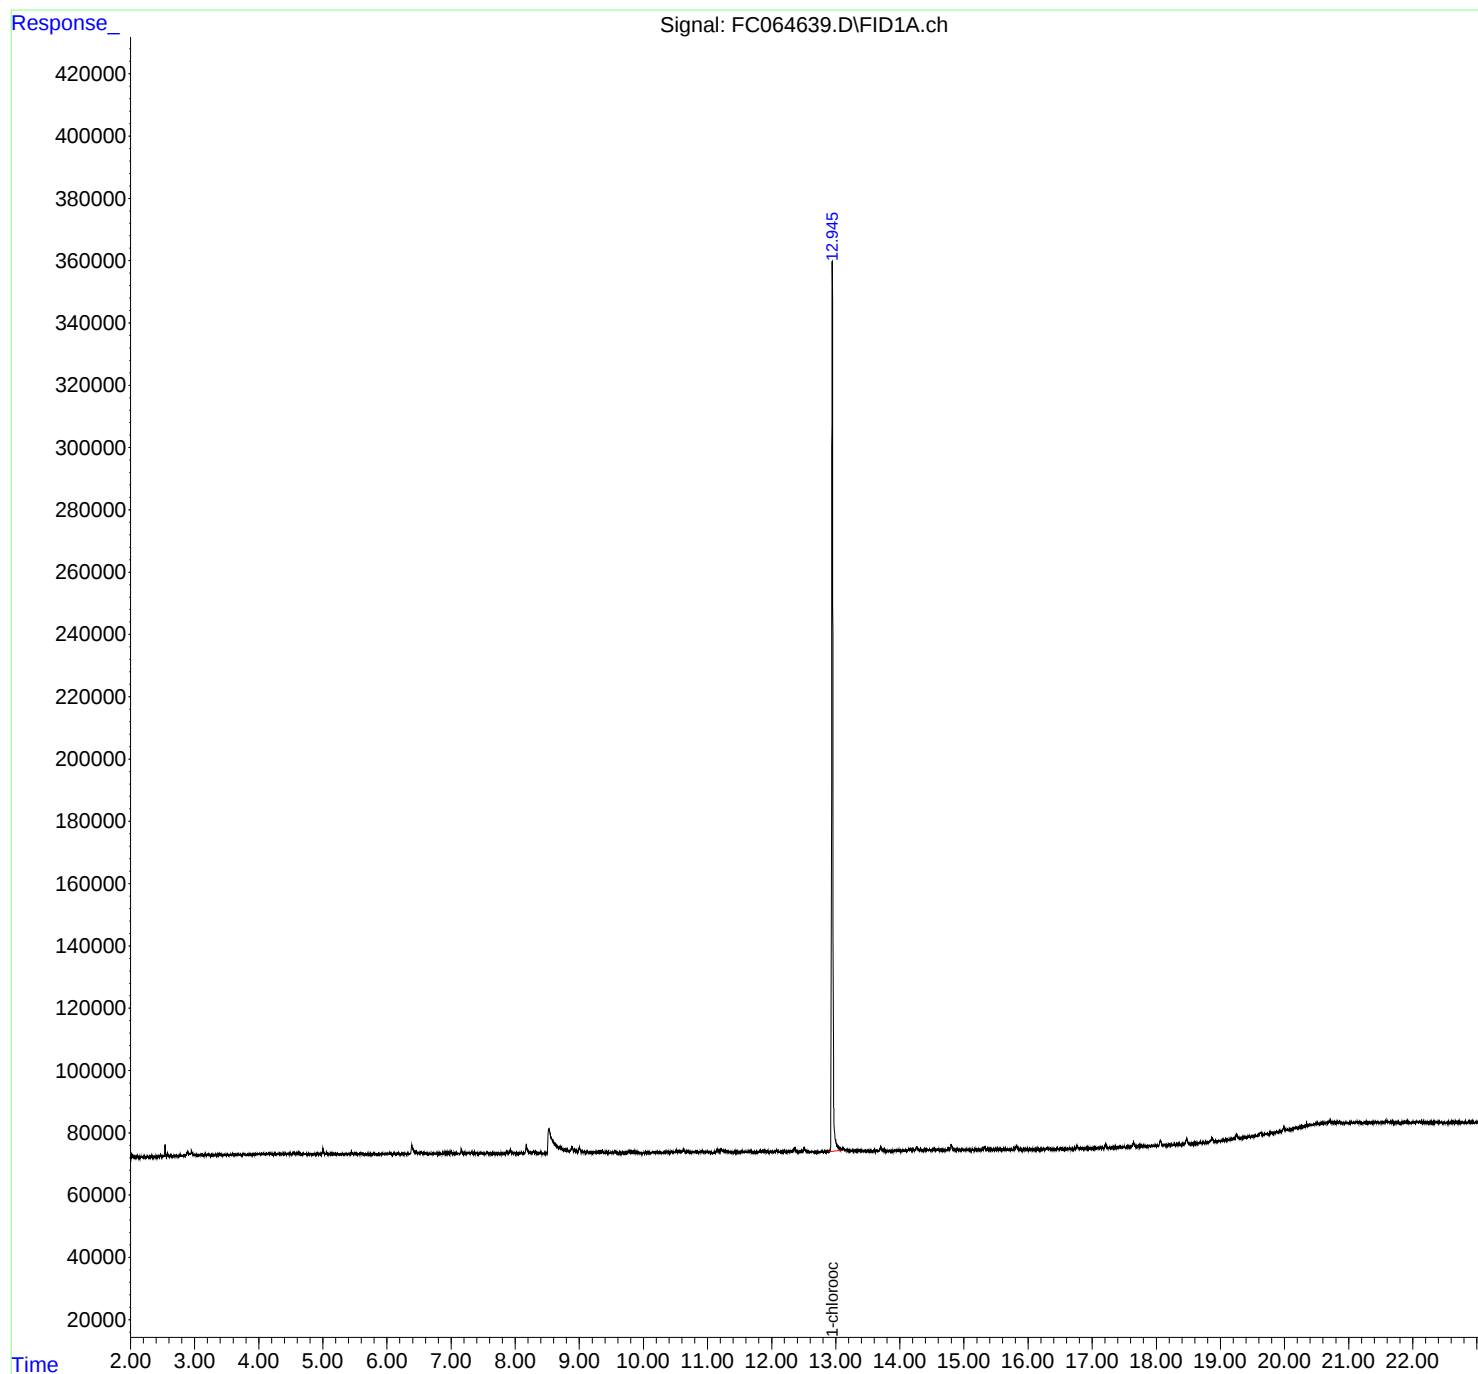


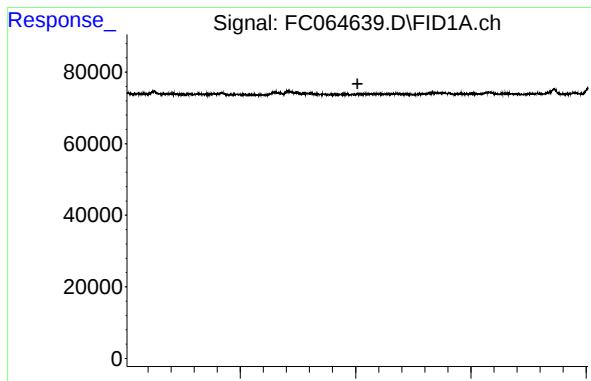

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
TRANSCO-M-R-HEATER

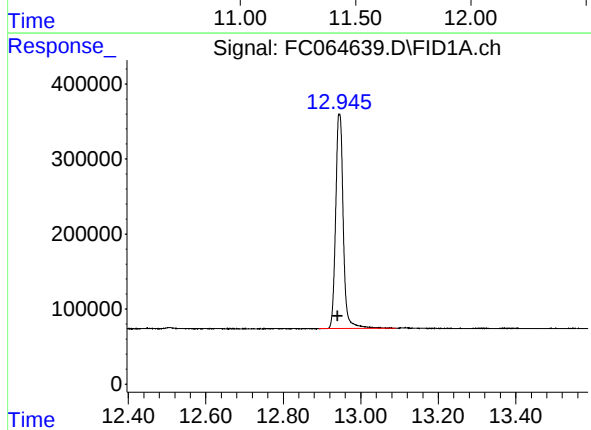

#12 1-chlorooctadecane (SURR)

R.T.: 12.945 min
Delta R.T.: 0.004 min
Response: 3896604
Conc: 26.75 ug/ml