

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092222AL\
 Data File : FC061602.D
 Signal(s) : FID1A.ch
 Acq On : 22 Sep 2022 15:22
 Operator : YP/AJ
 Sample : N4630-14DL 100X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 23 03:04:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092022.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 20 18:33:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.009	148003	1.083 ug/ml
Spiked Amount 50.000		Recovery =	2.17%
Target Compounds			
7) T n-Hexadecane (C16)	9.769	56682	0.367 ug/ml
13) T n-Docosane (C22)	13.760	56240	0.350 ug/ml
14) T n-Tetracosane (C24)	14.866	43264	0.270 ug/ml
15) T n-Hexacosane (C26)	15.931	174010	1.098 ug/ml
16) T n-Octacosane (C28)	16.860	474044	3.058 ug/ml
17) T n-Tricontane (C30)	17.723	284009	1.846 ug/ml
18) T n-Dotriacontane (C32)	18.560	101186	0.669 ug/ml
19) T n-Tetratriacontane (C34)	19.344	295816	2.086 ug/ml
20) T n-Hexatriacontane (C36)	20.079	97511	0.706 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092222AL\
Data File : FC061602.D
Signal(s) : FID1A.ch
Acq On : 22 Sep 2022 15:22
Operator : YP/AJ
Sample : N4630-14DL 100X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 23 03:04:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092022.M
Quant Title : GC Extractables
QLast Update : Tue Sep 20 18:33:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

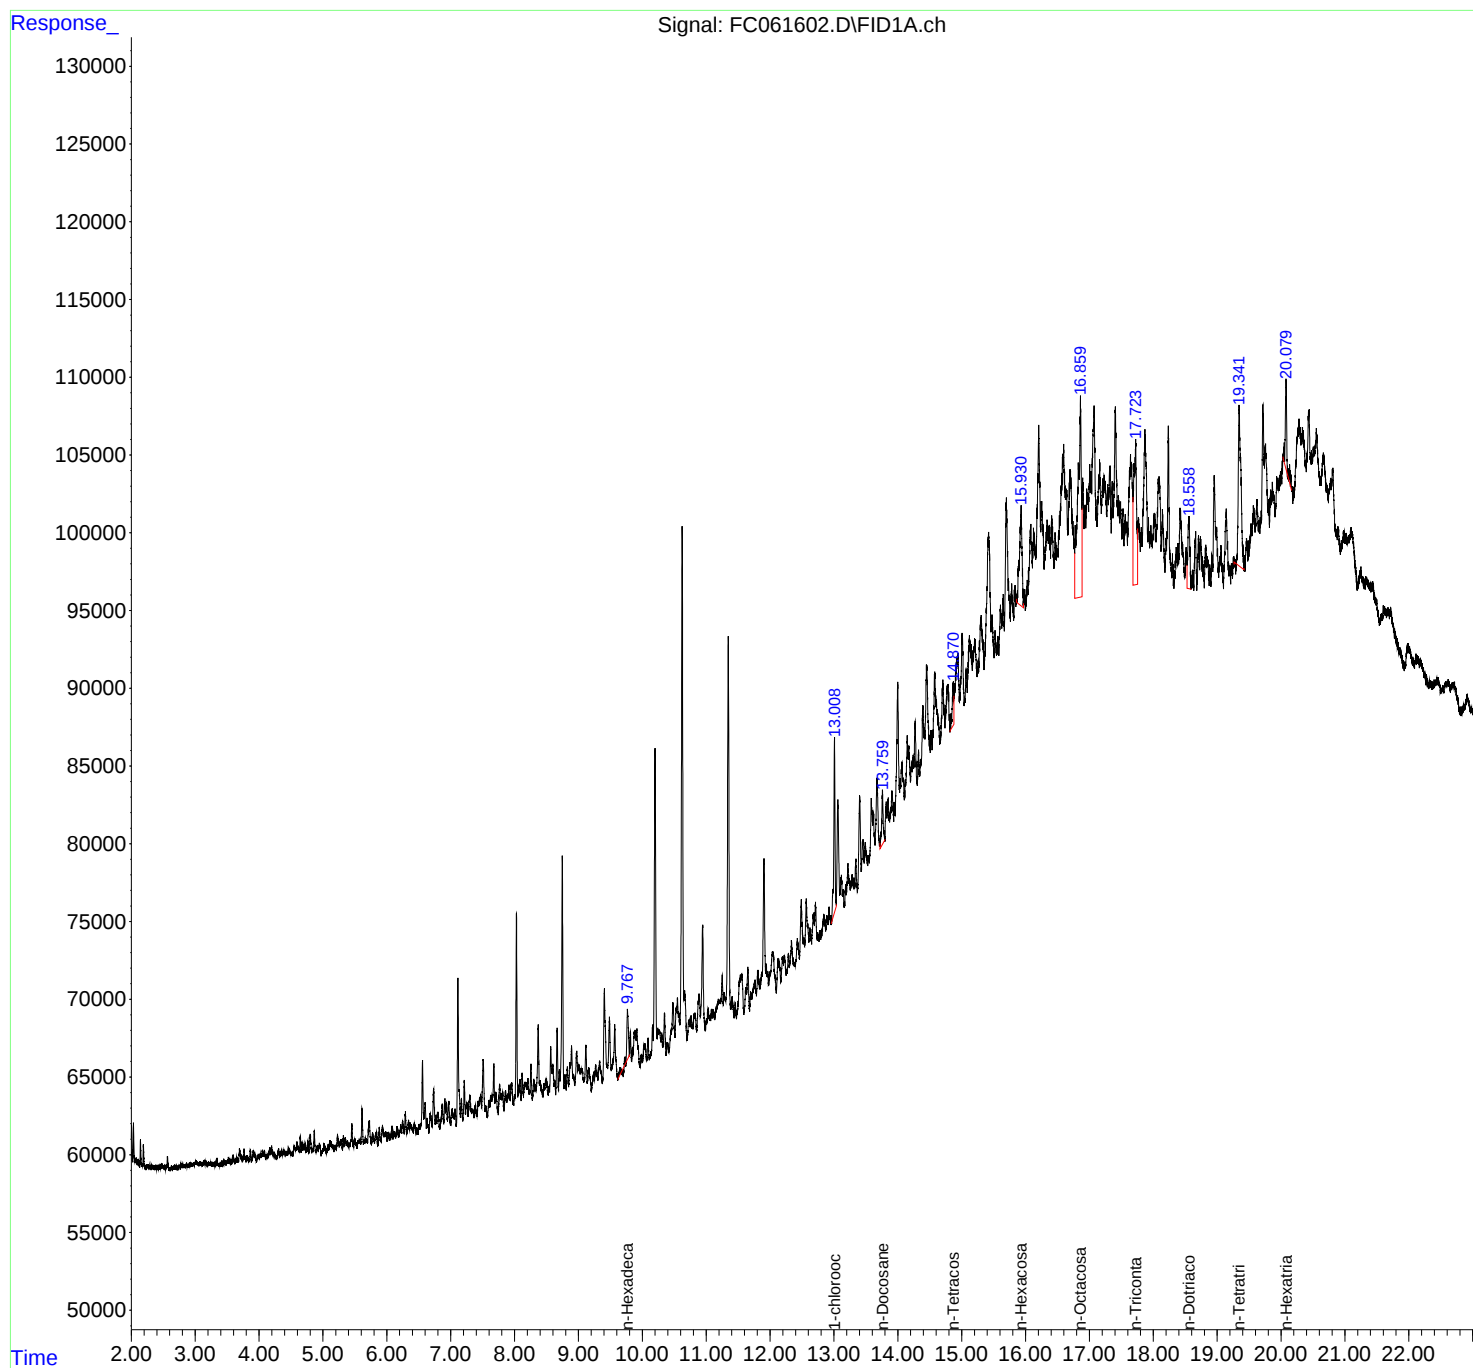


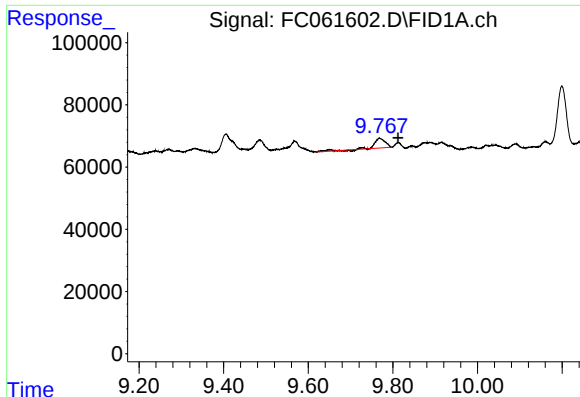

#7 n-Hexadecane (C16)


R.T.: 9.769 min
Delta R.T.: -0.043 min
Response: 56682
Conc: 0.37 ug/ml

Instrument :
FID_C
ClientSampleId :

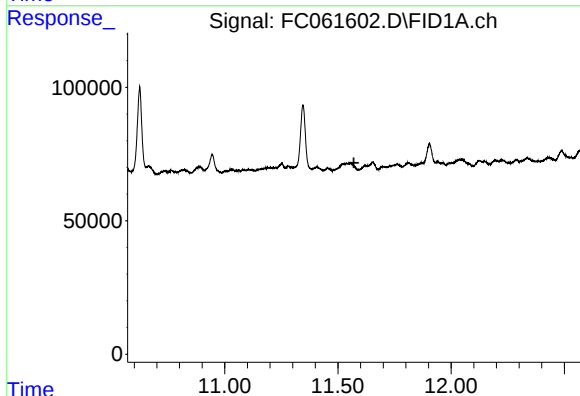


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.571 min
Response: 0
Conc: N.D.

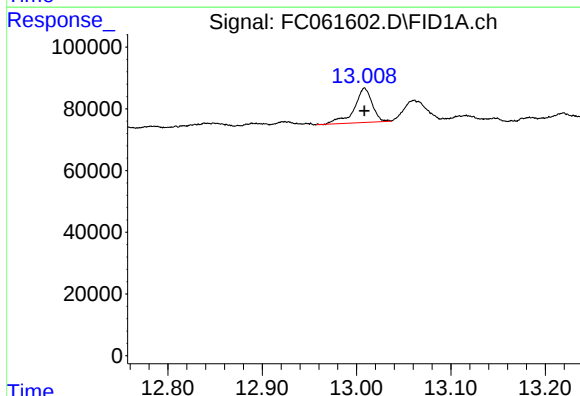


#12 1-chlorooctadecane (SURR)

R.T.: 13.009 min
Delta R.T.: 0.000 min
Response: 148003
Conc: 1.08 ug/ml

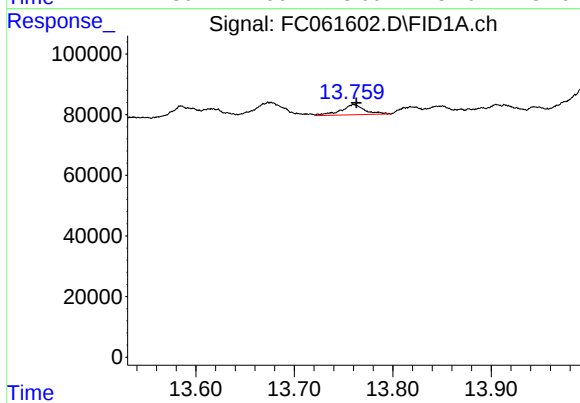

#13 n-Docosane (C22)


R.T.: 13.760 min
Delta R.T.: -0.003 min
Response: 56240
Conc: 0.35 ug/ml

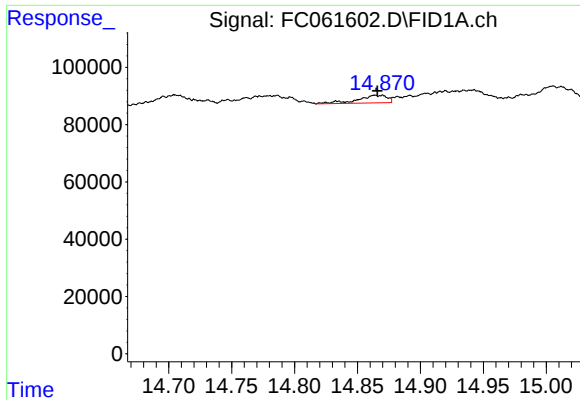

#14 n-Tetracosane (C24)


R.T.: 14.866 min
Delta R.T.: 0.000 min
Response: 43264
Conc: 0.27 ug/ml

Instrument :
FID_C
ClientSampleId :

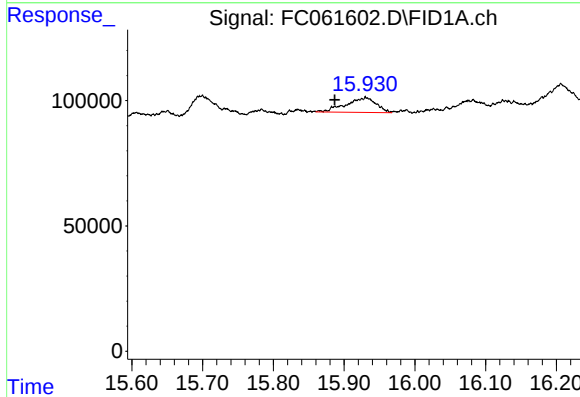


#15 n-Hexacosane (C26)

R.T.: 15.931 min
Delta R.T.: 0.044 min
Response: 174010
Conc: 1.10 ug/ml

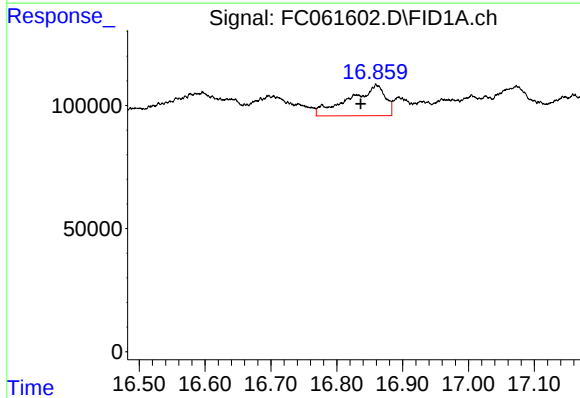


#16 n-Octacosane (C28)

R.T.: 16.860 min
Delta R.T.: 0.024 min
Response: 474044
Conc: 3.06 ug/ml

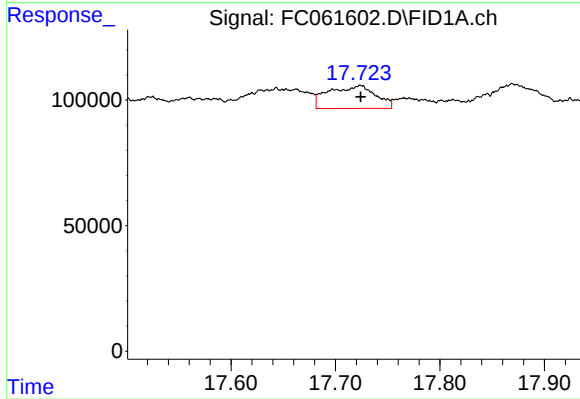

#17 n-Tricontane (C30)


R.T.: 17.723 min
Delta R.T.: 0.000 min
Response: 284009
Conc: 1.85 ug/ml

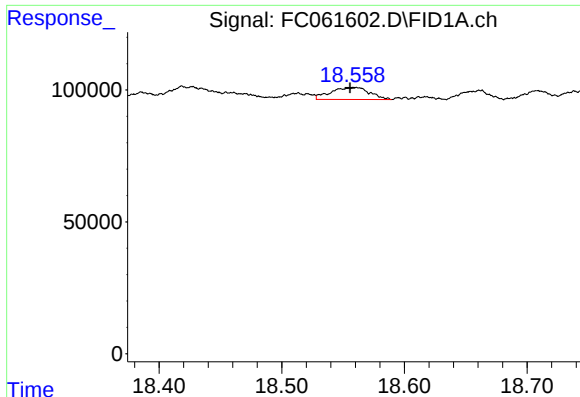

#18 n-Dotriacontane (C32)


R.T.: 18.560 min
Delta R.T.: 0.004 min
Response: 101186
Conc: 0.67 ug/ml

Instrument :
FID_C
ClientSampleId :

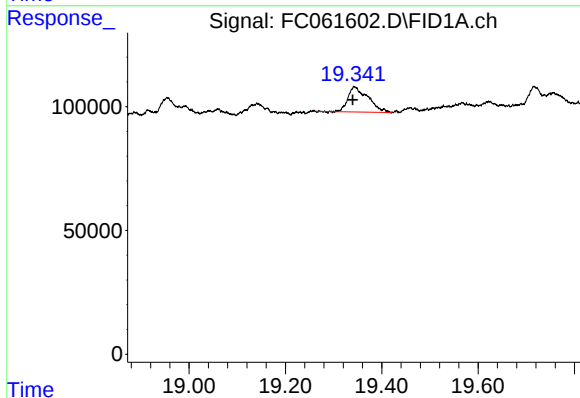

#19 n-Tetratriacontane (C34)

R.T.: 19.344 min
Delta R.T.: 0.004 min
Response: 295816
Conc: 2.09 ug/ml

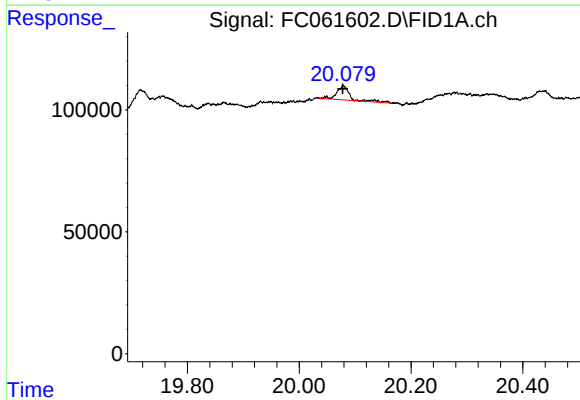

#20 n-Hexatriacontane (C36)

R.T.: 20.079 min
Delta R.T.: 0.001 min
Response: 97511
Conc: 0.71 ug/ml