

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092222AL\
 Data File : FC061603.D
 Signal(s) : FID1A.ch
 Acq On : 22 Sep 2022 16:40
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 23 03:04:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092022.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 20 18:33:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.339	128206	0.904 ug/ml
20) T n-Hexatriacontane (C36)	20.077	113300	0.821 ug/ml
21) T n-Octatriacontane (C38)	20.810	141506	1.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092222AL\
Data File : FC061603.D
Signal(s) : FID1A.ch
Acq On : 22 Sep 2022 16:40
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 23 03:04:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092022.M
Quant Title : GC Extractables
QLast Update : Tue Sep 20 18:33:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

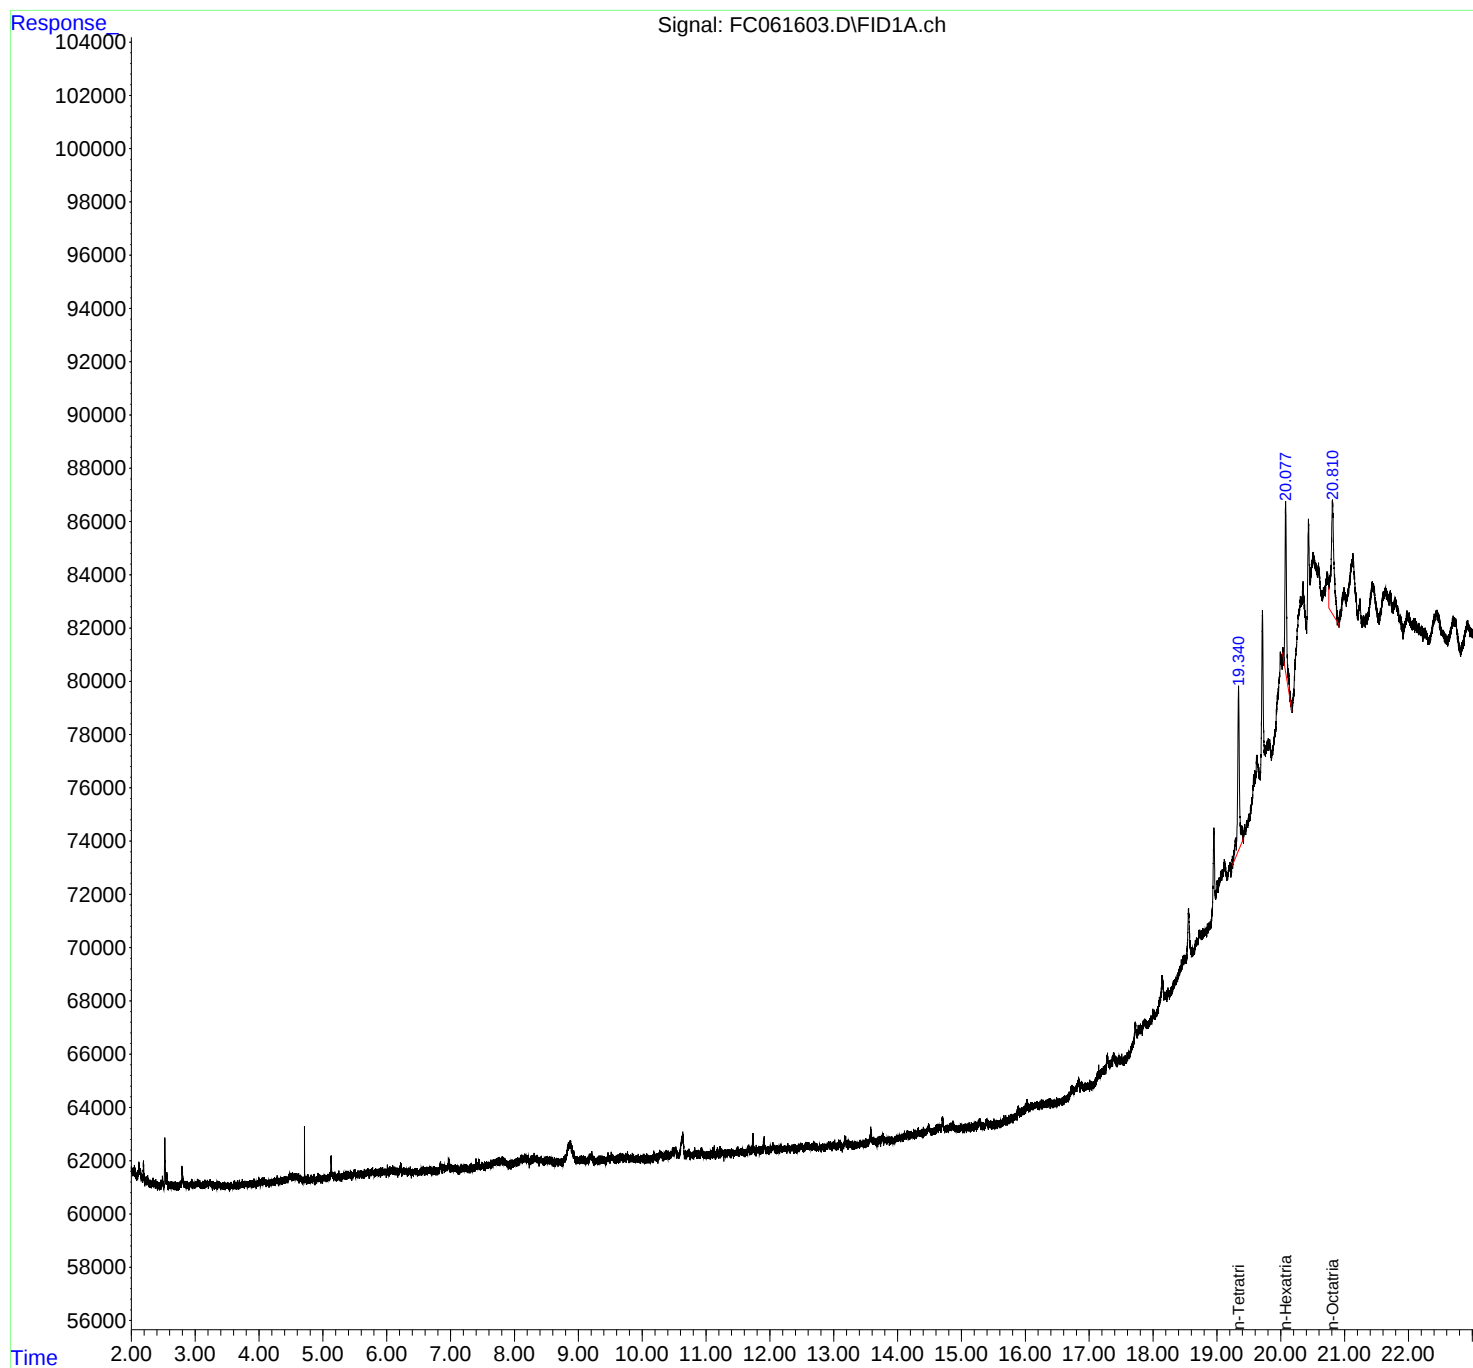


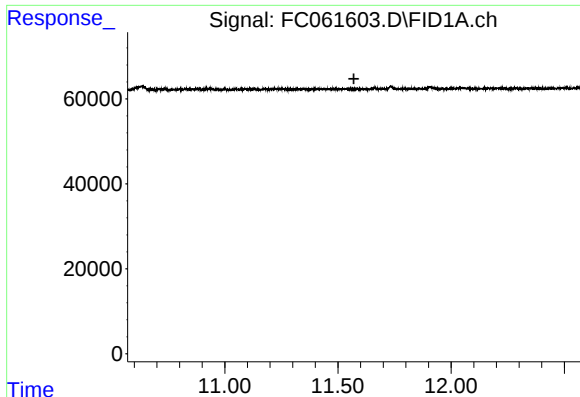

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.571 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

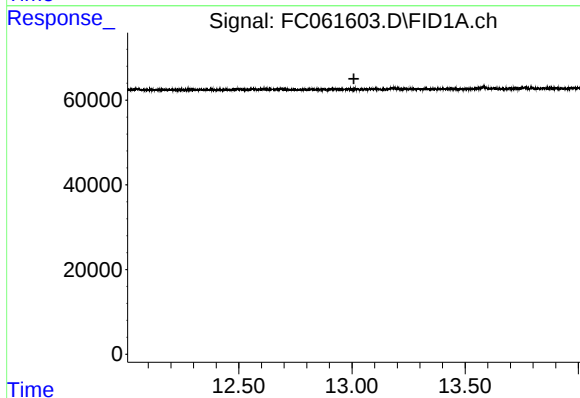


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.008 min
Response: 0
Conc: N.D.

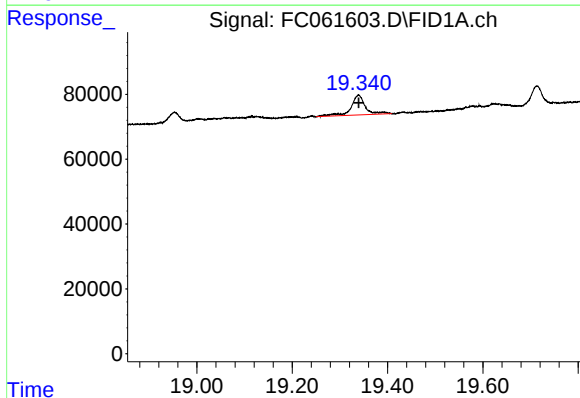


#19 n-Tetratriacontane (C34)

R.T.: 19.339 min
Delta R.T.: 0.000 min
Response: 128206
Conc: 0.90 ug/ml

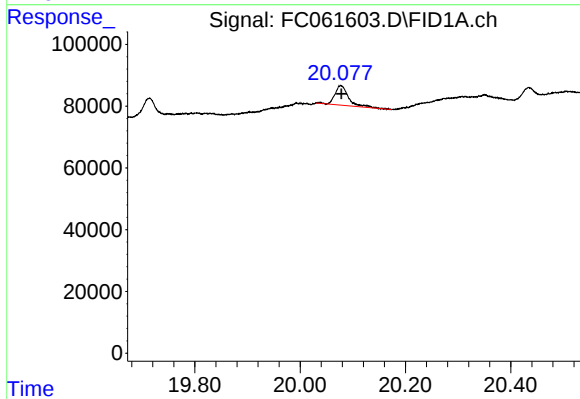

#20 n-Hexatriacontane (C36)

R.T.: 20.077 min
Delta R.T.: 0.000 min
Response: 113300
Conc: 0.82 ug/ml

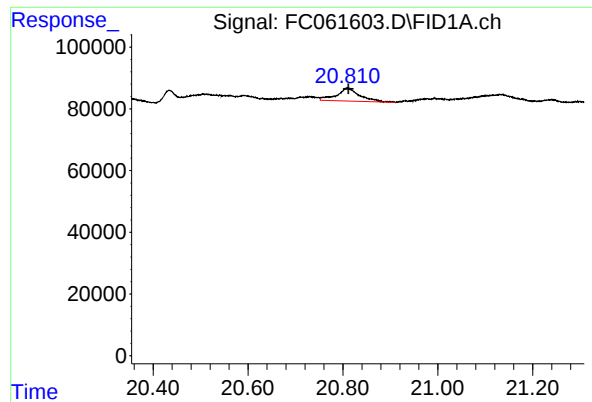

#21 n-Octatriacontane (C38)

R.T.: 20.810 min
Delta R.T.: -0.002 min
Response: 141506
Conc: 1.09 ug/ml

Instrument :

FID_C

ClientSampleId :