

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092320AL\
 Data File : FC049741.D
 Signal(s) : FID1A.CH
 Acq On : 24 Sep 2020 1:43
 Operator : DD\AJ
 Sample : L3864-14DL 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 24 02:50:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 090820.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 09 05:58:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.660	379376	3.302 ug/ml
Spiked Amount 50.000		Recovery =	6.60%
12) S 1-chlorooctadecane (S...	13.094	342023	3.840 ug/ml
Spiked Amount 50.000		Recovery =	7.68%
Target Compounds			
10) T n-Eicosane (C20)	12.719f	225049	2.102 ug/ml
14) T n-Tetracosane (C24)	14.941	113641	1.086 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092320AL\
Data File : FC049741.D
Signal(s) : FID1A.CH
Acq On : 24 Sep 2020 1:43
Operator : DD\AJ
Sample : L3864-14DL 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 24 02:50:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 090820.M
Quant Title : GC Extractables
QLast Update : Wed Sep 09 05:58:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

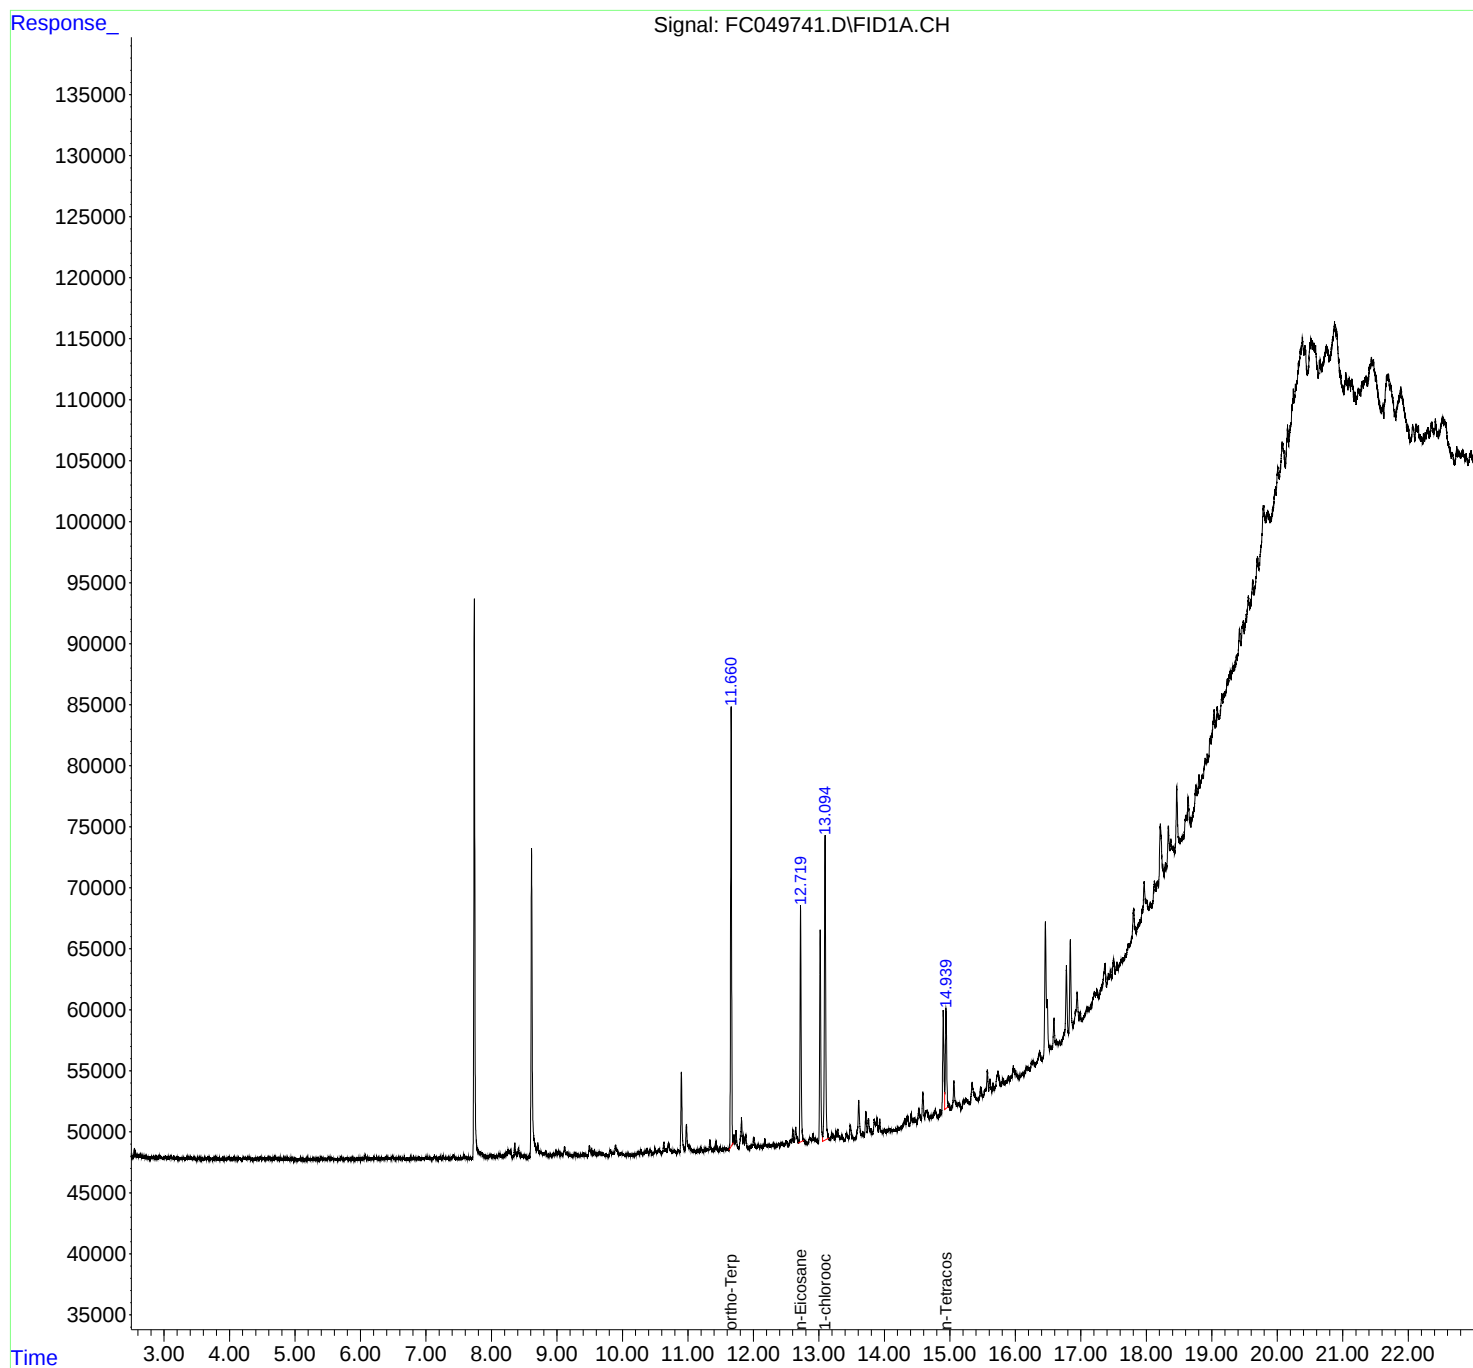


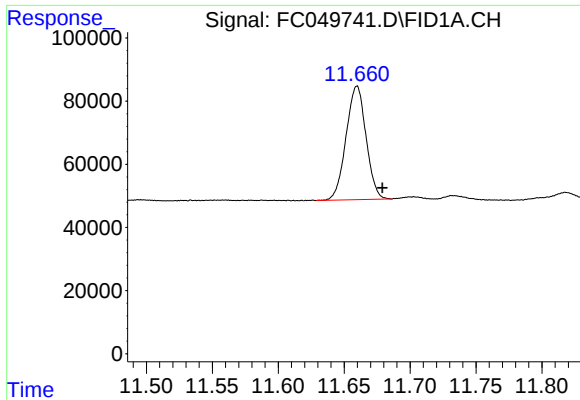

#9 ortho-Terphenyl (SURR)


R.T.: 11.660 min
Delta R.T.: -0.019 min
Response: 379376
Conc: 3.30 ug/ml

Instrument :
FID_C
ClientSampleId :

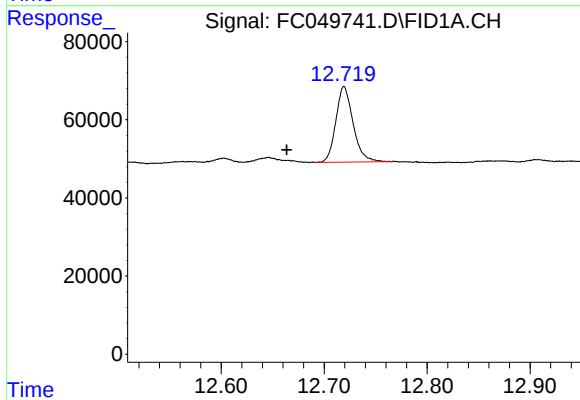


#10 n-Eicosane (C20)

R.T.: 12.719 min
Delta R.T.: 0.056 min
Response: 225049
Conc: 2.10 ug/ml

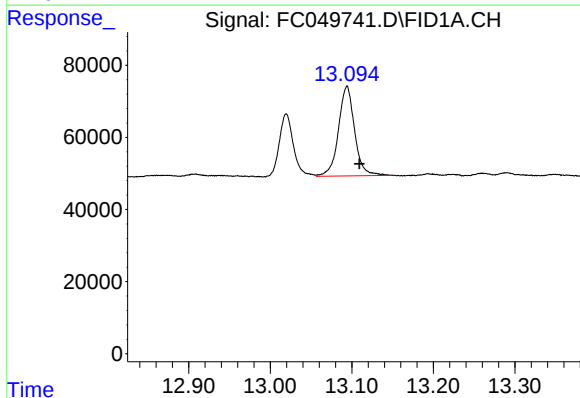

#12 1-chlorooctadecane (SURR)

R.T.: 13.094 min
Delta R.T.: -0.015 min
Response: 342023
Conc: 3.84 ug/ml

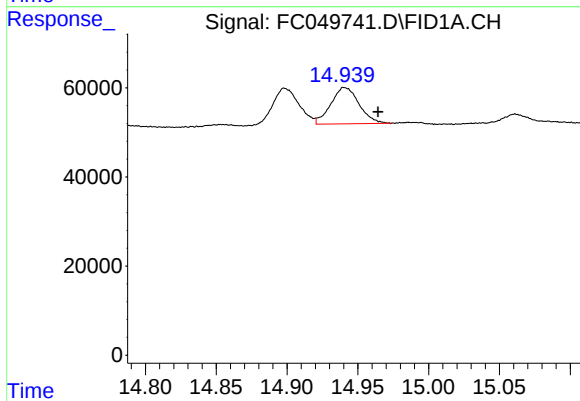

#14 n-Tetracosane (C24)

R.T.: 14.941 min
Delta R.T.: -0.024 min
Response: 113641
Conc: 1.09 ug/ml