

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092523AL\
Data File : FC064643.D
Signal(s) : FID1A.ch
Acq On : 25 Sep 2023 08:13
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 25 13:52:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.264	43538	0.306 ug/ml
20) T n-Hexatriacontane (C36)	20.032	111322	0.808 ug/ml
22) T n-Tetracontane (C40)	21.547	110596	0.813 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092523AL\
Data File : FC064643.D
Signal(s) : FID1A.ch
Acq On : 25 Sep 2023 08:13
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 25 13:52:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

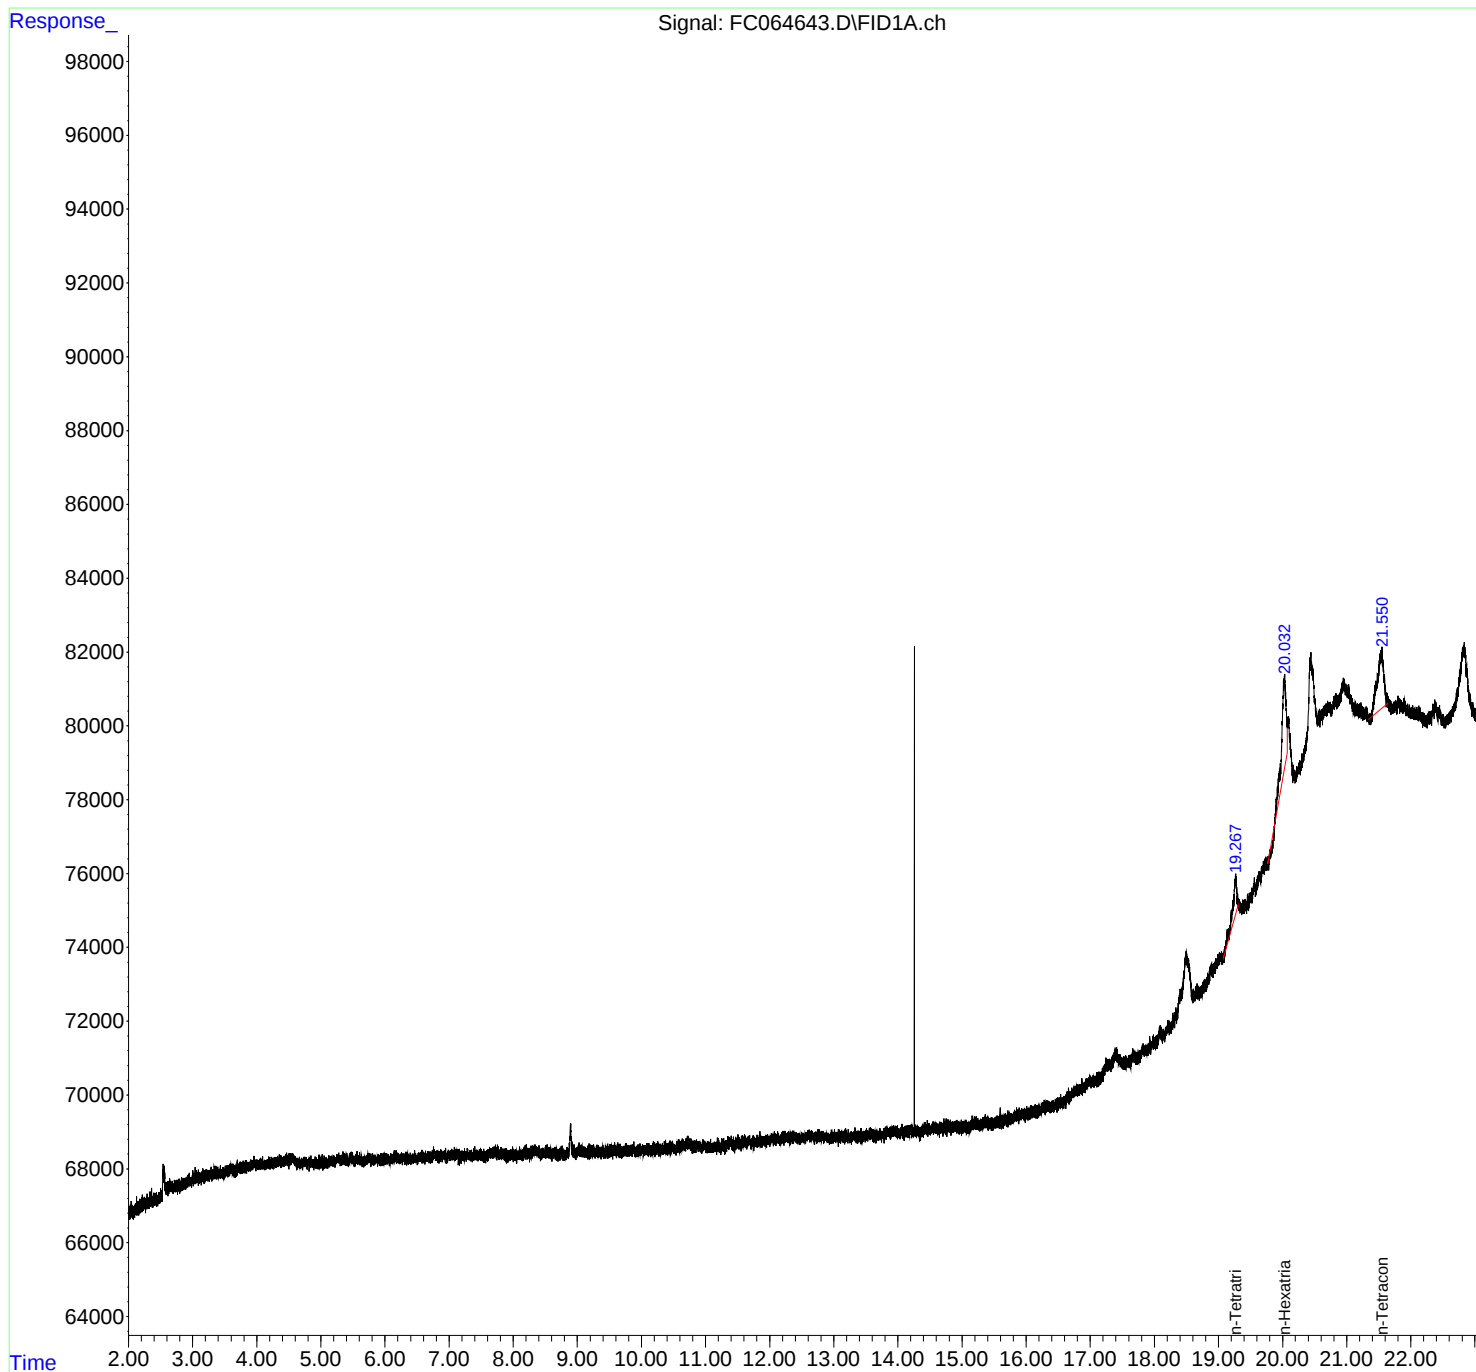


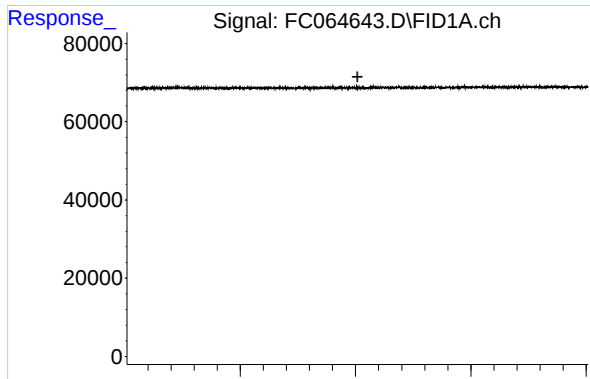

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

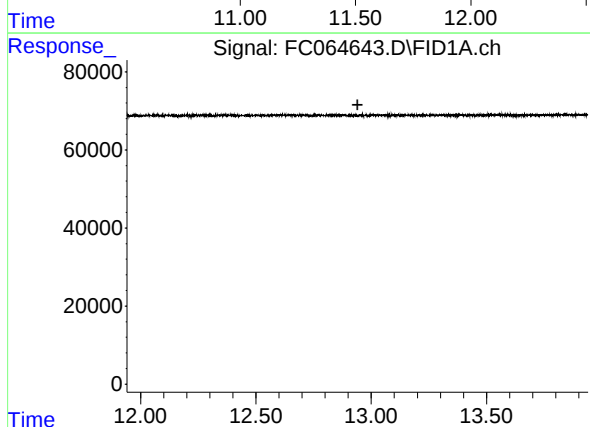


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.940 min
Response: 0
Conc: N.D.

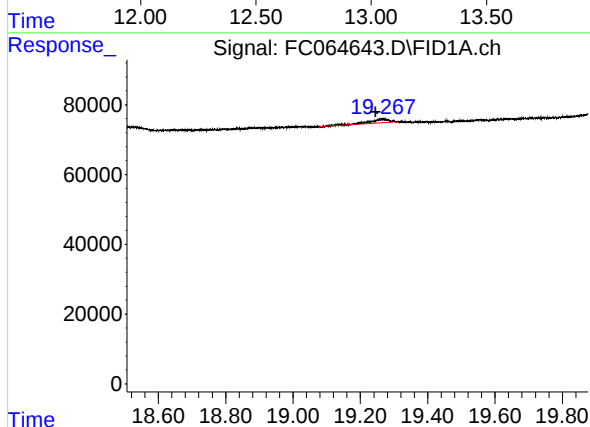


#19 n-Tetratriacontane (C34)

R.T.: 19.264 min
Delta R.T.: 0.018 min
Response: 43538
Conc: 0.31 ug/ml

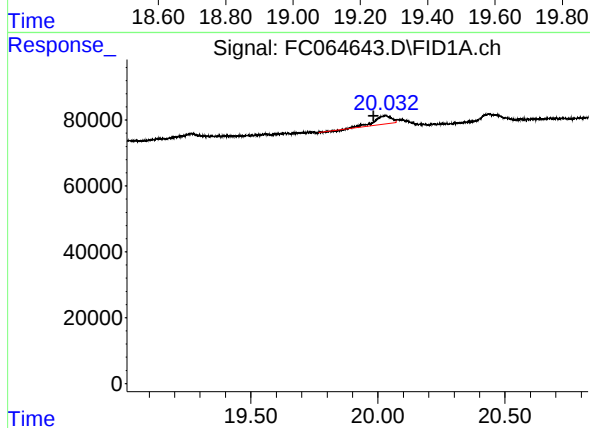

#20 n-Hexatriacontane (C36)

R.T.: 20.032 min
Delta R.T.: 0.048 min
Response: 111322
Conc: 0.81 ug/ml

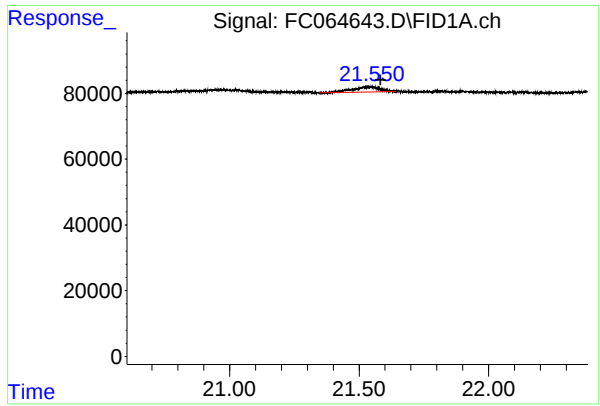

#22 n-Tetracontane (C40)

R.T.: 21.547 min
Delta R.T.: -0.036 min
Response: 110596
Conc: 0.81 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK