

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
Data File : FB028462.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2022 15:21
Operator : AJ/MA
Sample : N4723-10
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 28 03:33:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
6) t Toluene	10.697	1489	0.064 ng/ml
7) t Ethylbenzene	13.079	5027	0.226 ng/ml
8) t m-Xylene	13.210	21657	0.992 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	3308	0.165 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB092722\
Data File : FB028462.D
Signal(s) : FID2B.CH
Acq On : 27 Sep 2022 15:21
Operator : AJ/MA
Sample : N4723-10
Misc : 5.07G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: Calibration.e
Quant Time: Sep 28 03:33:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB090822.M
Quant Title :
QLast Update : Thu Sep 08 15:28:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

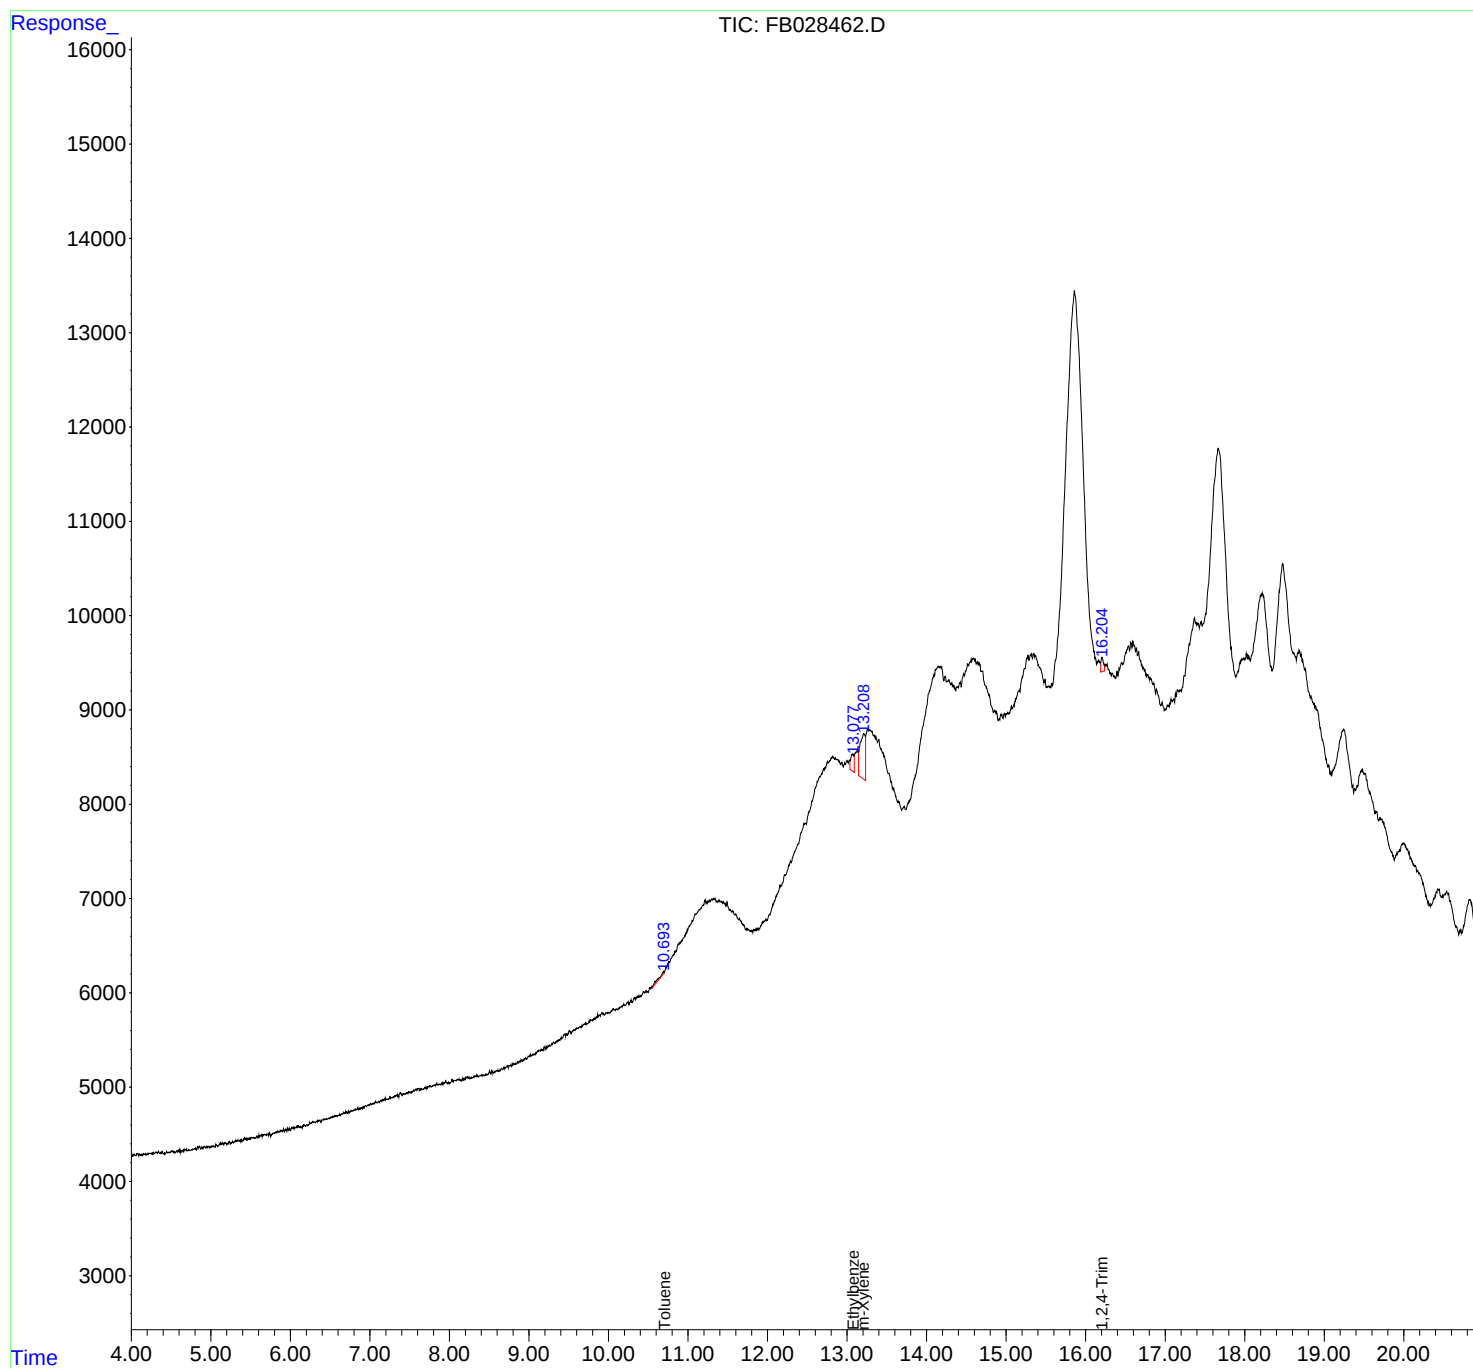


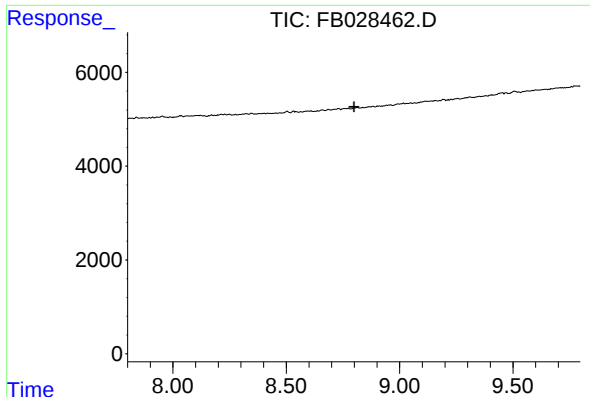

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.800 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

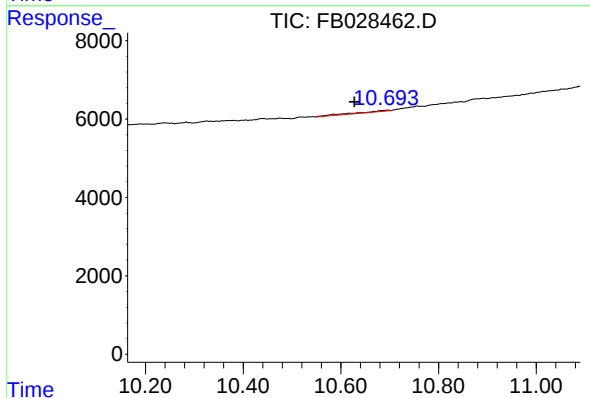


#6 Toluene

R.T.: 10.697 min
Delta R.T.: 0.069 min
Response: 1489
Conc: 0.06 ng/ml

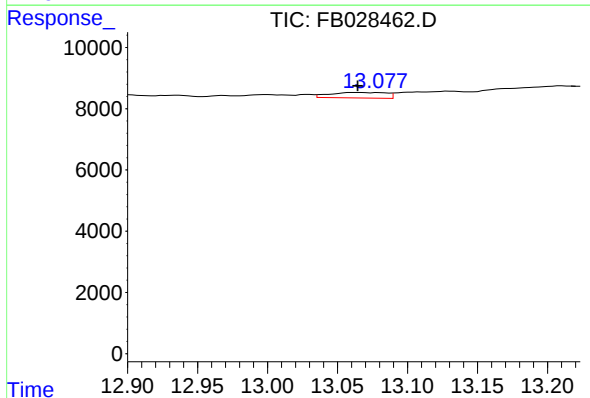


#7 Ethylbenzene

R.T.: 13.079 min
Delta R.T.: 0.015 min
Response: 5027
Conc: 0.23 ng/ml

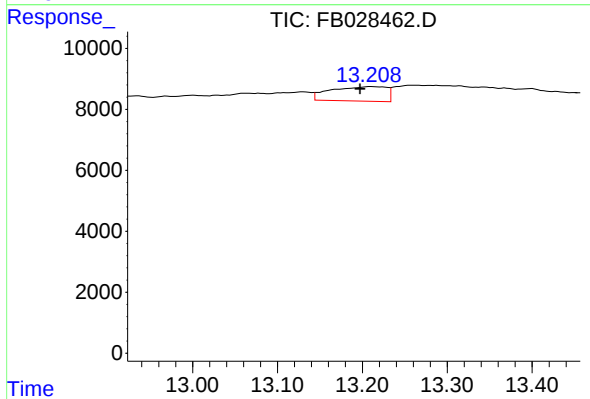

#8 m-Xylene

R.T.: 13.210 min
Delta R.T.: 0.013 min
Response: 21657
Conc: 0.99 ng/ml

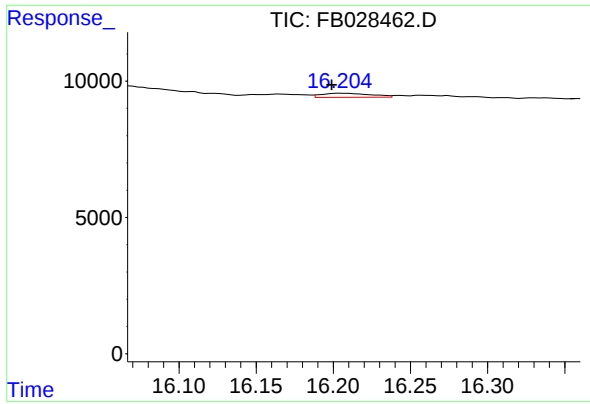

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.007 min
Response: 3308
Conc: 0.16 ng/ml

Instrument :
FID_C
ClientSampleId :