

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092722AL\
Data File : FC061643.D
Signal(s) : FID1A.ch
Acq On : 28 Sep 2022 04:03
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 28 05:19:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092022.M
Quant Title : GC Extractables
QLast Update : Tue Sep 20 18:33:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.730	93618	0.608 ug/ml
18) T	n-Dotriacontane (C32)	18.566	429553	2.841 ug/ml
22) T	n-Tetracontane (C40)	21.765	247374	2.024 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092722AL\
Data File : FC061643.D
Signal(s) : FID1A.ch
Acq On : 28 Sep 2022 04:03
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 28 05:19:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 092022.M
Quant Title : GC Extractables
QLast Update : Tue Sep 20 18:33:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

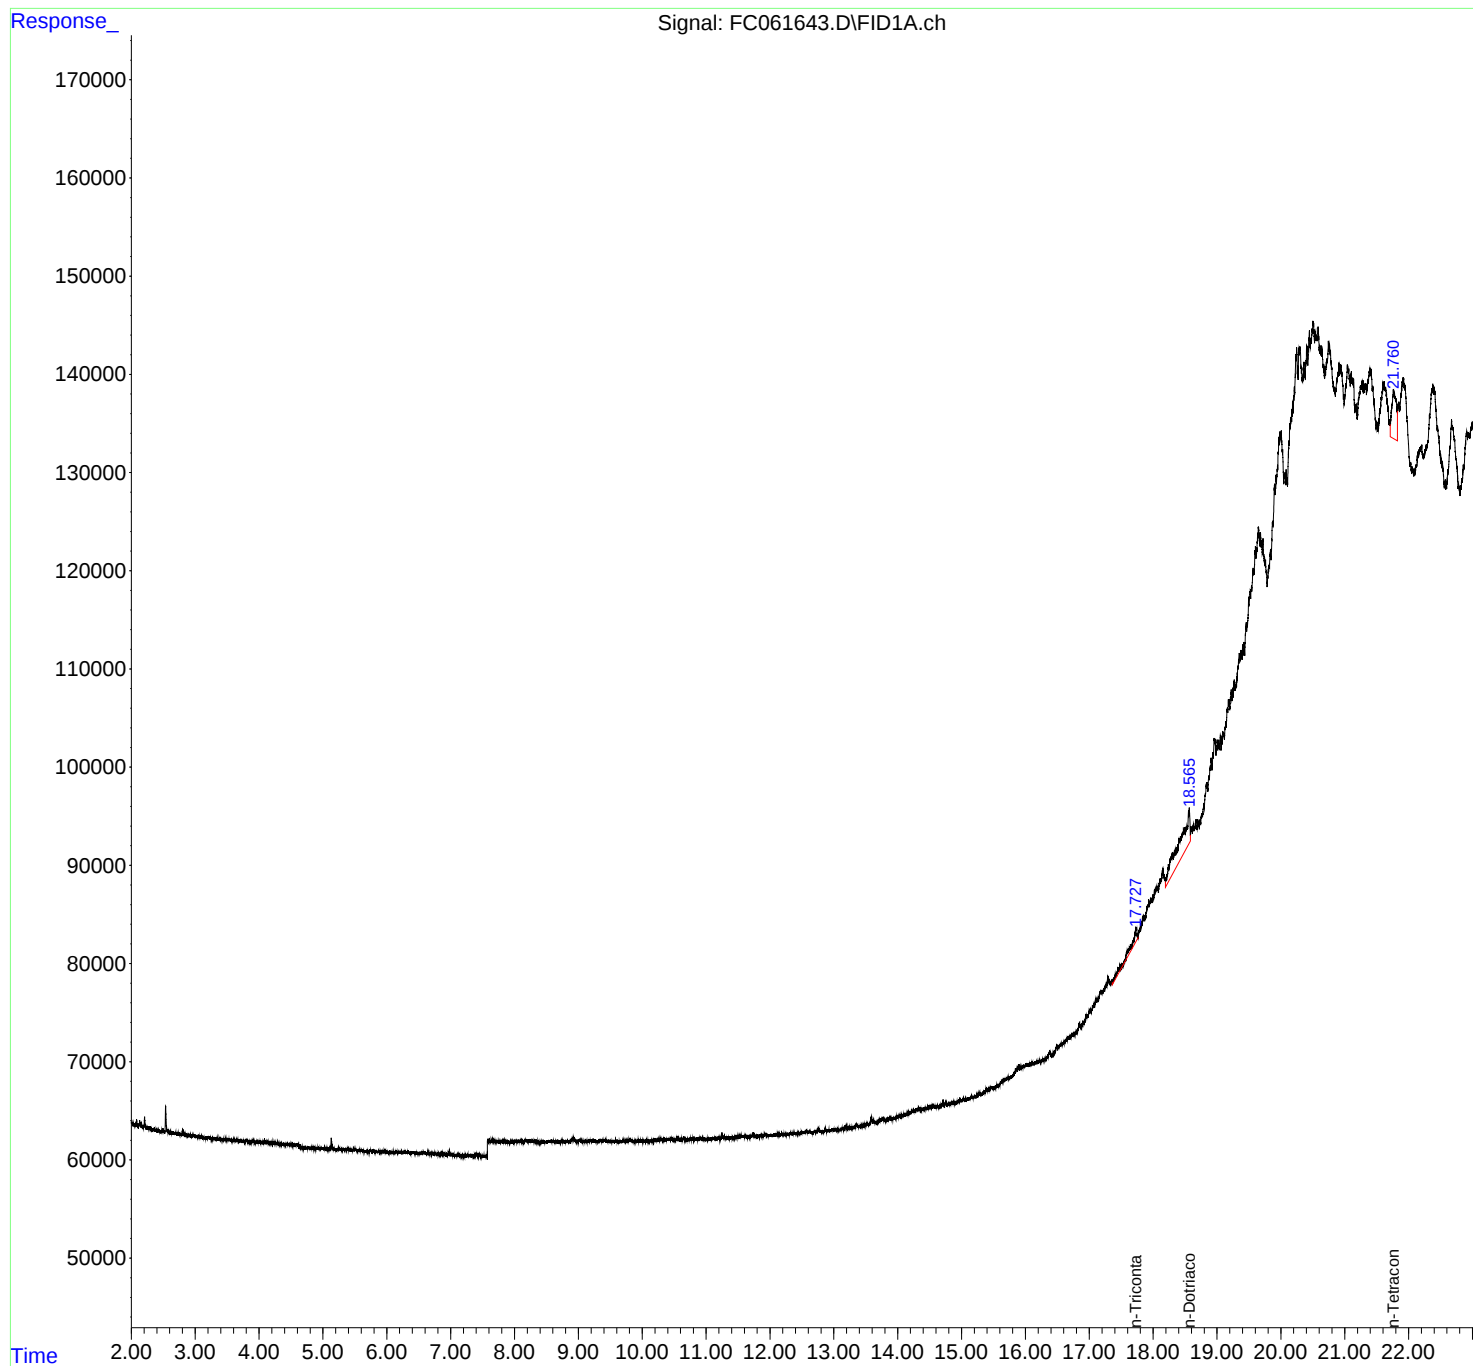


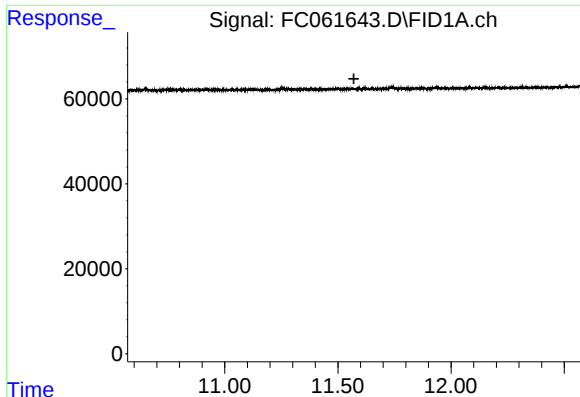

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.571 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

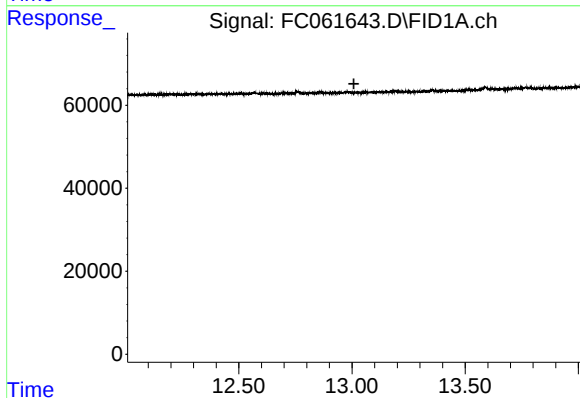


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.008 min
Response: 0
Conc: N.D.

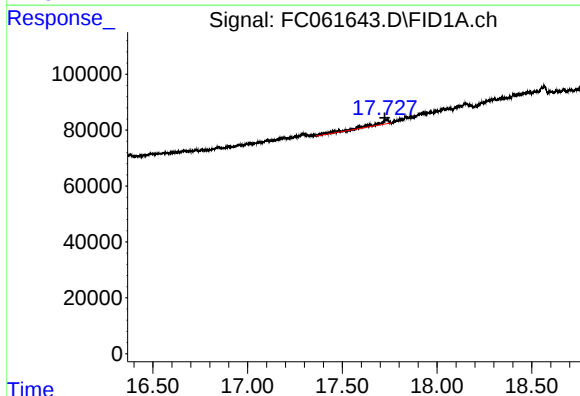


#17 n-Tricontane (C30)

R.T.: 17.730 min
Delta R.T.: 0.006 min
Response: 93618
Conc: 0.61 ug/ml

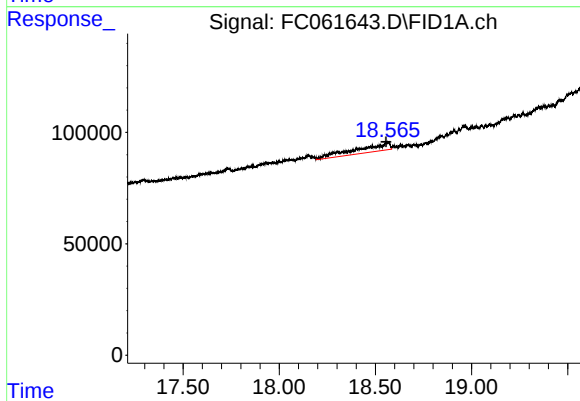

#18 n-Dotriacontane (C32)

R.T.: 18.566 min
Delta R.T.: 0.010 min
Response: 429553
Conc: 2.84 ug/ml

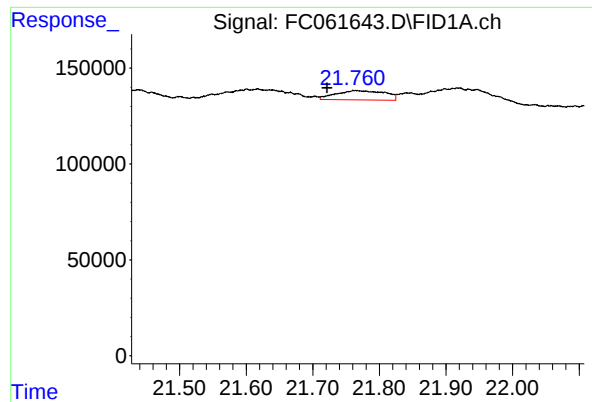

#22 n-Tetracontane (C40)

R.T.: 21.765 min
Delta R.T.: 0.043 min
Response: 247374
Conc: 2.02 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK