

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092822AL\
Data File : FE037818.D
Signal(s) : FID1B.ch
Acq On : 28 Sep 2022 03:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 28 06:24:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 092822.M
Quant Title : GC Extractables
QLast Update : Wed Sep 28 06:23:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.558	86043	0.546 ug/ml
20) T	n-Hexatriacontane (C36)	20.099	164023	1.138 ug/ml
22) T	n-Tetracontane (C40)	21.551	120934	0.950 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE092822AL\
Data File : FE037818.D
Signal(s) : FID1B.ch
Acq On : 28 Sep 2022 03:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 28 06:24:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 092822.M
Quant Title : GC Extractables
QLast Update : Wed Sep 28 06:23:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

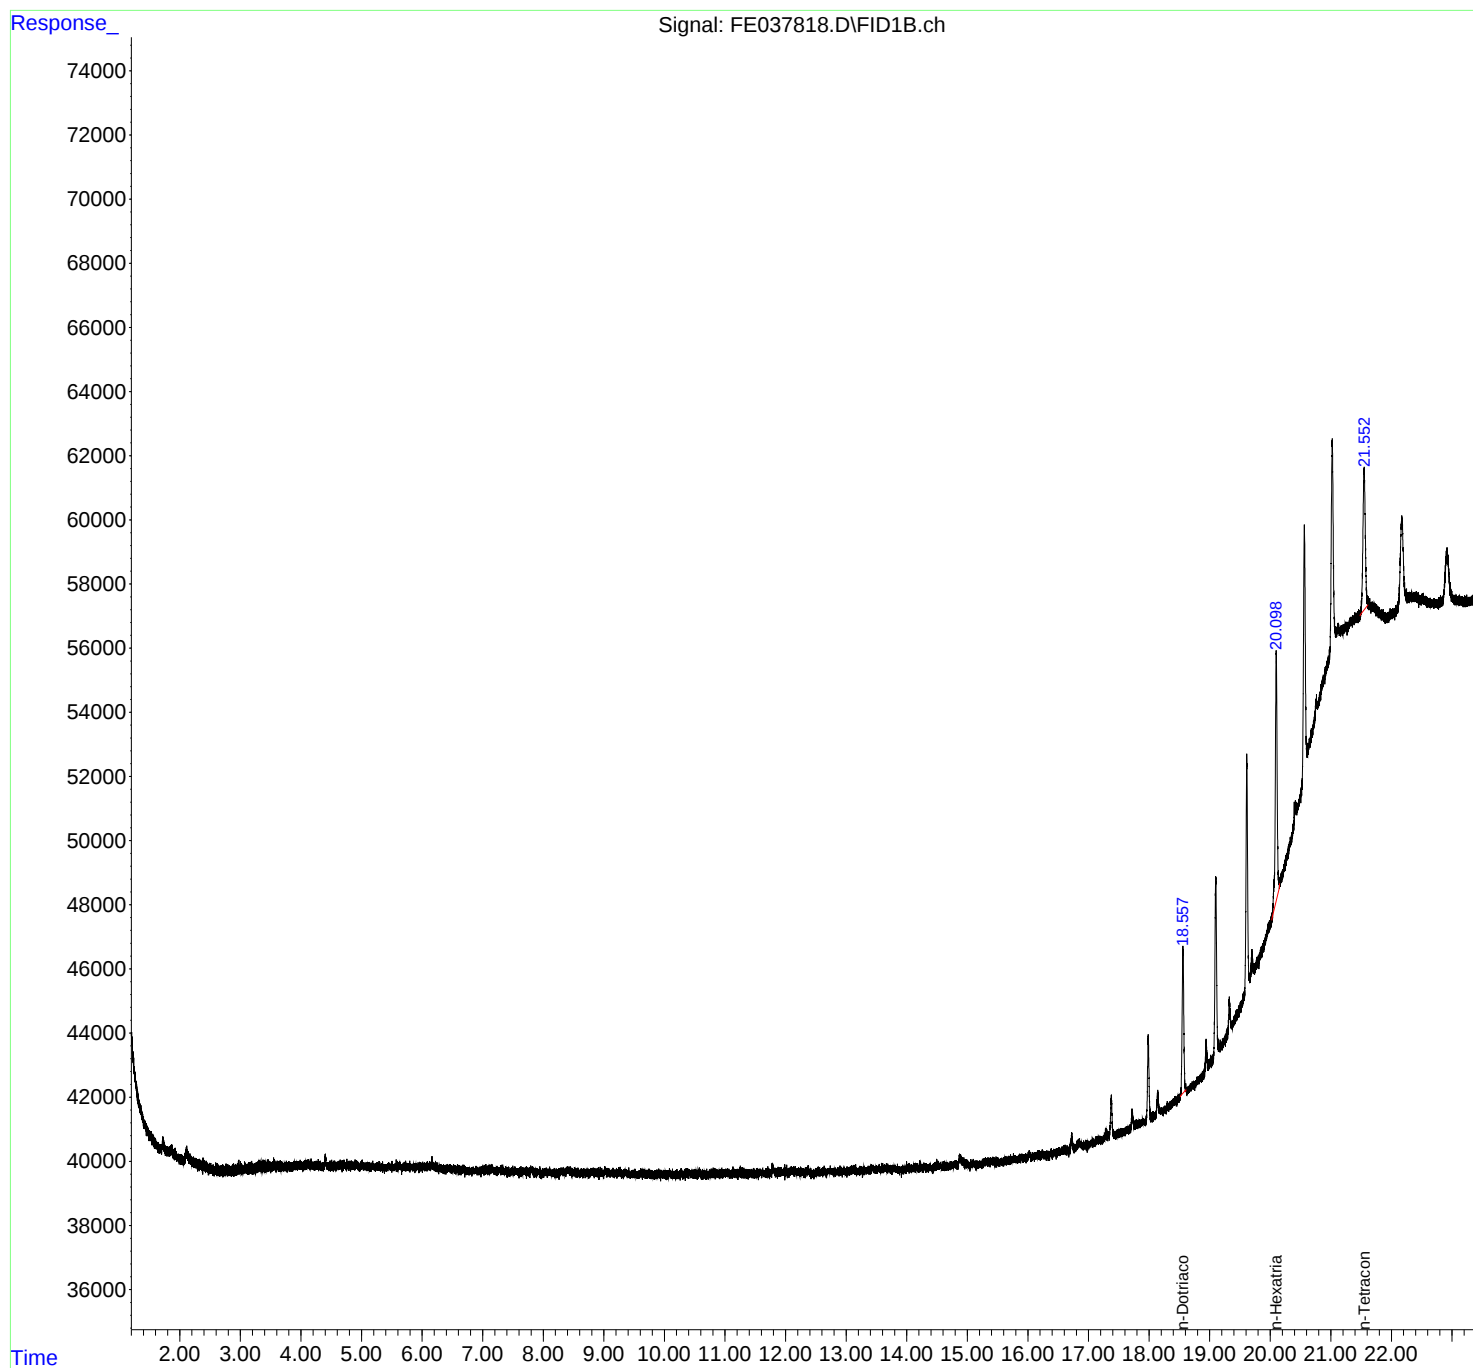


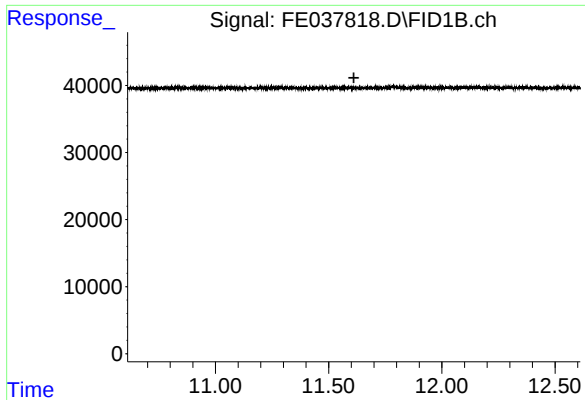

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.612 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
I.BLK

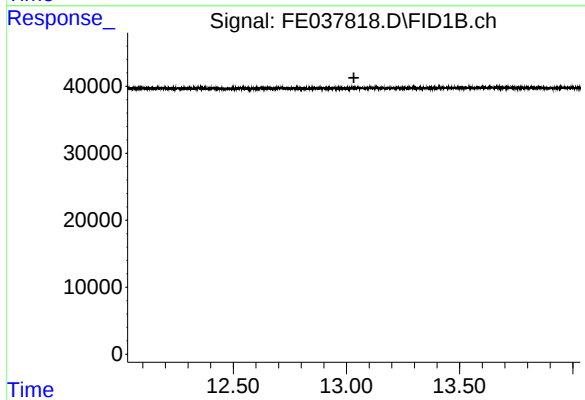


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.033 min
Response: 0
Conc: N.D.

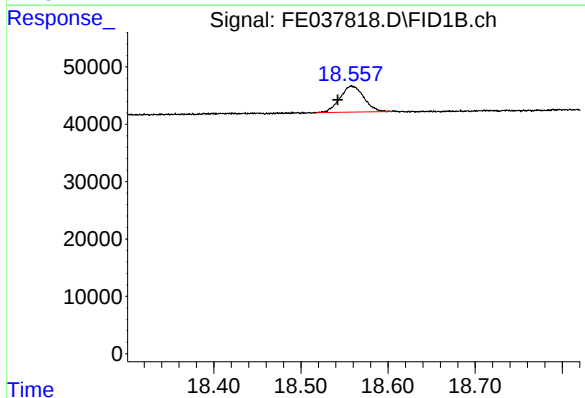


#18 n-Dotriacontane (C32)

R.T.: 18.558 min
Delta R.T.: 0.016 min
Response: 86043
Conc: 0.55 ug/ml

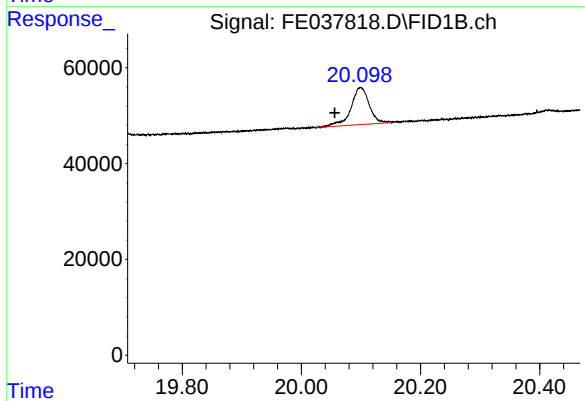

#20 n-Hexatriacontane (C36)

R.T.: 20.099 min
Delta R.T.: 0.043 min
Response: 164023
Conc: 1.14 ug/ml

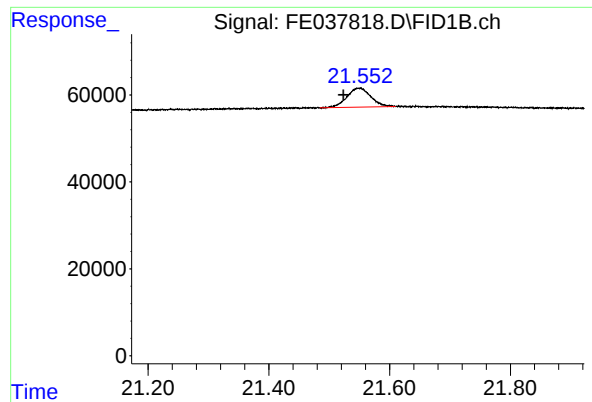

#22 n-Tetracontane (C40)

R.T.: 21.551 min
Delta R.T.: 0.028 min
Response: 120934
Conc: 0.95 ug/ml

Instrument :
FID_C
ClientSampleId :
I.BLK