

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092724AL\
 Data File : FC067292.D
 Signal(s) : FID1A.ch
 Acq On : 27 Sep 2024 05:53
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 28 01:56:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091024.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 11 02:55:44 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.482	71108	0.682 ug/ml
19) T	n-Tetratriacontane (C34)	19.263	71461	0.775 ug/ml
20) T	n-Hexatriacontane (C36)	20.003	88518	1.117 ug/ml
21) T	n-Octatriacontane (C38)	20.726	132716	1.767 ug/ml
22) T	n-Tetracontane (C40)	21.612	207186	2.966 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC092724AL\
Data File : FC067292.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2024 05:53
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 28 01:56:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091024.M
Quant Title : GC Extractables
QLast Update : Wed Sep 11 02:55:44 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

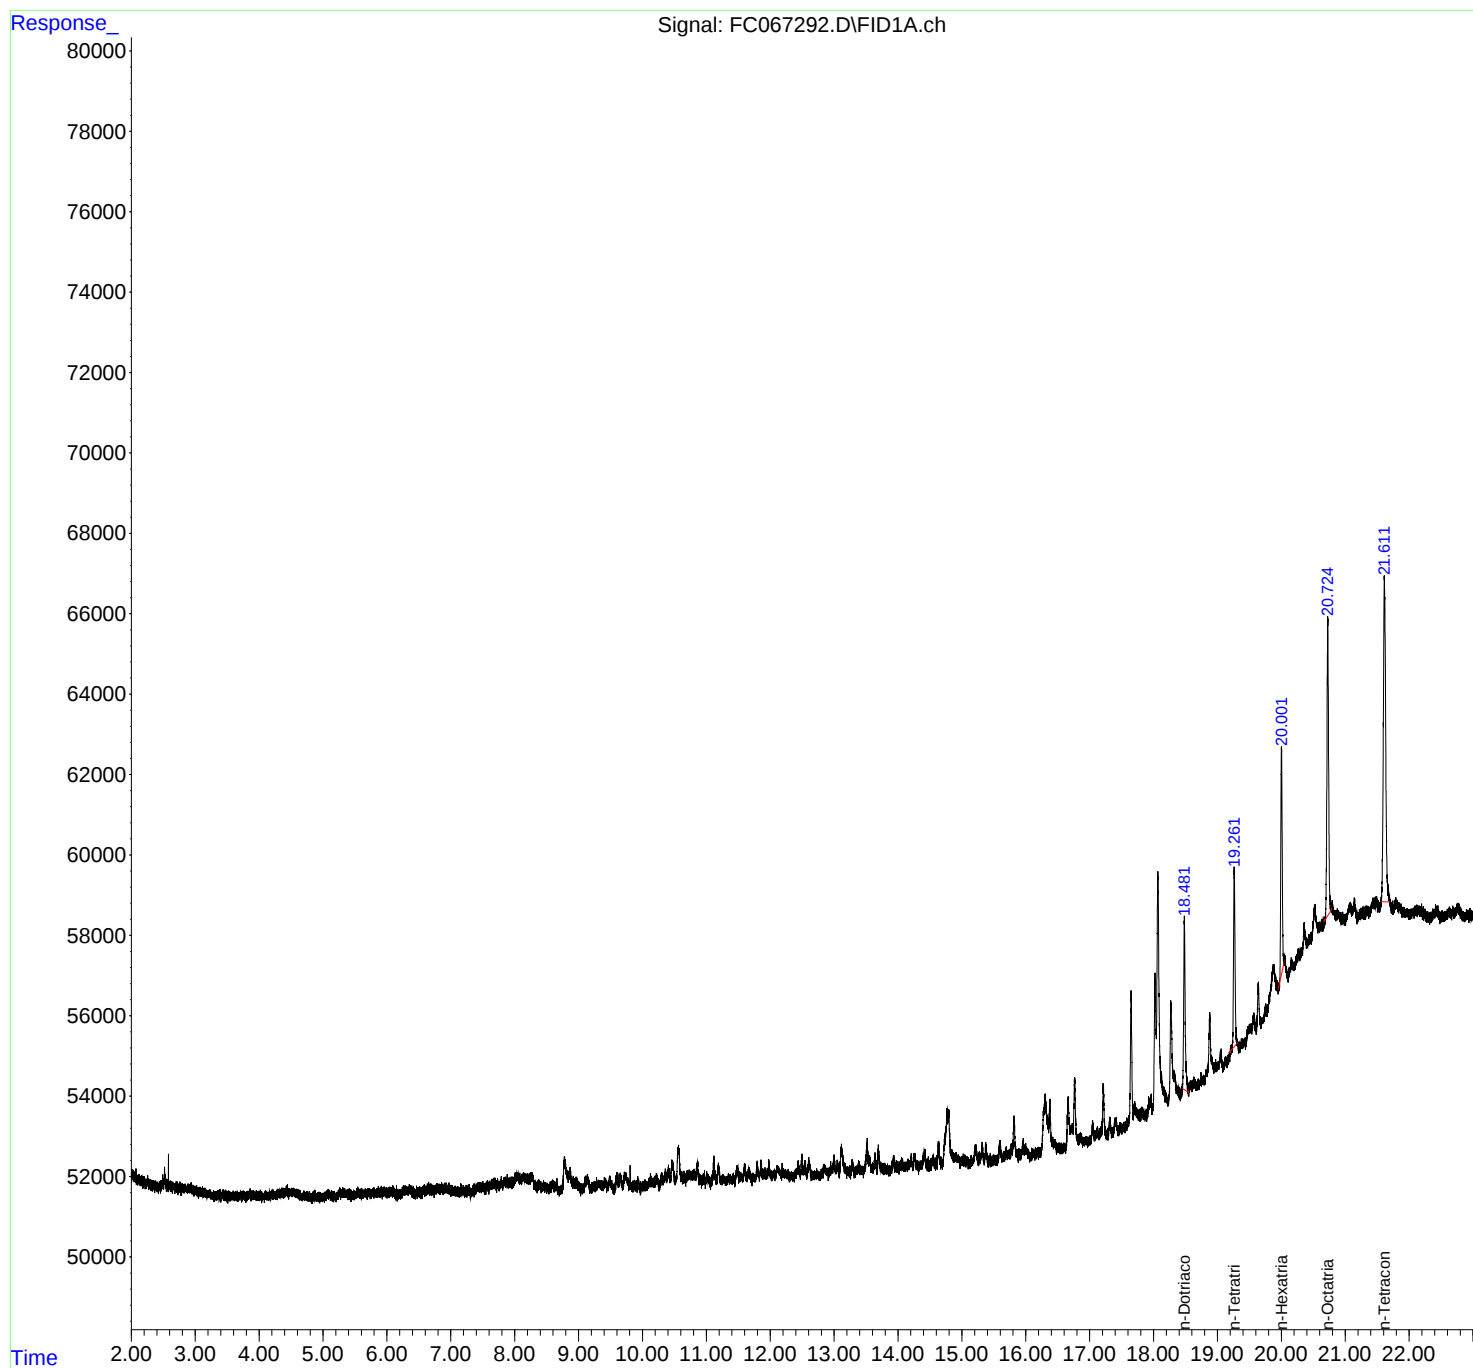


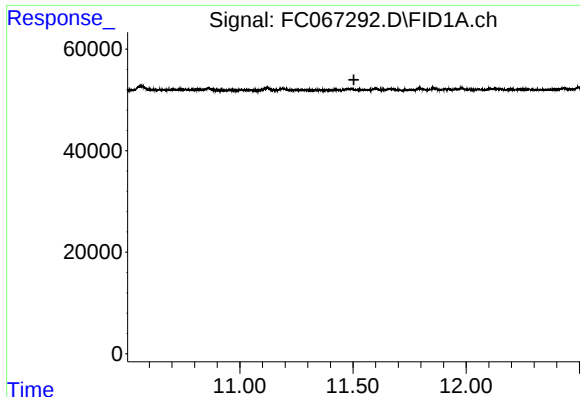

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.504 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

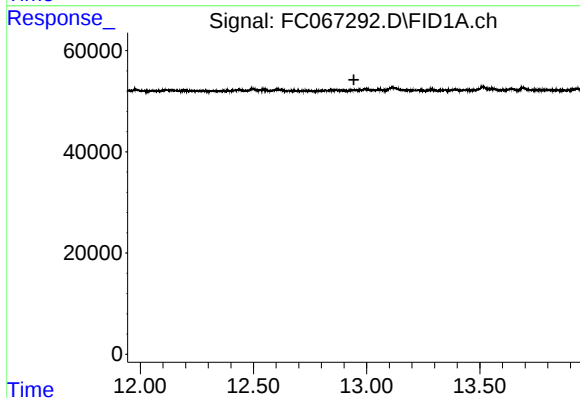


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.943 min
Response: 0
Conc: N.D.

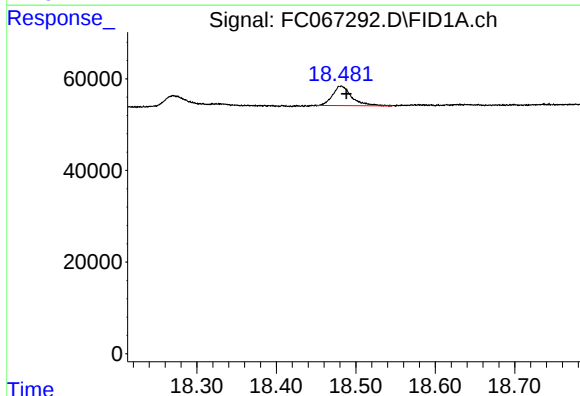


#18 n-Dotriacontane (C32)

R.T.: 18.482 min
Delta R.T.: -0.007 min
Response: 71108
Conc: 0.68 ug/ml

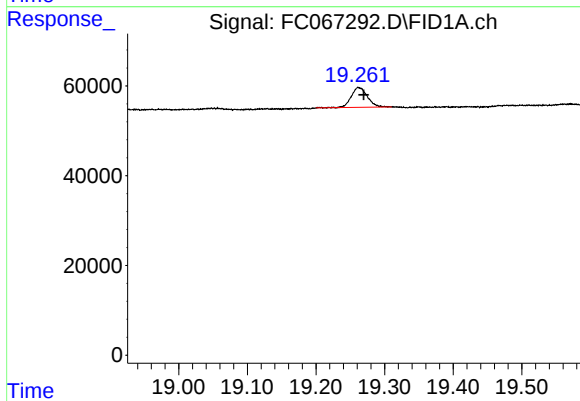

#19 n-Tetratriacontane (C34)


R.T.: 19.263 min
Delta R.T.: -0.007 min
Response: 71461
Conc: 0.77 ug/ml

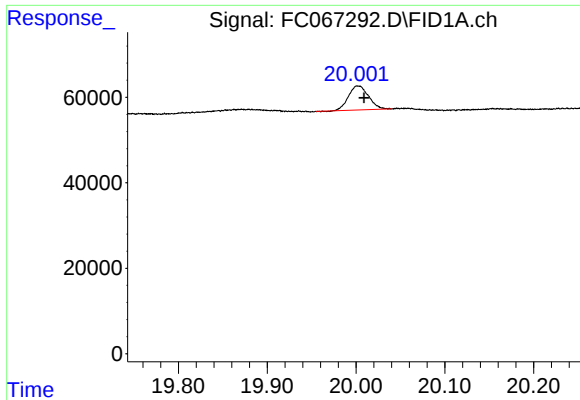

#20 n-Hexatriacontane (C36)


R.T.: 20.003 min
Delta R.T.: -0.006 min
Response: 88518
Conc: 1.12 ug/ml

Instrument :
FID_C
ClientSampleId :

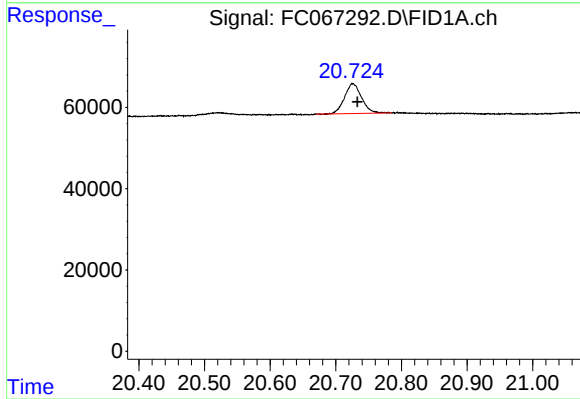

#21 n-Octatriacontane (C38)

R.T.: 20.726 min
Delta R.T.: -0.007 min
Response: 132716
Conc: 1.77 ug/ml

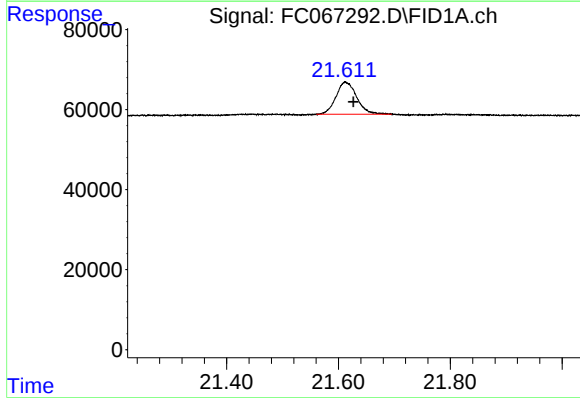

#22 n-Tetracontane (C40)

R.T.: 21.612 min
Delta R.T.: -0.014 min
Response: 207186
Conc: 2.97 ug/ml