

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100423AL\
 Data File : FC064718.D
 Signal(s) : FID1A.ch
 Acq On : 04 Oct 2023 09:01
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 05 00:13:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:25:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.006f	39003	0.268 ug/ml
Spiked Amount 50.000		Recovery =	0.54%
Target Compounds			
11) T n-Heneicosane (C21)	13.119	31584	0.191 ug/ml
14) T n-Tetracosane (C24)	14.798	111262	0.701 ug/ml
15) T n-Hexacosane (C26)	15.818	44435	0.291 ug/ml
16) T n-Octacosane (C28)	16.761	30451	0.206 ug/ml
17) T n-Tricontane (C30)	17.647	40806	0.275 ug/ml
18) T n-Dotriacontane (C32)	18.477	107639	0.738 ug/ml
19) T n-Tetratriacontane (C34)	19.255	60035	0.422 ug/ml
20) T n-Hexatriacontane (C36)	19.991	55642	0.404 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100423AL\
Data File : FC064718.D
Signal(s) : FID1A.ch
Acq On : 04 Oct 2023 09:01
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 00:13:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

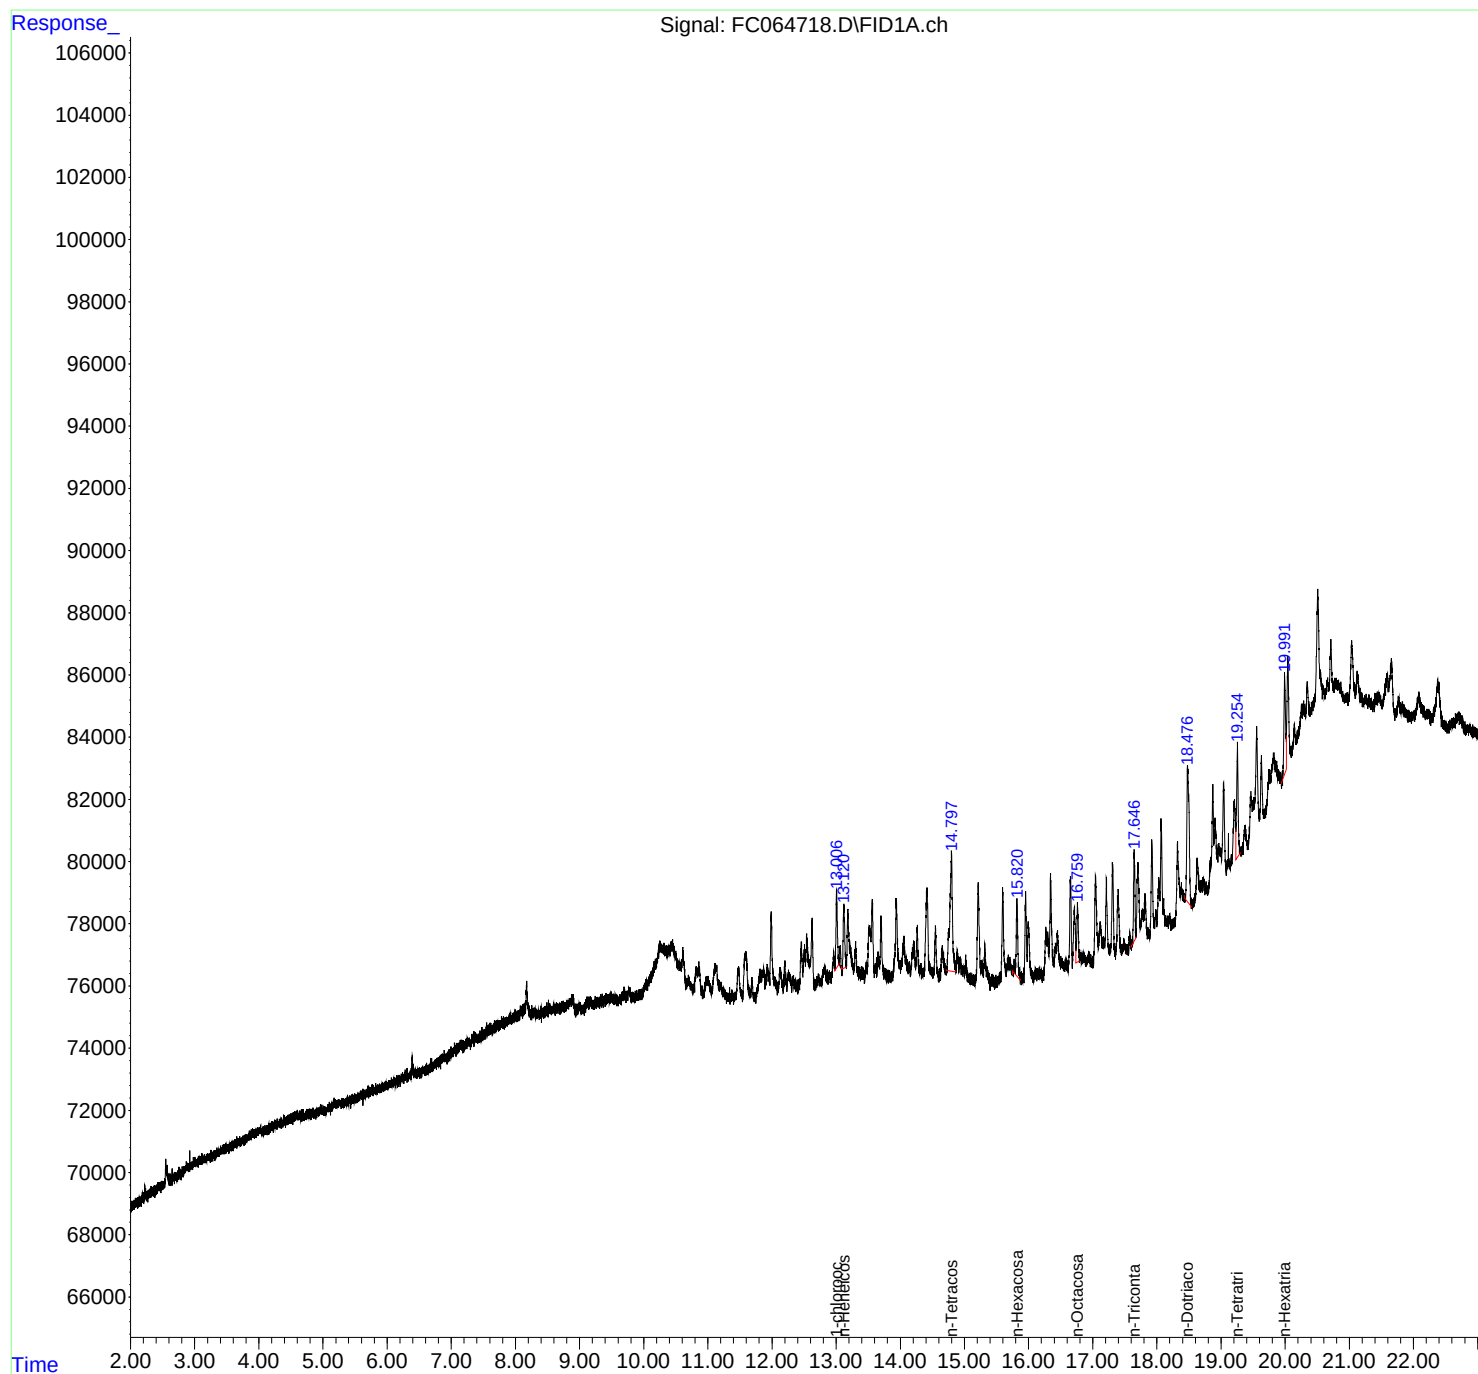


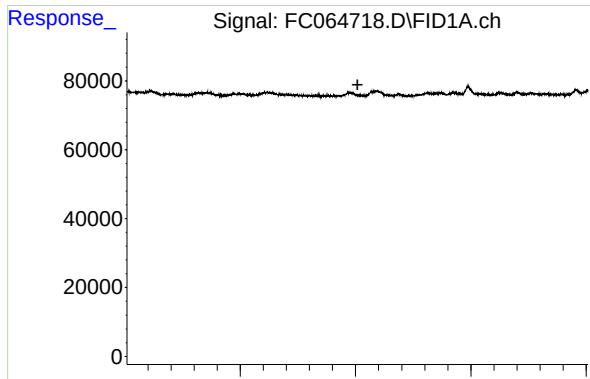

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

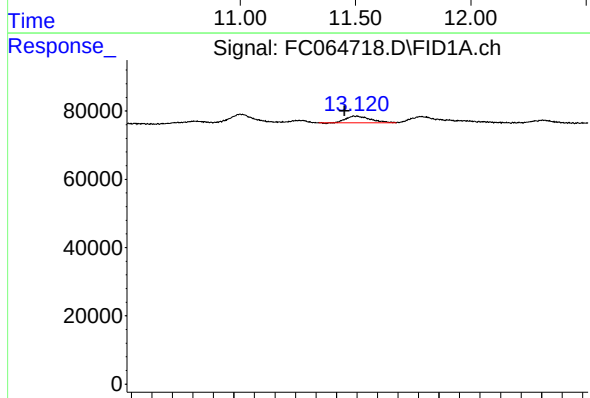


#11 n-Heneicosane (C21)

R.T.: 13.119 min
Delta R.T.: 0.011 min
Response: 31584
Conc: 0.19 ug/ml

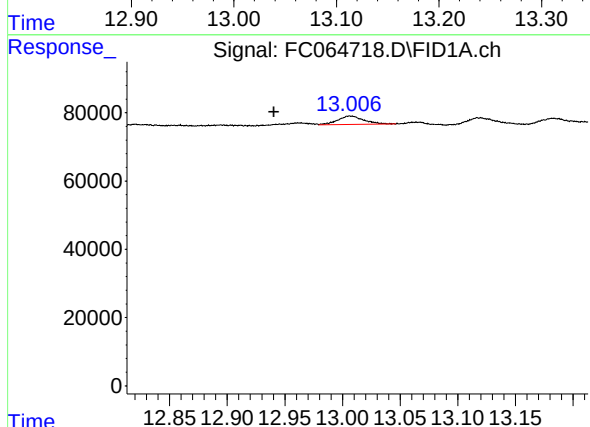


#12 1-chlorooctadecane (SURR)

R.T.: 13.006 min
Delta R.T.: 0.066 min
Response: 39003
Conc: 0.27 ug/ml

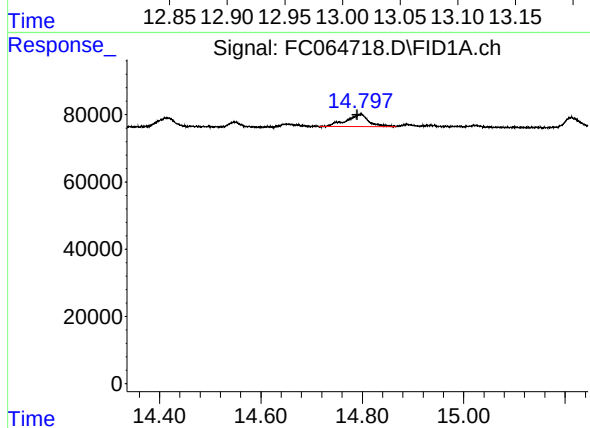

#14 n-Tetracosane (C24)

R.T.: 14.798 min
Delta R.T.: 0.008 min
Response: 111262
Conc: 0.70 ug/ml

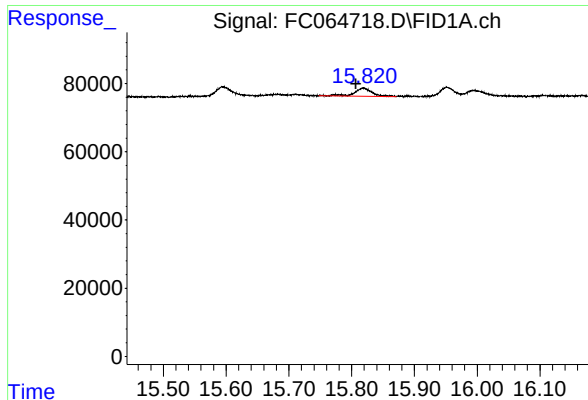


#15 n-Hexacosane (C26)

R.T.: 15.818 min
Delta R.T.: 0.011 min
Response: 44435
Conc: 0.29 ug/ml

Instrument :


FID_C

ClientSampleId :

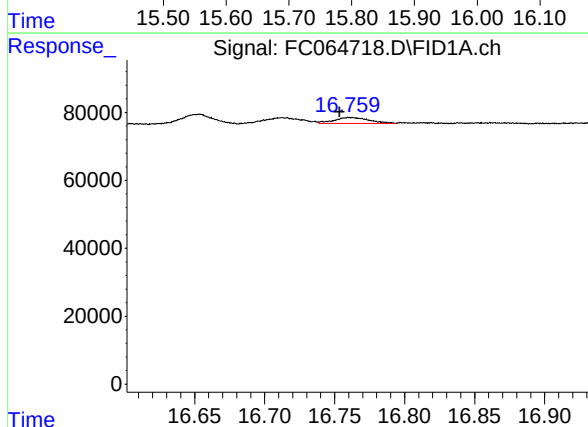


#16 n-Octacosane (C28)

R.T.: 16.761 min
Delta R.T.: 0.007 min
Response: 30451
Conc: 0.21 ug/ml

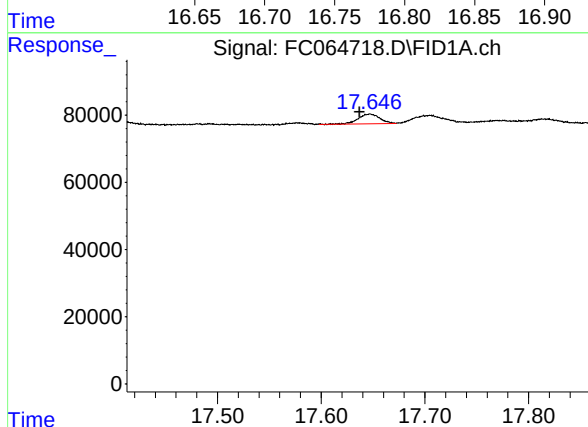


#17 n-Tricontane (C30)

R.T.: 17.647 min
Delta R.T.: 0.010 min
Response: 40806
Conc: 0.27 ug/ml

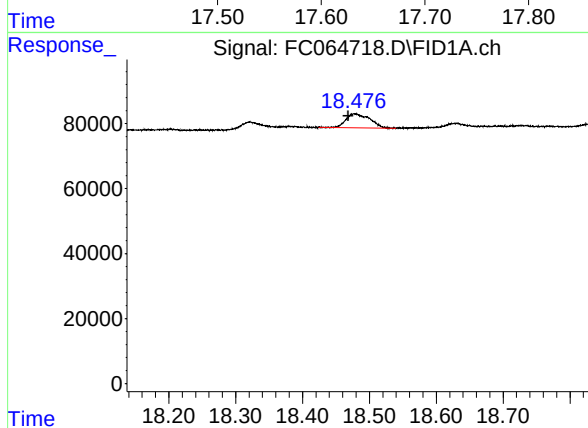

#18 n-Dotriacontane (C32)


R.T.: 18.477 min
Delta R.T.: 0.009 min
Response: 107639
Conc: 0.74 ug/ml

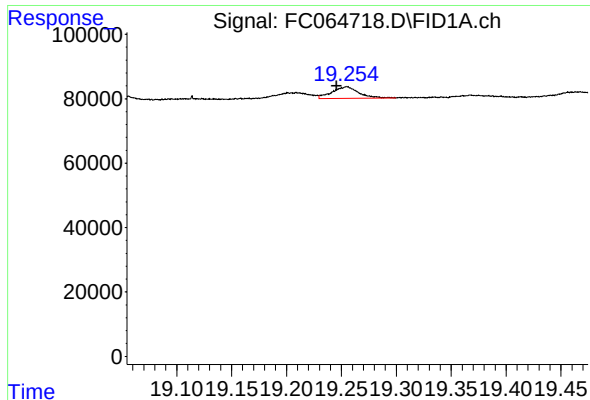

#19 n-Tetratriacontane (C34)

R.T.: 19.255 min
Delta R.T.: 0.009 min
Response: 60035
Conc: 0.42 ug/ml

Instrument :
FID_C
ClientSampleId :

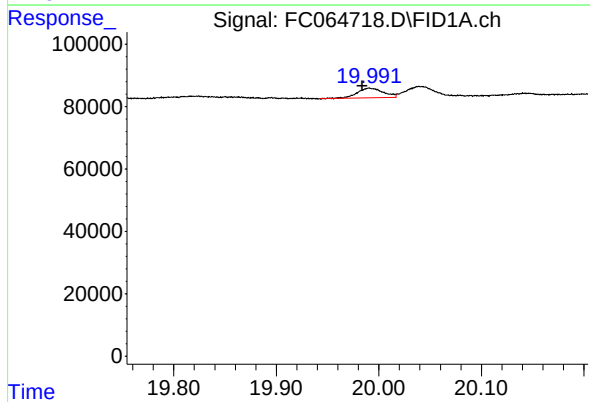

#20 n-Hexatriacontane (C36)

R.T.: 19.991 min
Delta R.T.: 0.007 min
Response: 55642
Conc: 0.40 ug/ml