

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100423AL\
 Data File : FC064733.D
 Signal(s) : FID1A.ch
 Acq On : 05 Oct 2023 01:51
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 05 02:54:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:25:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.653	49118	0.331 ug/ml
18) T	n-Dotriacontane (C32)	18.486	67352	0.462 ug/ml
19) T	n-Tetratriacontane (C34)	19.260	49240	0.346 ug/ml
20) T	n-Hexatriacontane (C36)	19.998	17938	0.130 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100423AL\
Data File : FC064733.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2023 01:51
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 05 02:54:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

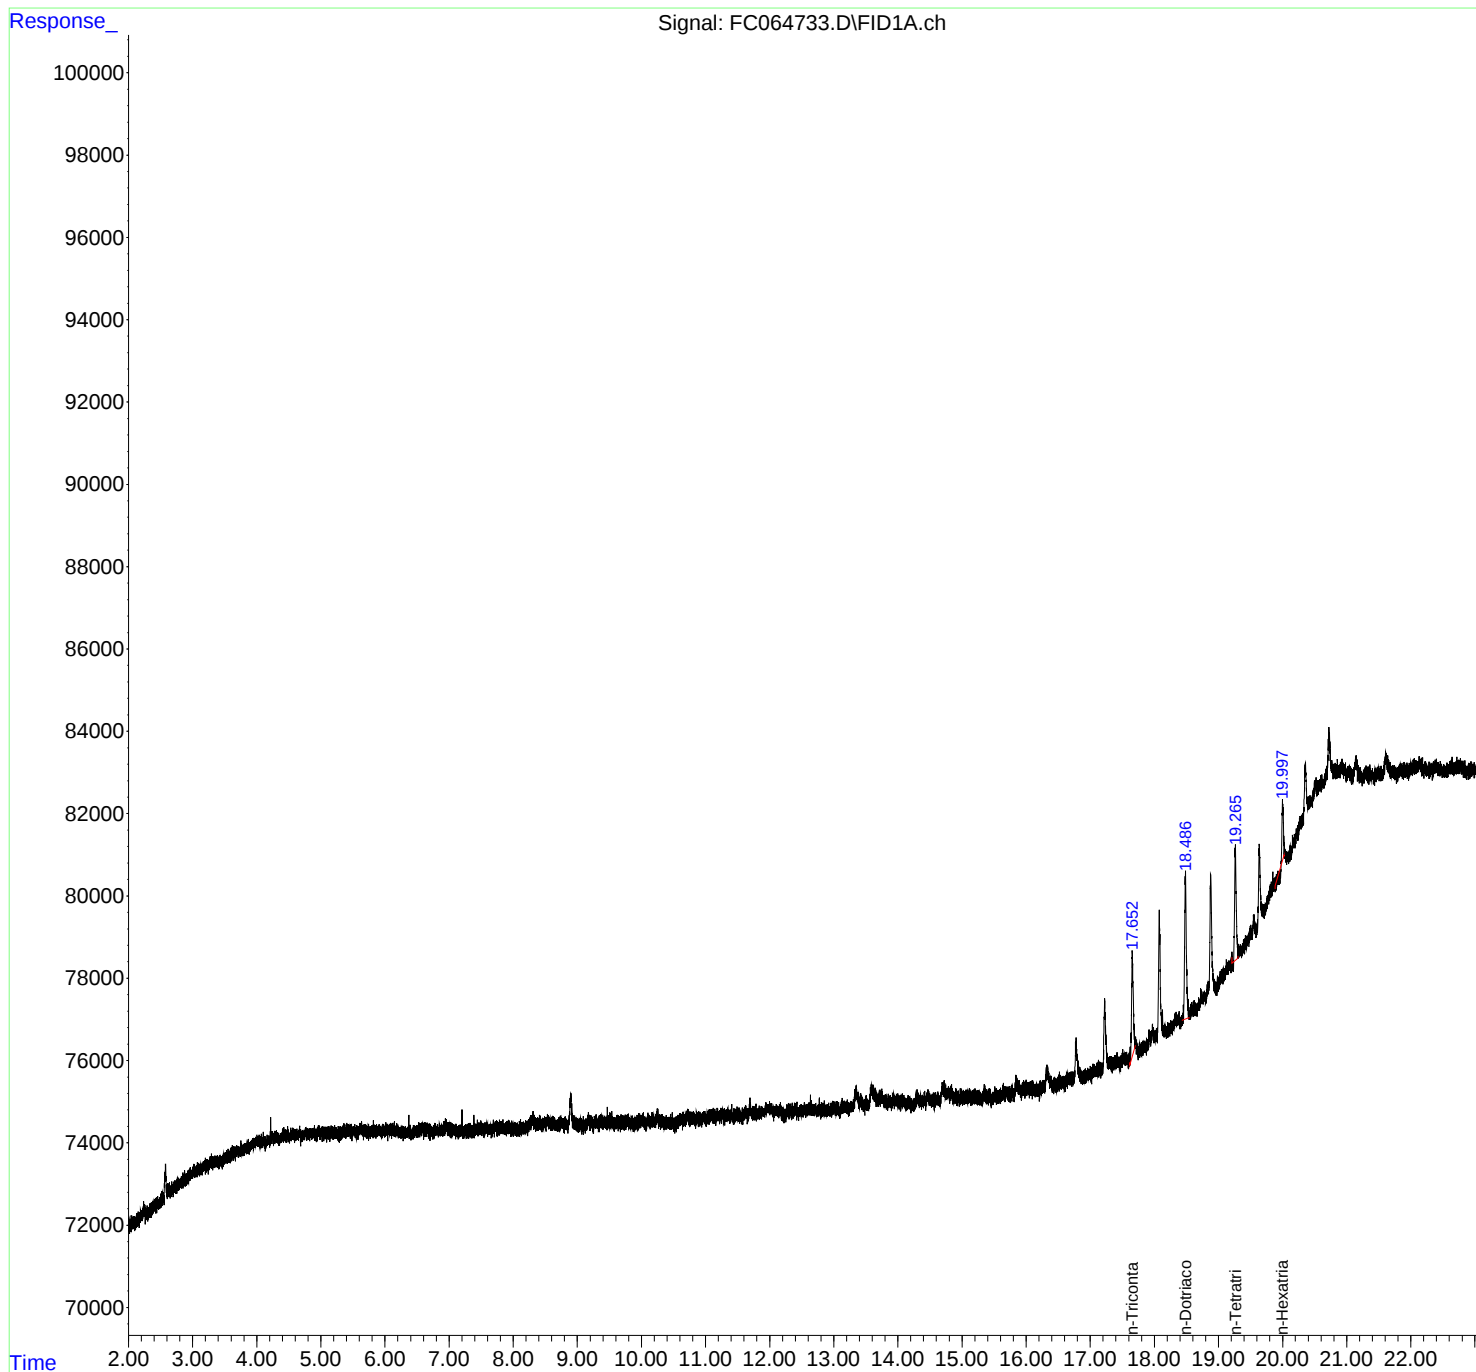


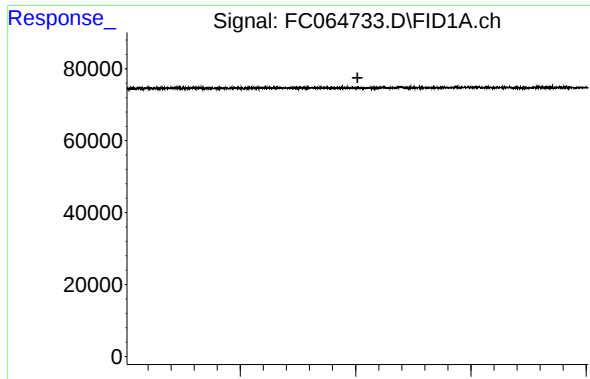

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

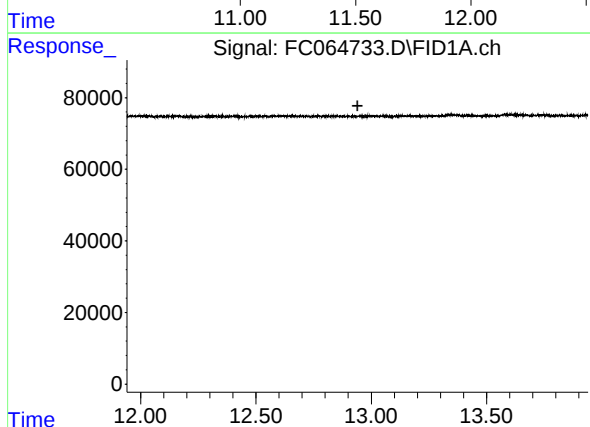


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.940 min
Response: 0
Conc: N.D.

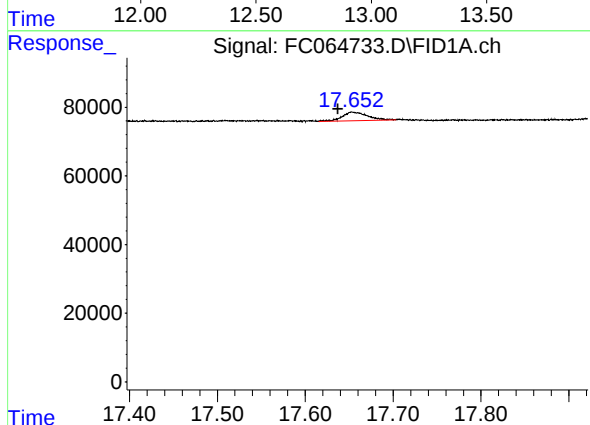


#17 n-Tricontane (C30)

R.T.: 17.653 min
Delta R.T.: 0.016 min
Response: 49118
Conc: 0.33 ug/ml

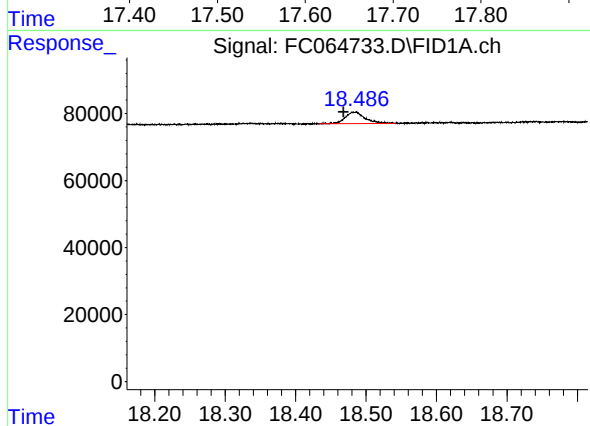

#18 n-Dotriacontane (C32)

R.T.: 18.486 min
Delta R.T.: 0.017 min
Response: 67352
Conc: 0.46 ug/ml

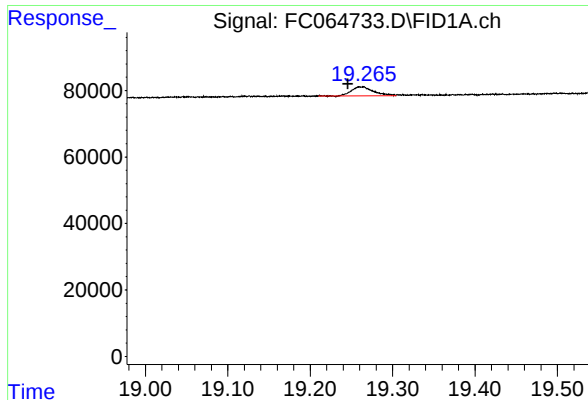


#19 n-Tetratriacontane (C34)

R.T.: 19.260 min
Delta R.T.: 0.014 min
Response: 49240
Conc: 0.35 ug/ml

Instrument :

FID_C

ClientSampleId :

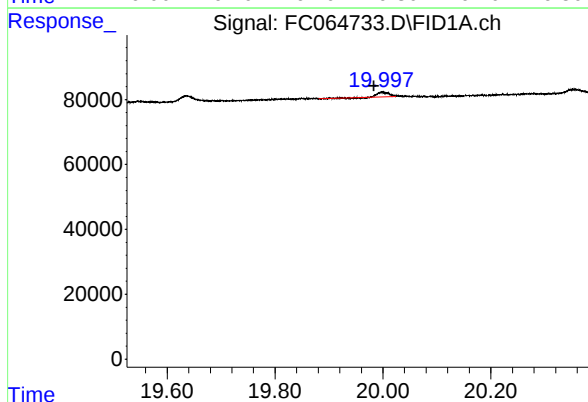

#20 n-Hexatriacontane (C36)

R.T.: 19.998 min
Delta R.T.: 0.014 min
Response: 17938
Conc: 0.13 ug/ml