

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100623AL\
 Data File : FC064754.D
 Signal(s) : FID1A.ch
 Acq On : 06 Oct 2023 06:44
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 07 02:36:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:25:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.008f	26676	0.183 ug/ml
Spiked Amount 50.000		Recovery =	0.37%
Target Compounds			
14) T n-Tetracosane (C24)	14.799	60708	0.382 ug/ml
16) T n-Octacosane (C28)	16.766	34318	0.232 ug/ml
17) T n-Tricontane (C30)	17.648	53551	0.360 ug/ml
18) T n-Dotriacontane (C32)	18.479	108233	0.742 ug/ml
19) T n-Tetratriacontane (C34)	19.258	56842	0.400 ug/ml
20) T n-Hexatriacontane (C36)	19.997	43339	0.315 ug/ml
21) T n-Octatriacontane (C38)	20.713	31533	0.230 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100623AL\
Data File : FC064754.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2023 06:44
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 07 02:36:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

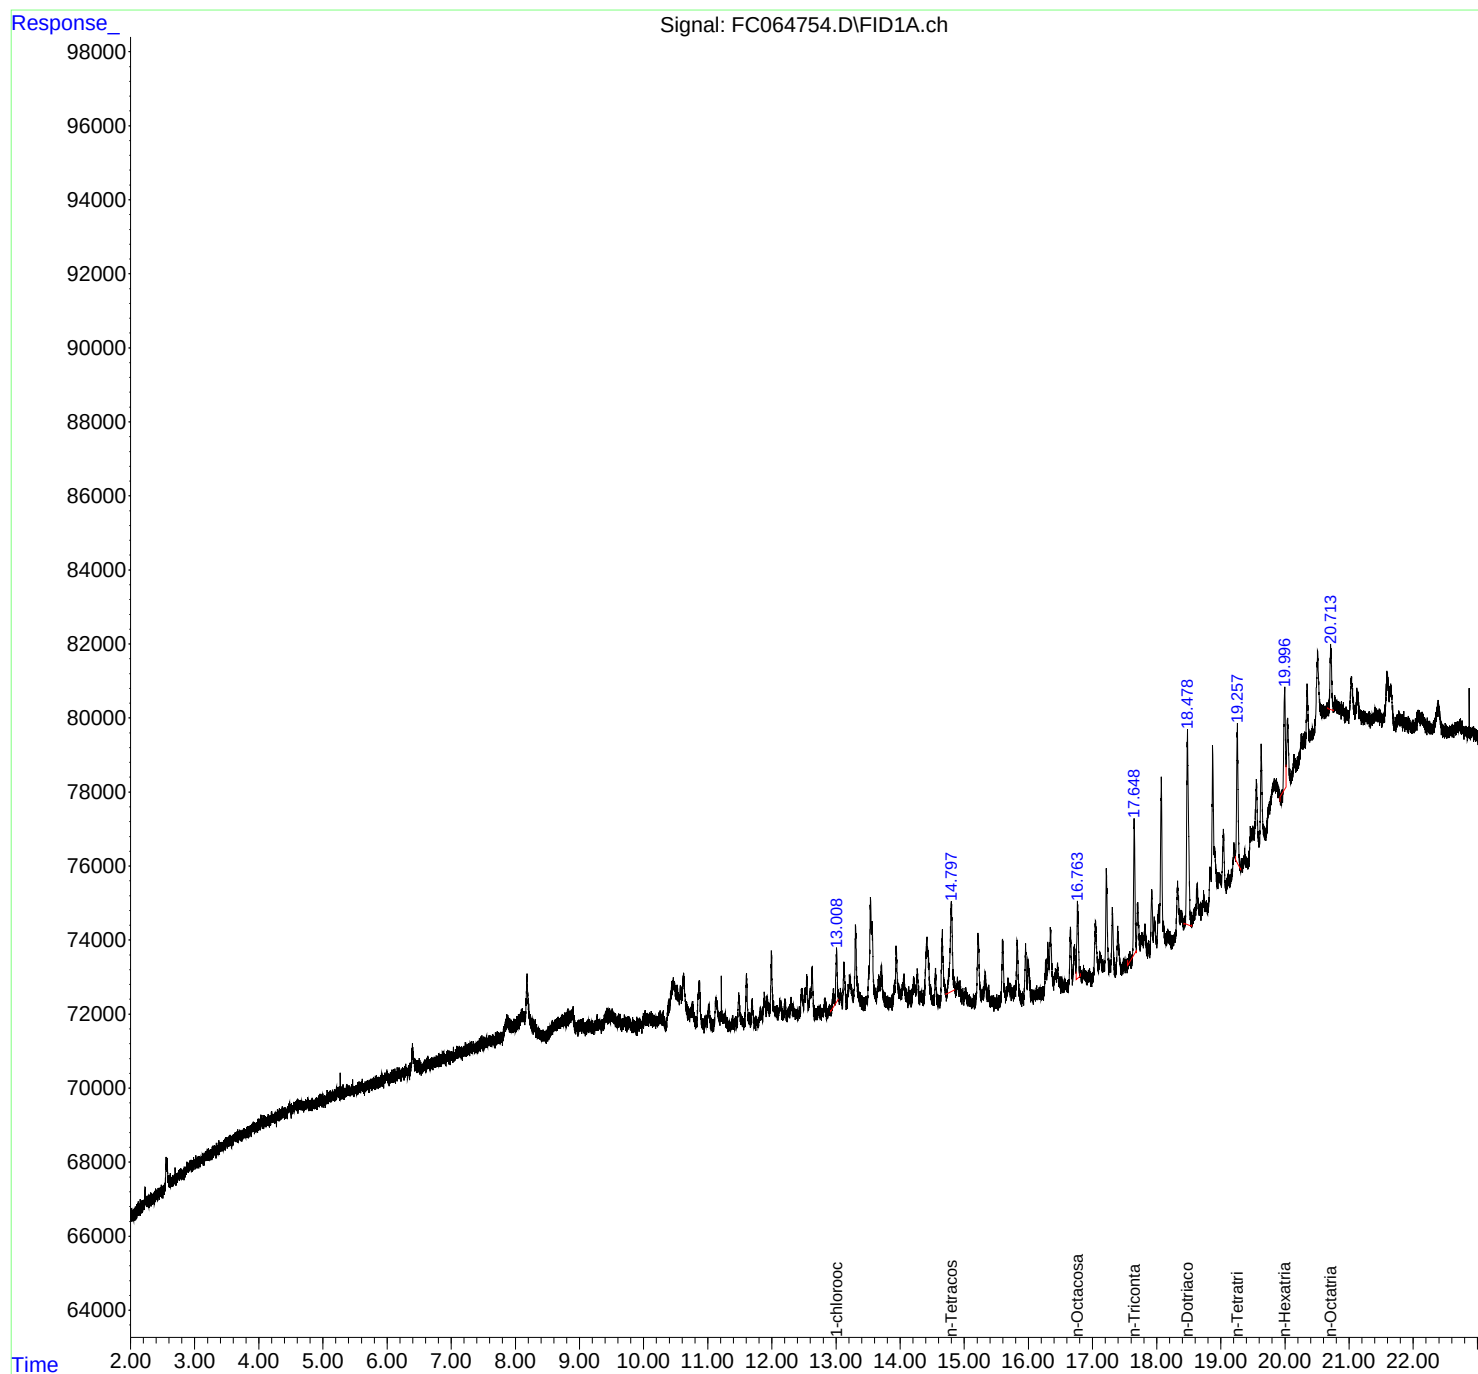


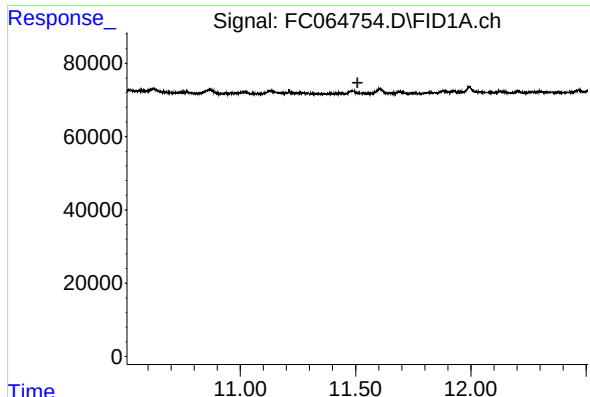

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

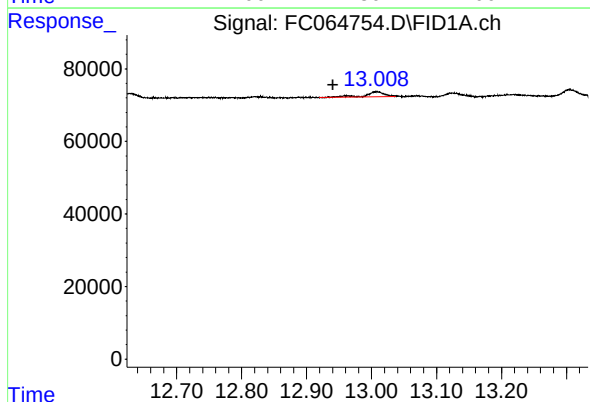


#12 1-chlorooctadecane (SURR)

R.T.: 13.008 min
Delta R.T.: 0.068 min
Response: 26676
Conc: 0.18 ug/ml

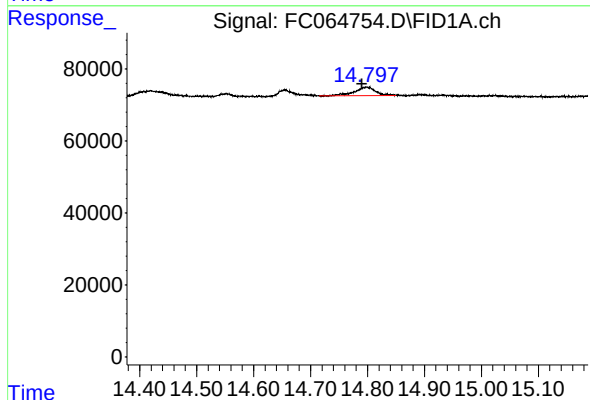


#14 n-Tetracosane (C24)

R.T.: 14.799 min
Delta R.T.: 0.008 min
Response: 60708
Conc: 0.38 ug/ml

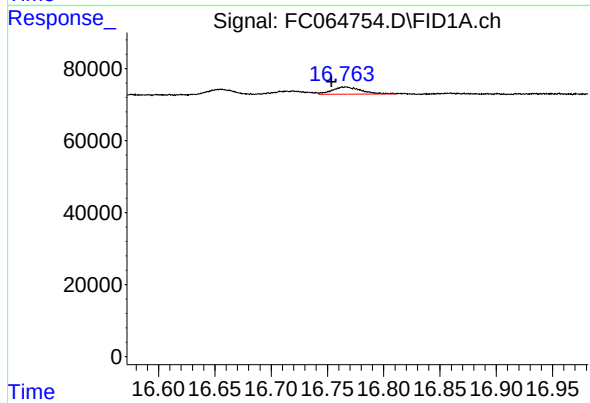

#16 n-Octacosane (C28)


R.T.: 16.766 min
Delta R.T.: 0.012 min
Response: 34318
Conc: 0.23 ug/ml

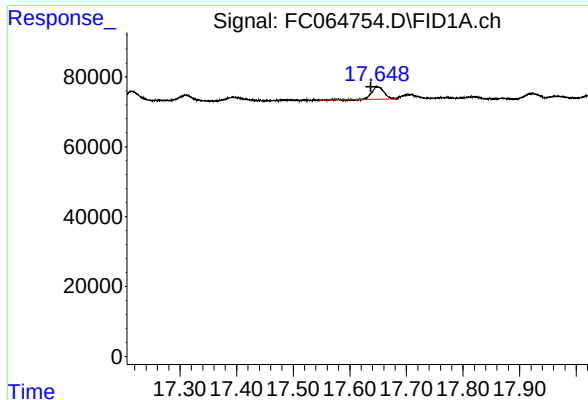

#17 n-Tricontane (C30)


R.T.: 17.648 min
Delta R.T.: 0.011 min
Response: 53551
Conc: 0.36 ug/ml

Instrument :
FID_C
ClientSampleId :

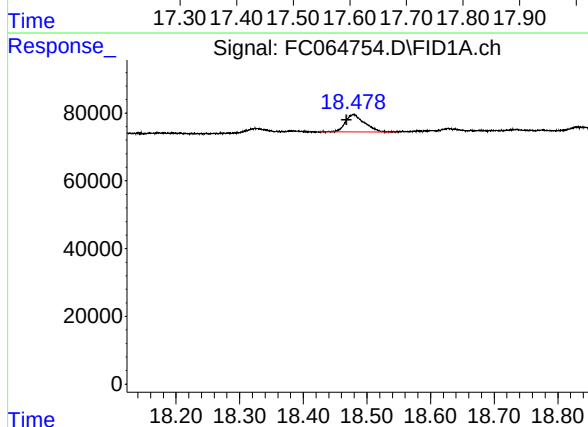


#18 n-Dotriacontane (C32)

R.T.: 18.479 min
Delta R.T.: 0.011 min
Response: 108233
Conc: 0.74 ug/ml

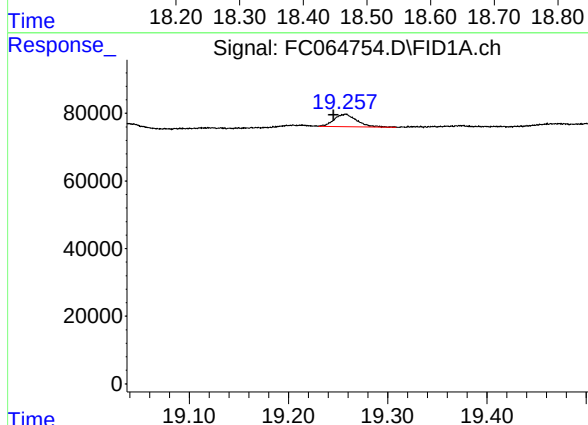


#19 n-Tetratriacontane (C34)

R.T.: 19.258 min
Delta R.T.: 0.012 min
Response: 56842
Conc: 0.40 ug/ml

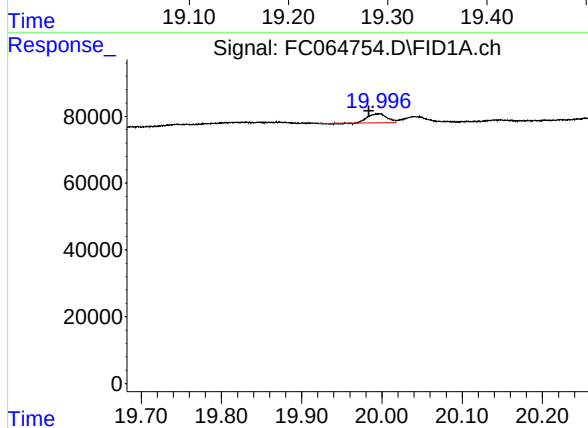

#20 n-Hexatriacontane (C36)

R.T.: 19.997 min
Delta R.T.: 0.013 min
Response: 43339
Conc: 0.31 ug/ml

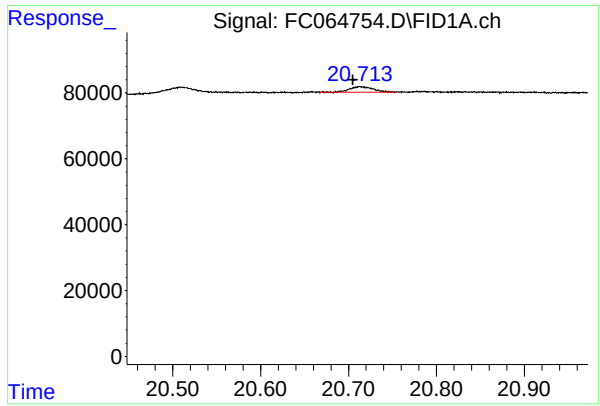

#21 n-Octatriacontane (C38)

R.T.: 20.713 min
Delta R.T.: 0.008 min
Response: 31533
Conc: 0.23 ug/ml

Instrument :

FID_C

ClientSampleId :