

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100623AL\
Data File : FC064761.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2023 13:14
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 07 02:37:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.655	54251	0.365 ug/ml
18) T	n-Dotriacontane (C32)	18.483	78794	0.540 ug/ml
19) T	n-Tetratriacontane (C34)	19.264	64369	0.453 ug/ml
20) T	n-Hexatriacontane (C36)	20.001	41365	0.300 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100623AL\
Data File : FC064761.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2023 13:14
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 07 02:37:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

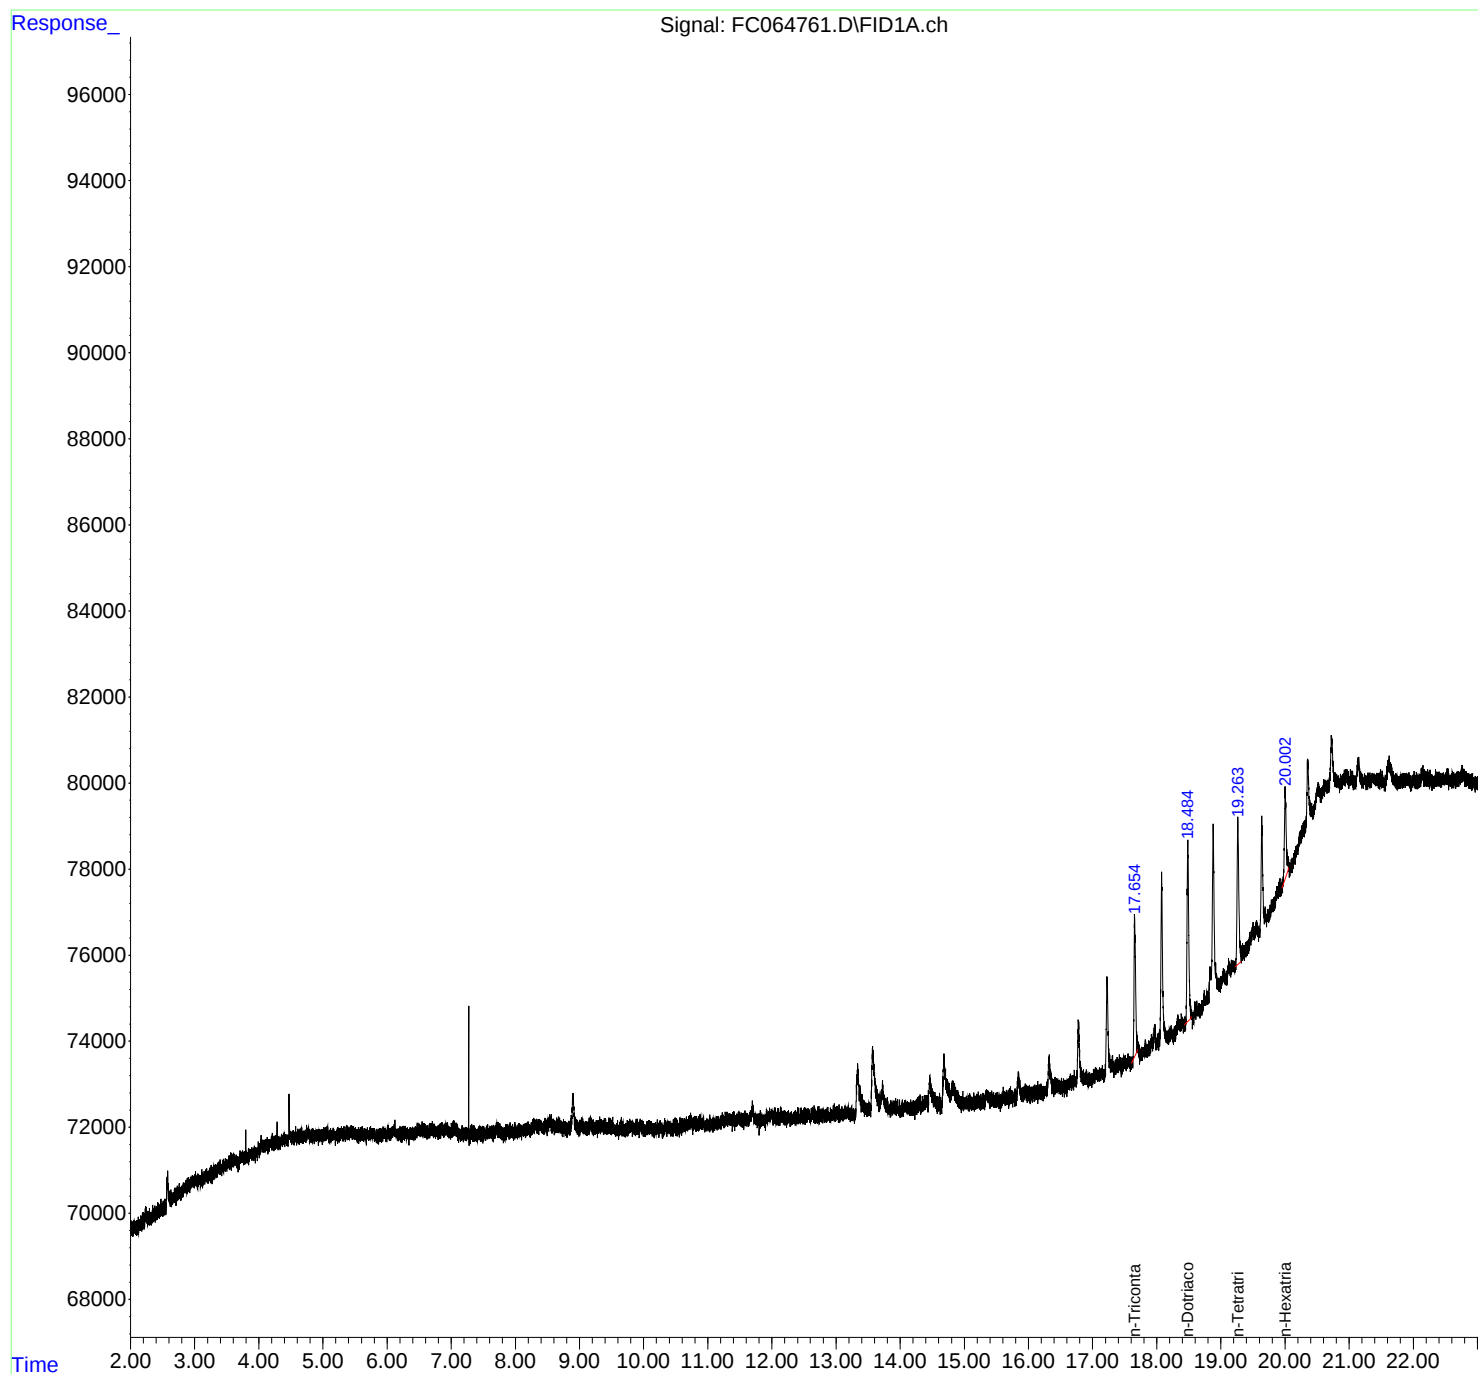


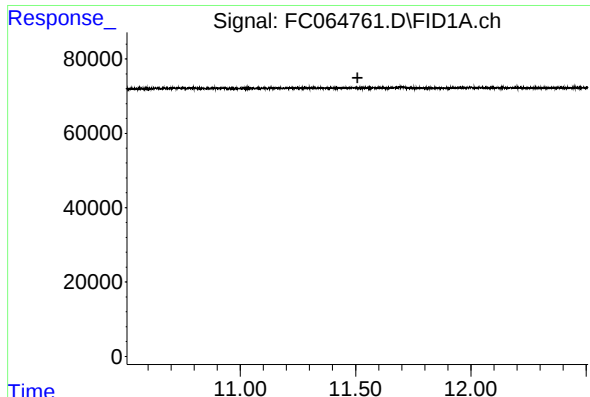

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

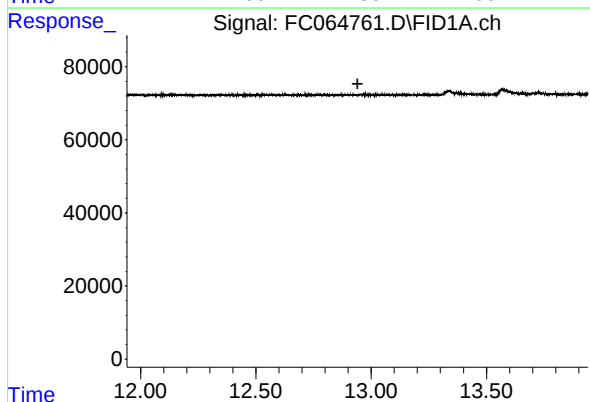


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.940 min
Response: 0
Conc: N.D.

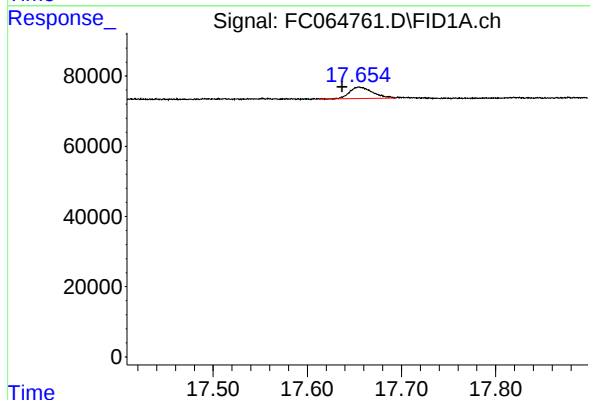


#17 n-Tricontane (C30)

R.T.: 17.655 min
Delta R.T.: 0.018 min
Response: 54251
Conc: 0.37 ug/ml

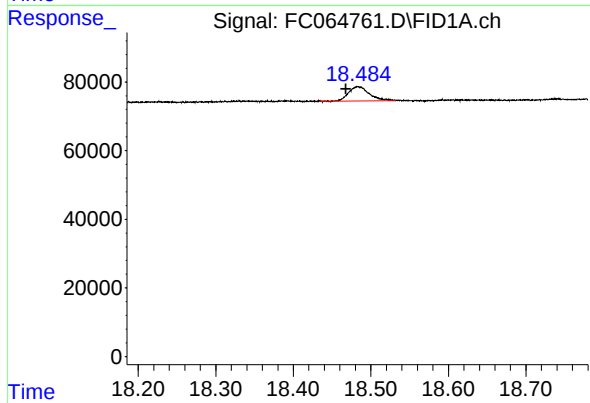

#18 n-Dotriacontane (C32)

R.T.: 18.483 min
Delta R.T.: 0.015 min
Response: 78794
Conc: 0.54 ug/ml

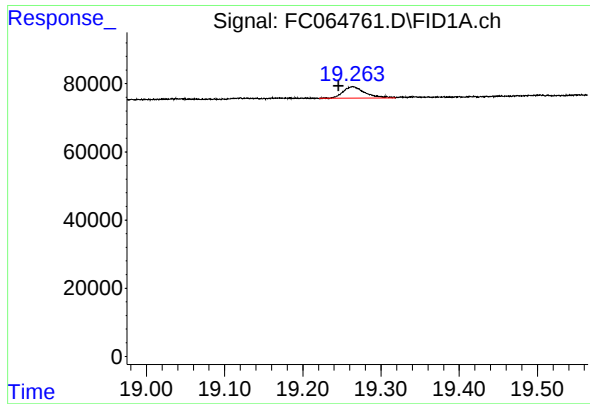


#19 n-Tetratriacontane (C34)

R.T.: 19.264 min
Delta R.T.: 0.018 min
Response: 64369
Conc: 0.45 ug/ml

Instrument :

FID_C

ClientSampleId :

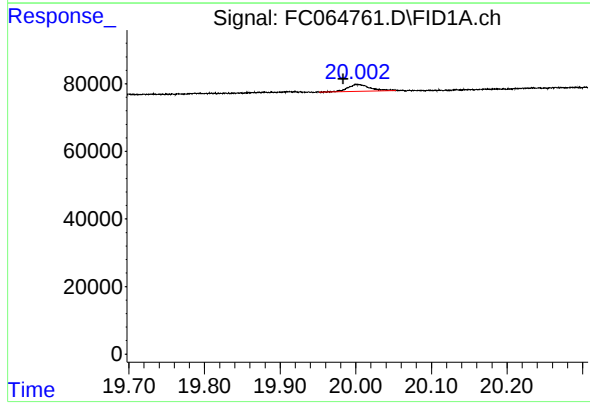

#20 n-Hexatriacontane (C36)

R.T.: 20.001 min
Delta R.T.: 0.017 min
Response: 41365
Conc: 0.30 ug/ml