

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100623AL\
 Data File : FC064770.D
 Signal(s) : FID1A.ch
 Acq On : 06 Oct 2023 22:38
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 07 02:38:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 15 01:25:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) T n-Octacosane (C28)	16.770	27078	0.183 ug/ml
17) T n-Tricontane (C30)	17.651	59749	0.402 ug/ml
18) T n-Dotriacontane (C32)	18.479	87434	0.599 ug/ml
19) T n-Tetratriacontane (C34)	19.258	97472	0.686 ug/ml
20) T n-Hexatriacontane (C36)	19.998	154685	1.123 ug/ml
21) T n-Octatriacontane (C38)	20.715	92001	0.671 ug/ml
22) T n-Tetracontane (C40)	21.640	150995	1.110 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100623AL\
Data File : FC064770.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2023 22:38
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 07 02:38:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 091523.M
Quant Title : GC Extractables
QLast Update : Fri Sep 15 01:25:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

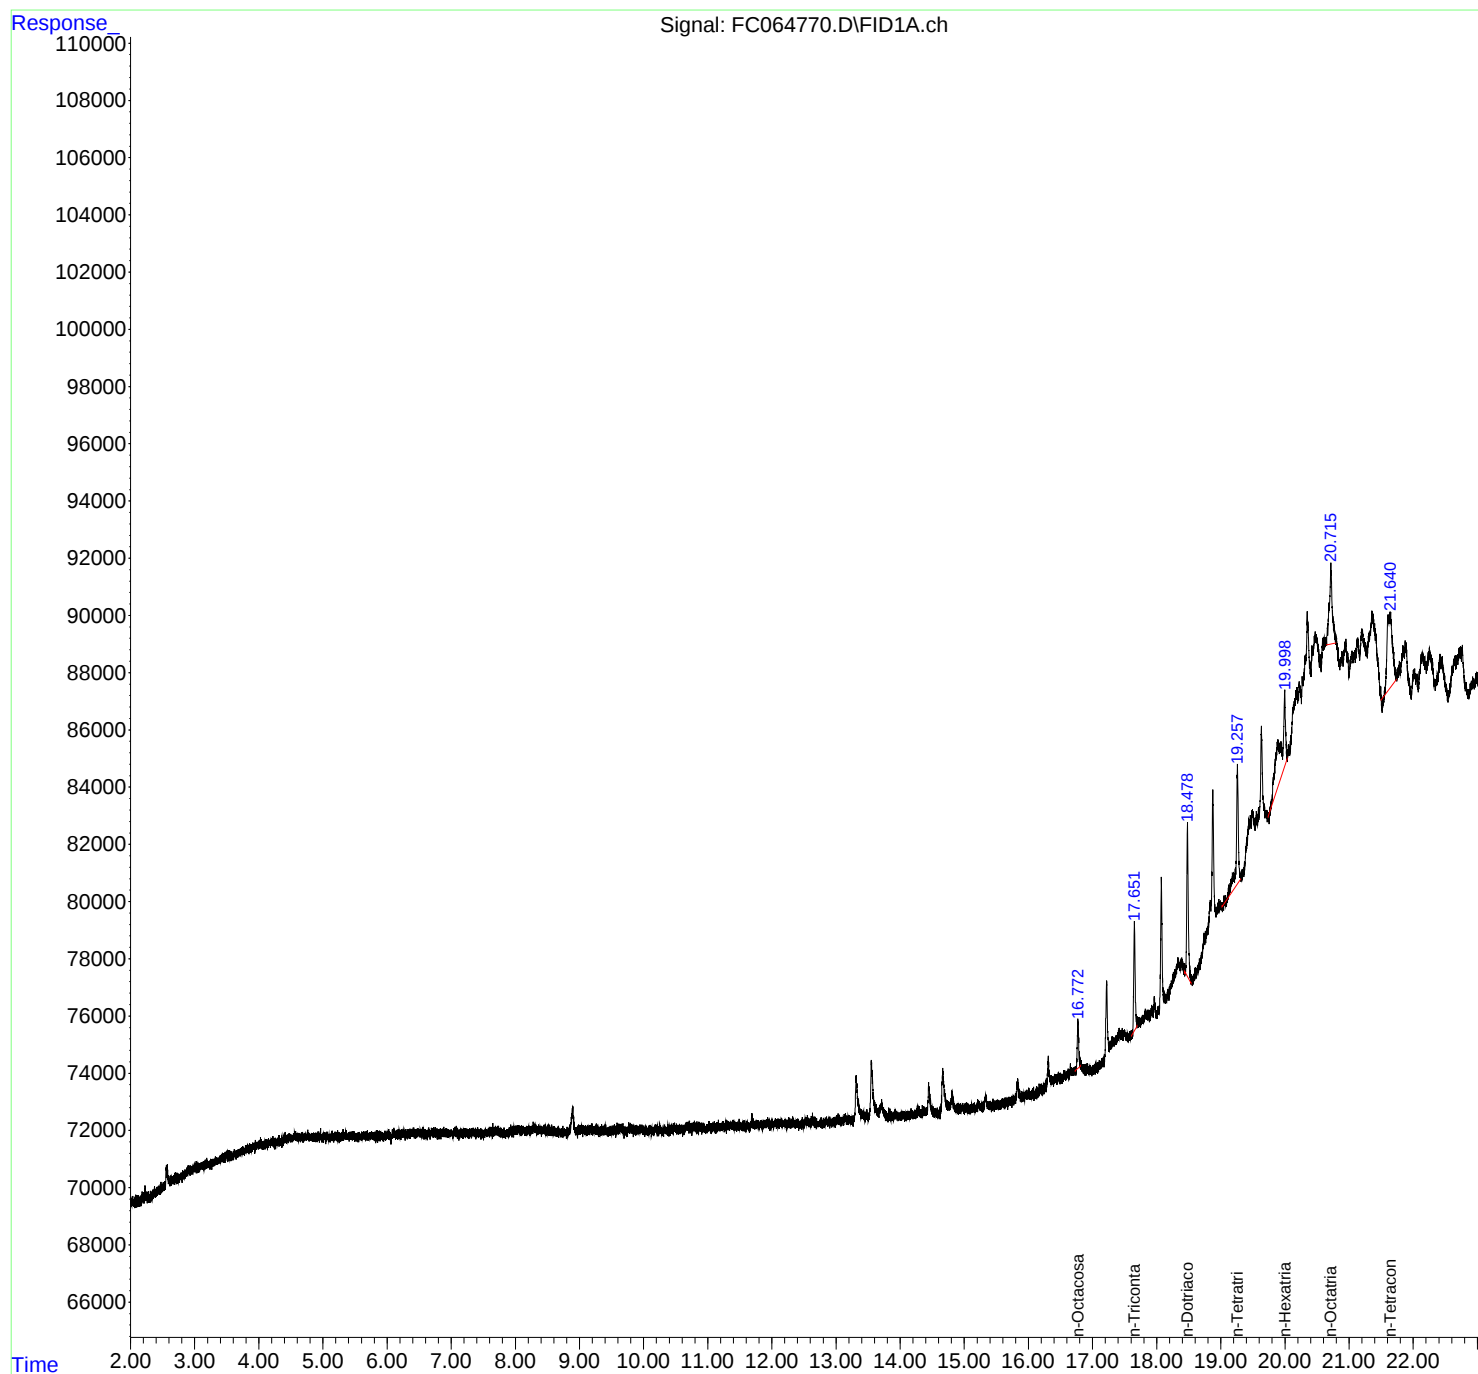


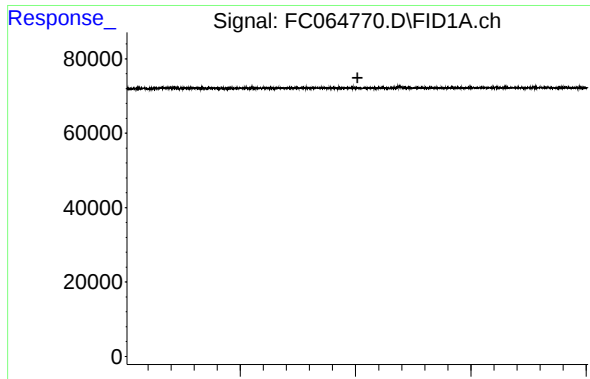

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.508 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

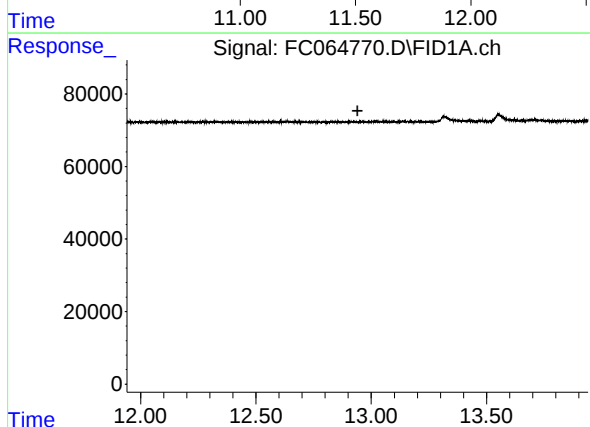


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.940 min
Response: 0
Conc: N.D.

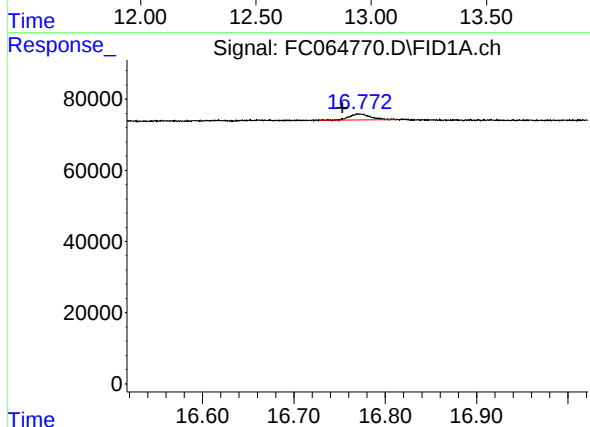


#16 n-Octacosane (C28)

R.T.: 16.770 min
Delta R.T.: 0.017 min
Response: 27078
Conc: 0.18 ug/ml

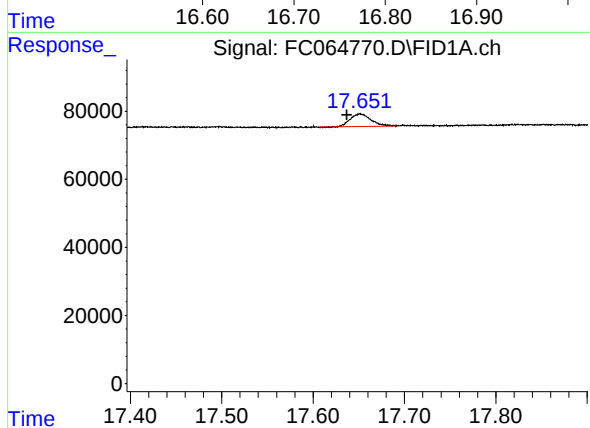

#17 n-Tricontane (C30)


R.T.: 17.651 min
Delta R.T.: 0.014 min
Response: 59749
Conc: 0.40 ug/ml

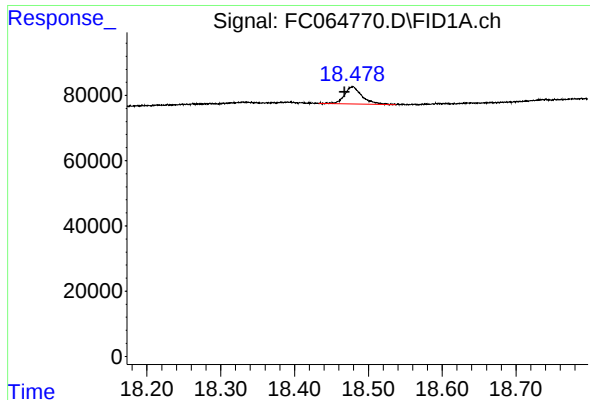

#18 n-Dotriacontane (C32)


R.T.: 18.479 min
Delta R.T.: 0.011 min
Response: 87434
Conc: 0.60 ug/ml

Instrument :
FID_C
ClientSampleId :

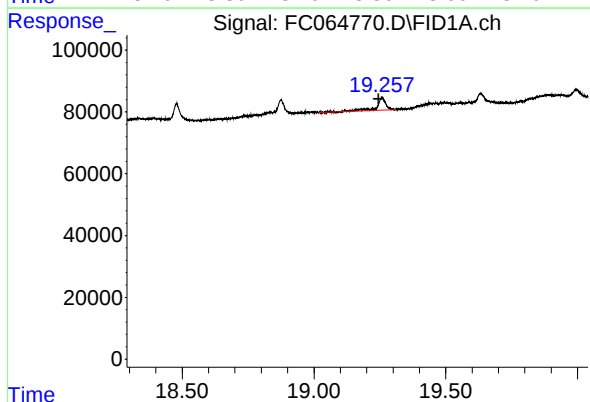


#19 n-Tetratriacontane (C34)

R.T.: 19.258 min
Delta R.T.: 0.013 min
Response: 97472
Conc: 0.69 ug/ml

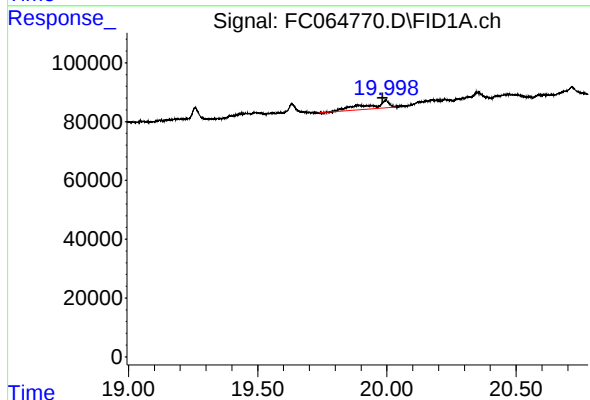


#20 n-Hexatriacontane (C36)

R.T.: 19.998 min
Delta R.T.: 0.014 min
Response: 154685
Conc: 1.12 ug/ml

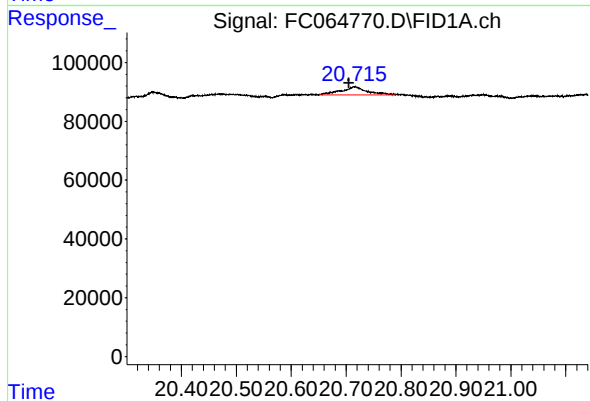

#21 n-Octatriacontane (C38)

R.T.: 20.715 min
Delta R.T.: 0.010 min
Response: 92001
Conc: 0.67 ug/ml

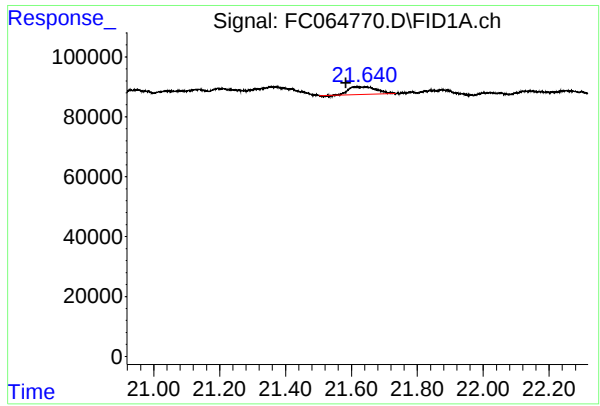

#22 n-Tetracontane (C40)

R.T.: 21.640 min

Delta R.T.: 0.057 min

Response: 150995

Conc: 1.11 ug/ml

Instrument :

FID_C

ClientSampleId :