

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100824AL\
Data File : FC067383.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2024 06:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 02:09:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.266	150092	1.373 ug/ml
21) T	n-Octatriacontane (C38)	20.671	687055	7.834 ug/ml
22) T	n-Tetracontane (C40)	21.593	887743	10.317 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100824AL\
Data File : FC067383.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2024 06:36
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 02:09:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

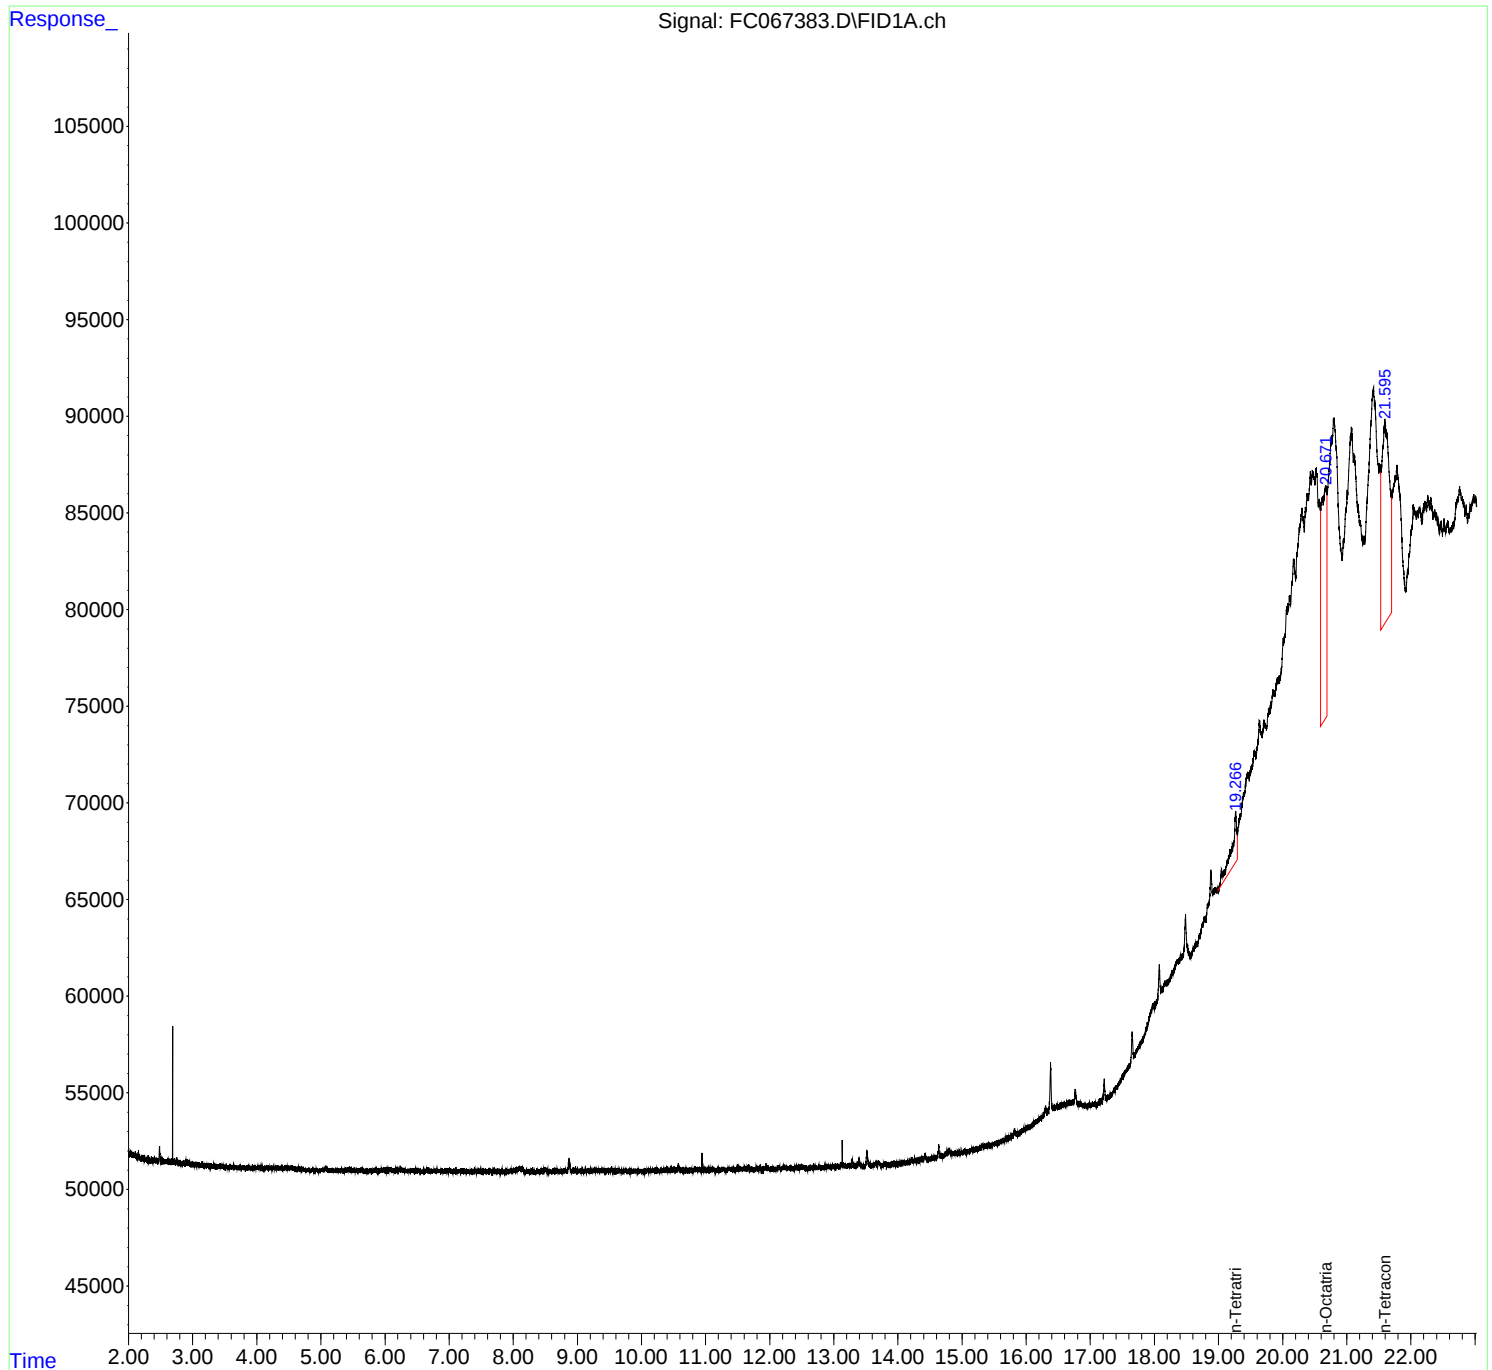


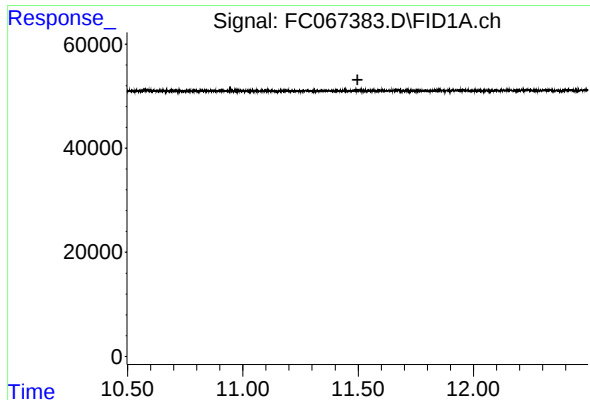

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

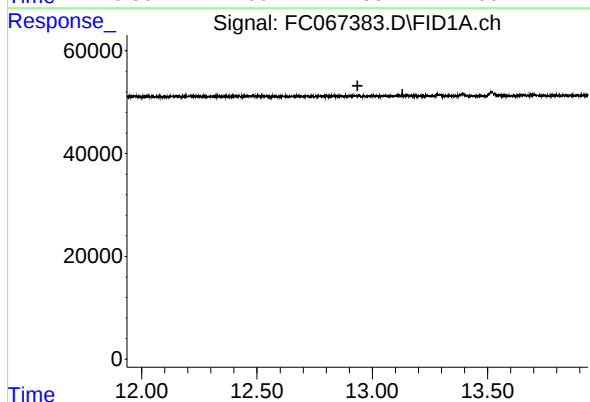


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

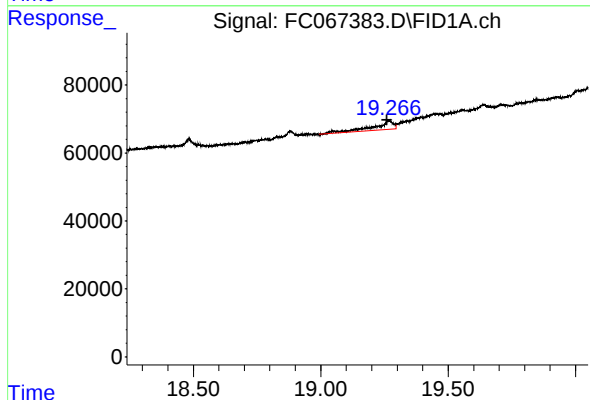


#19 n-Tetratriacontane (C34)

R.T.: 19.266 min
Delta R.T.: 0.006 min
Response: 150092
Conc: 1.37 ug/ml

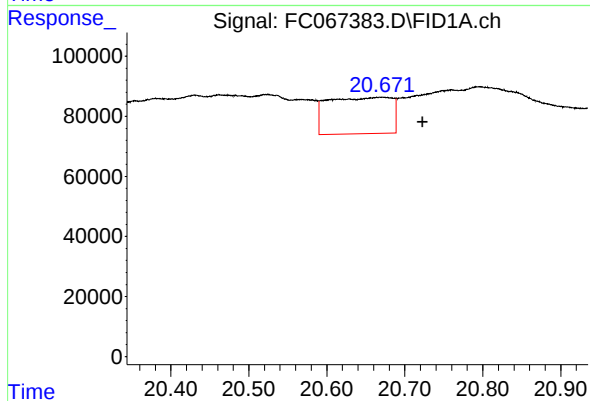

#21 n-Octatriacontane (C38)

R.T.: 20.671 min
Delta R.T.: -0.052 min
Response: 687055
Conc: 7.83 ug/ml

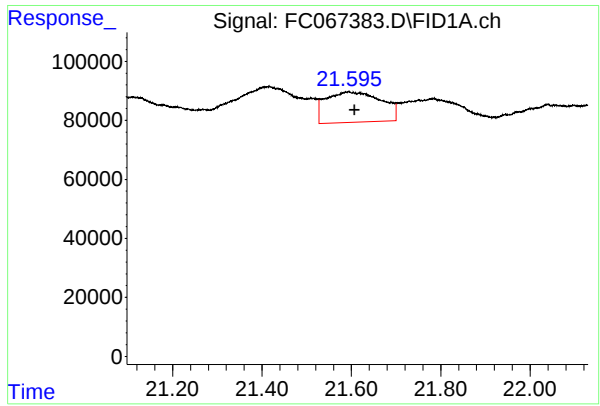

#22 n-Tetracontane (C40)

R.T.: 21.593 min
Delta R.T.: -0.014 min
Response: 887743
Conc: 10.32 ug/ml

Instrument :
FID_C
ClientSampleId :