

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100824AL\
 Data File : FC067386.D
 Signal(s) : FID1A.ch
 Acq On : 08 Oct 2024 09:58
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 09 02:10:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 01 09:13:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
20) T	n-Hexatriacontane (C36)	19.995	259425	2.745 ug/ml
21) T	n-Octatriacontane (C38)	20.787f	1017218	11.599 ug/ml
22) T	n-Tetracontane (C40)	21.570	604315	7.023 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC100824AL\
Data File : FC067386.D
Signal(s) : FID1A.ch
Acq On : 08 Oct 2024 09:58
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 09 02:10:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

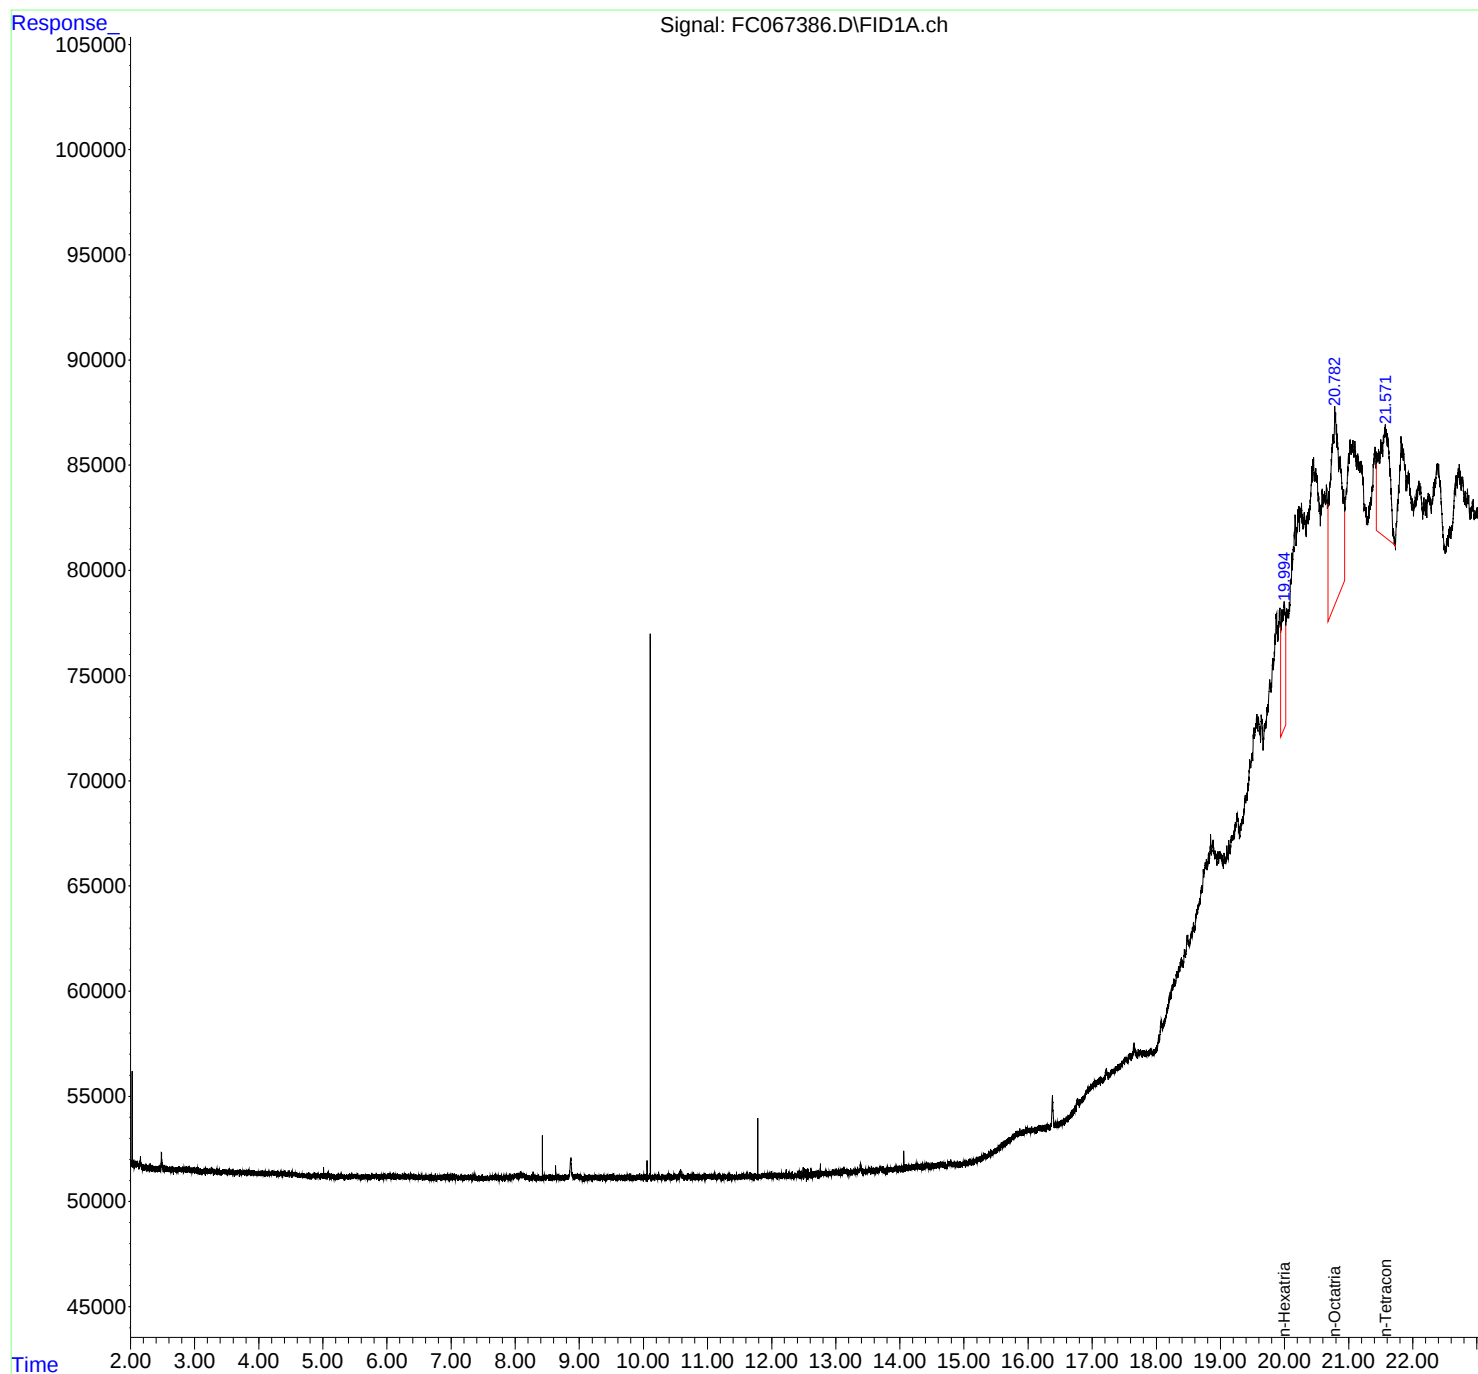


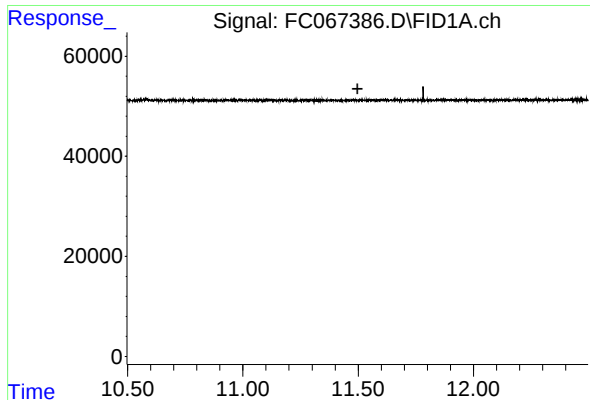

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

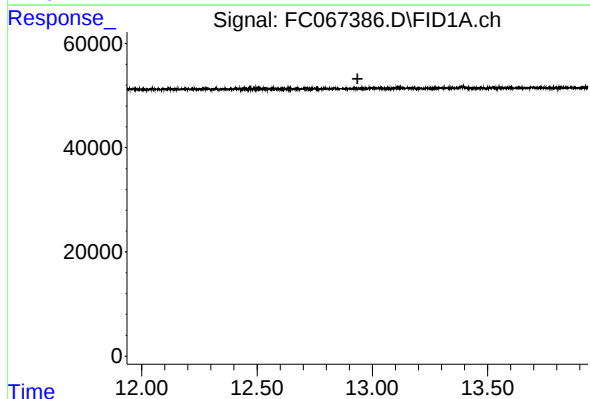


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.936 min
Response: 0
Conc: N.D.

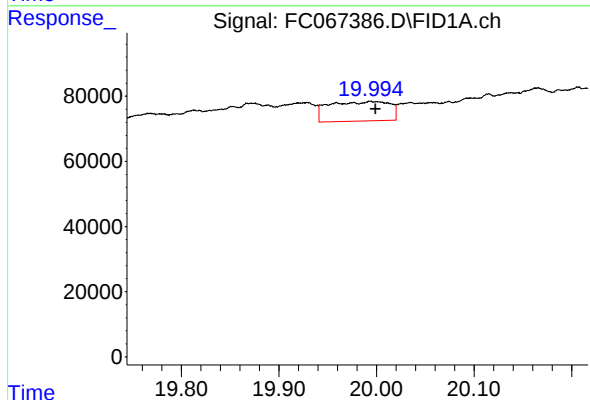


#20 n-Hexatriacontane (C36)

R.T.: 19.995 min
Delta R.T.: -0.004 min
Response: 259425
Conc: 2.74 ug/ml

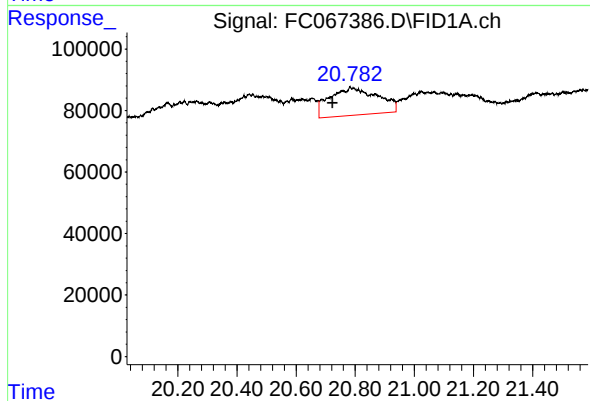

#21 n-Octatriacontane (C38)

R.T.: 20.787 min
Delta R.T.: 0.064 min
Response: 1017218
Conc: 11.60 ug/ml

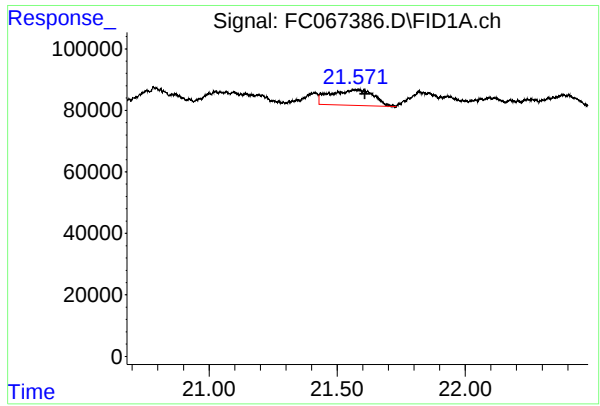

#22 n-Tetracontane (C40)

R.T.: 21.570 min
Delta R.T.: -0.038 min
Response: 604315
Conc: 7.02 ug/ml

Instrument :

FID_C

ClientSampleId :