

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101223AL\
Data File : FC064791.D
Signal(s) : FID1A.ch
Acq On : 12 Oct 2023 08:07
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 13 01:10:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 12:17:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	14.798	78164	0.491 ug/ml
21) T	n-Octatriacontane (C38)	20.719	102002	0.770 ug/ml
22) T	n-Tetracontane (C40)	21.604	304941	2.437 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101223AL\
Data File : FC064791.D
Signal(s) : FID1A.ch
Acq On : 12 Oct 2023 08:07
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 13 01:10:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 12:17:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

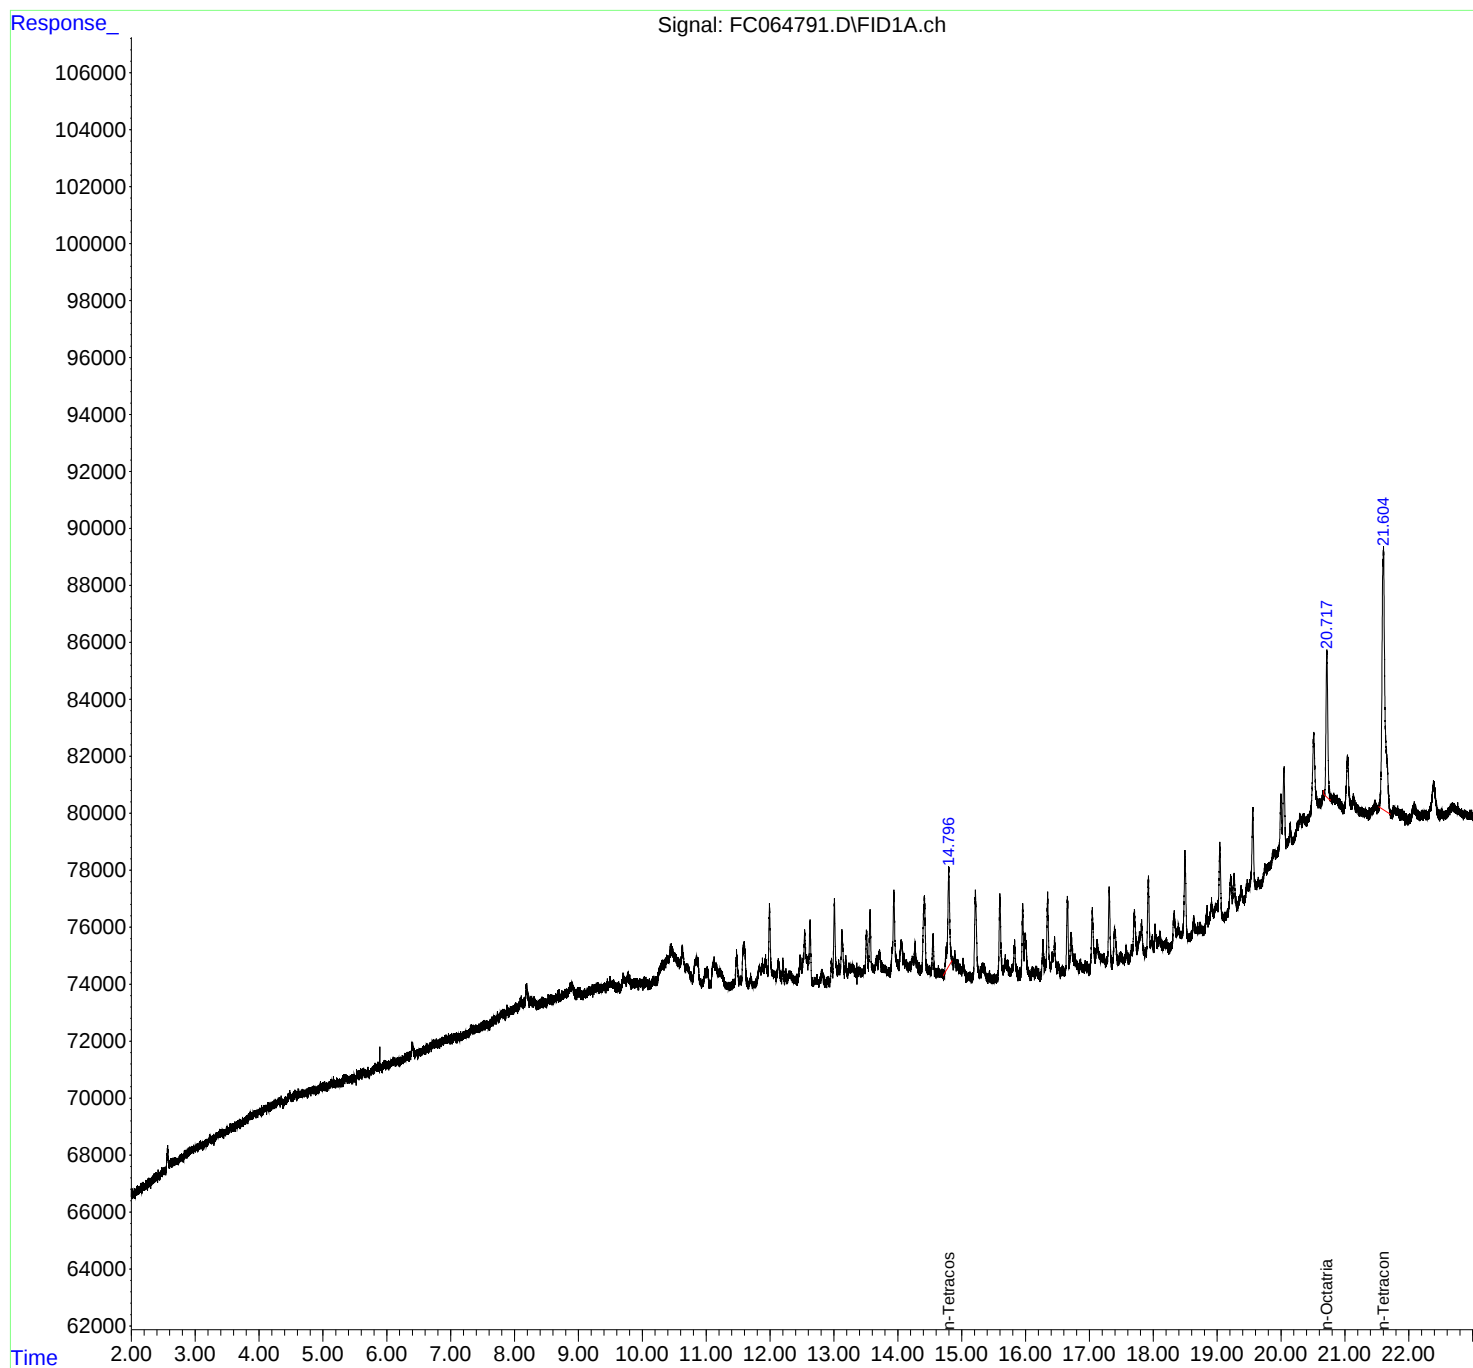


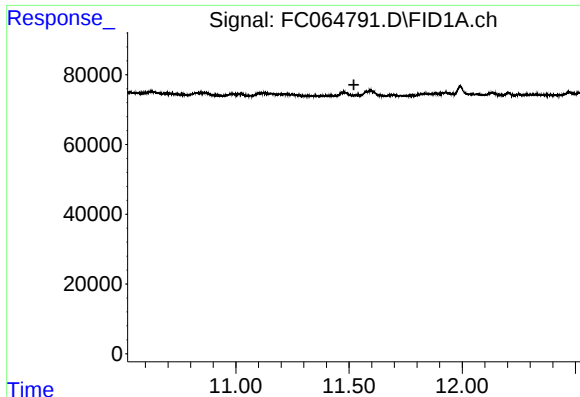

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.521 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

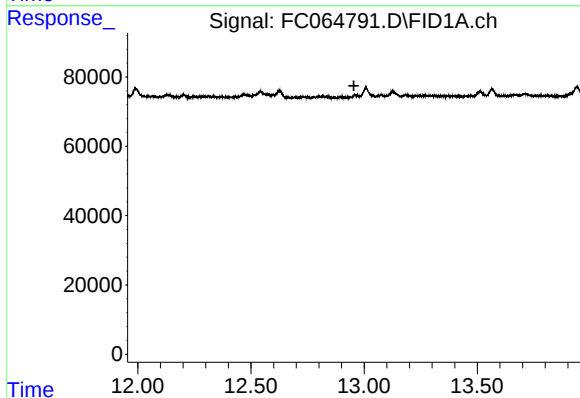


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

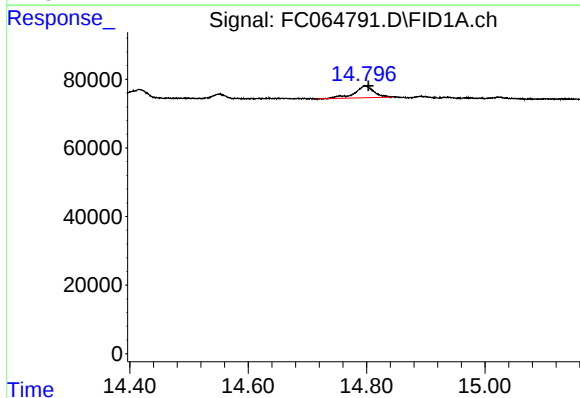


#14 n-Tetracosane (C24)

R.T.: 14.798 min
Delta R.T.: -0.005 min
Response: 78164
Conc: 0.49 ug/ml

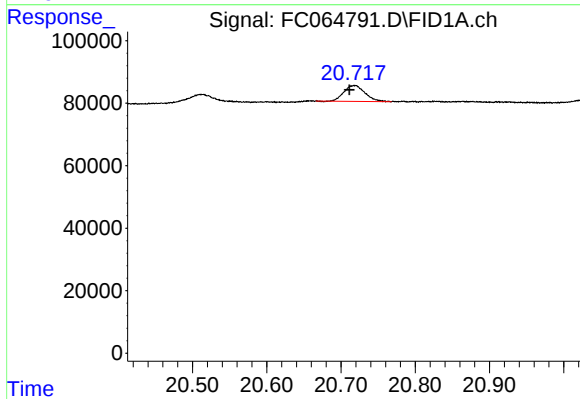

#21 n-Octatriacontane (C38)

R.T.: 20.719 min
Delta R.T.: 0.008 min
Response: 102002
Conc: 0.77 ug/ml

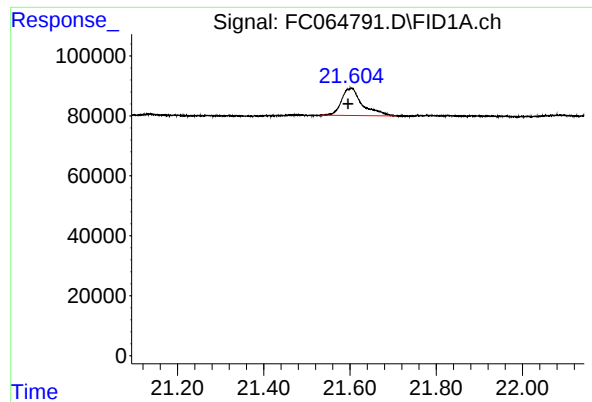

#22 n-Tetracontane (C40)

R.T.: 21.604 min
Delta R.T.: 0.008 min
Response: 304941
Conc: 2.44 ug/ml

Instrument :

FID_C

ClientSampleId :