

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101323AL\
 Data File : FC064817.D
 Signal(s) : FID1A.ch
 Acq On : 13 Oct 2023 23:38
 Operator : YP/AJ
 Sample : 04798-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 14 02:59:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 12:17:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.952	4603393	30.701 ug/ml
Spiked Amount 50.000		Recovery =	61.40%
Target Compounds			
10) T n-Eicosane (C20)	12.514	67625	0.393 ug/ml
11) T n-Heneicosane (C21)	13.121	30873	0.182 ug/ml
13) T n-Docosane (C22)	13.705	52772	0.320 ug/ml
14) T n-Tetracosane (C24)	14.801	36740	0.231 ug/ml
15) T n-Hexacosane (C26)	15.818	28470	0.186 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101323AL\
Data File : FC064817.D
Signal(s) : FID1A.ch
Acq On : 13 Oct 2023 23:38
Operator : YP/AJ
Sample : 04798-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 02:59:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 12:17:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

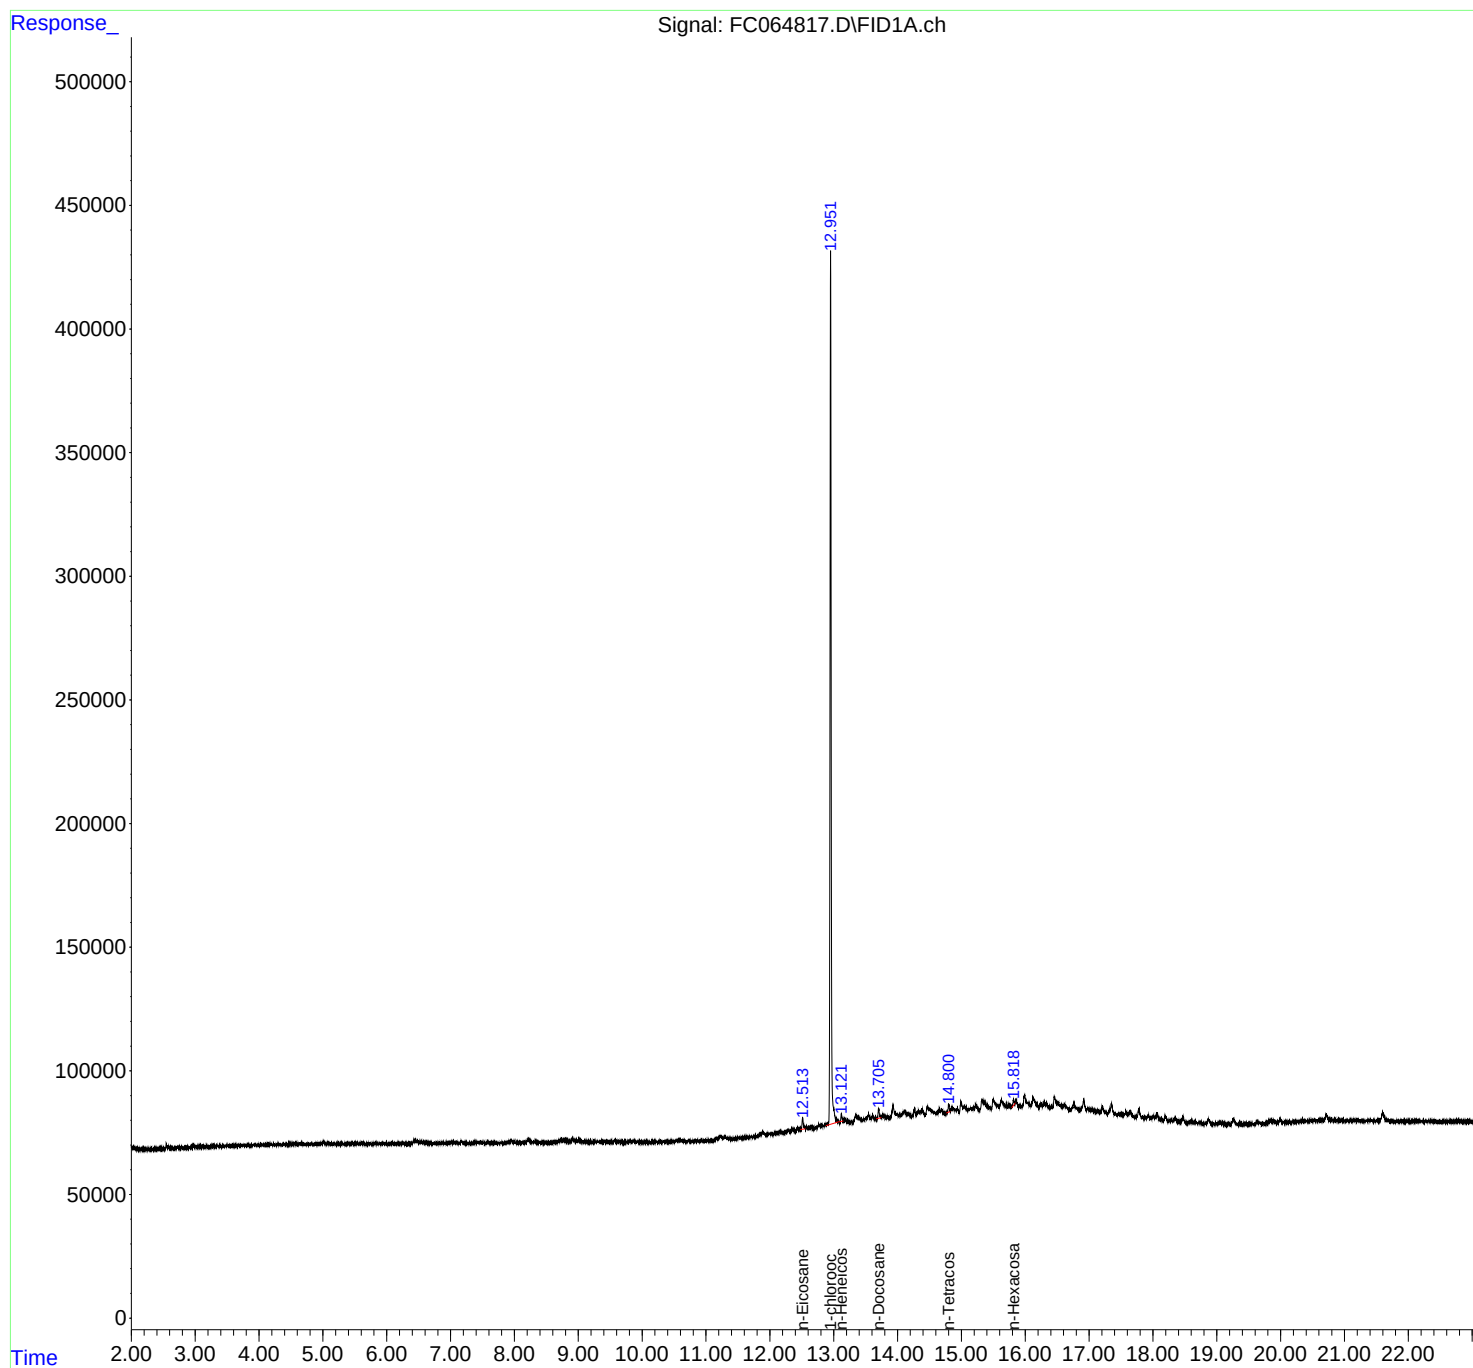


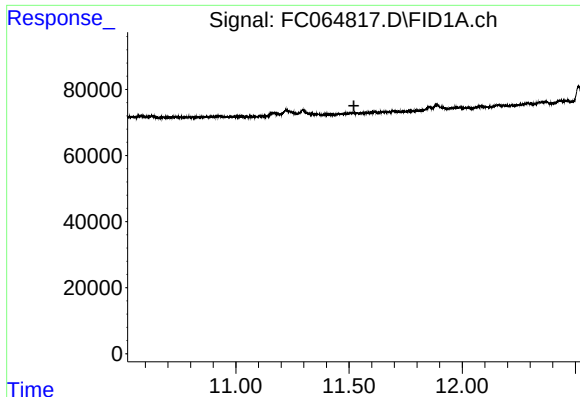

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.521 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

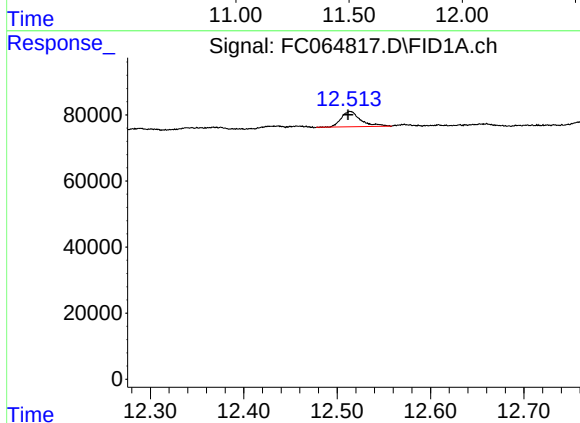


#10 n-Eicosane (C20)

R.T.: 12.514 min
Delta R.T.: 0.003 min
Response: 67625
Conc: 0.39 ug/ml

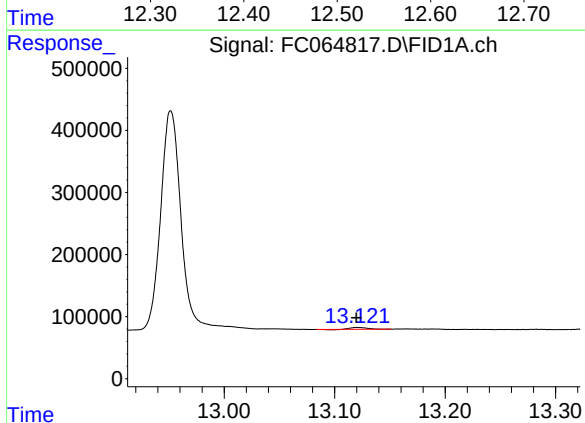


#11 n-Heneicosane (C21)

R.T.: 13.121 min
Delta R.T.: 0.001 min
Response: 30873
Conc: 0.18 ug/ml

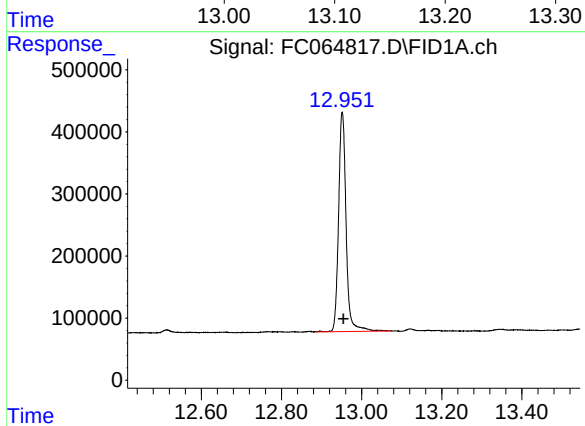

#12 1-chlorooctadecane (SURR)


R.T.: 12.952 min
Delta R.T.: -0.003 min
Response: 4603393
Conc: 30.70 ug/ml

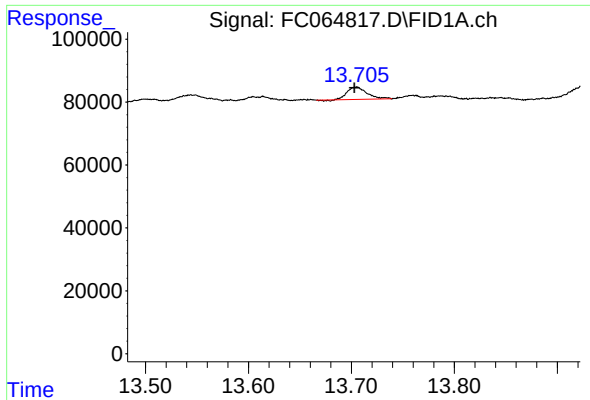

#13 n-Docosane (C22)


R.T.: 13.705 min
Delta R.T.: 0.002 min
Response: 52772
Conc: 0.32 ug/ml

Instrument :
FID_C
ClientSampleId :

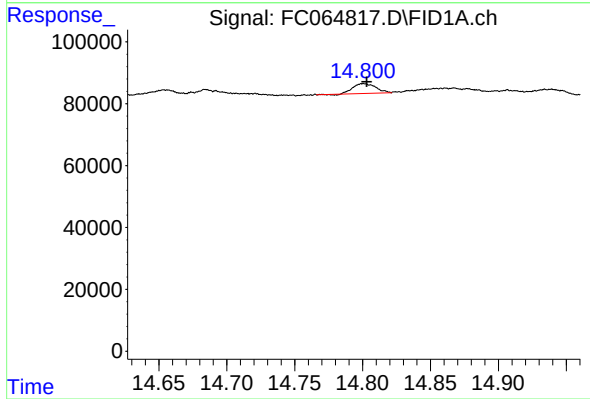

#14 n-Tetracosane (C24)

R.T.: 14.801 min
Delta R.T.: -0.002 min
Response: 36740
Conc: 0.23 ug/ml

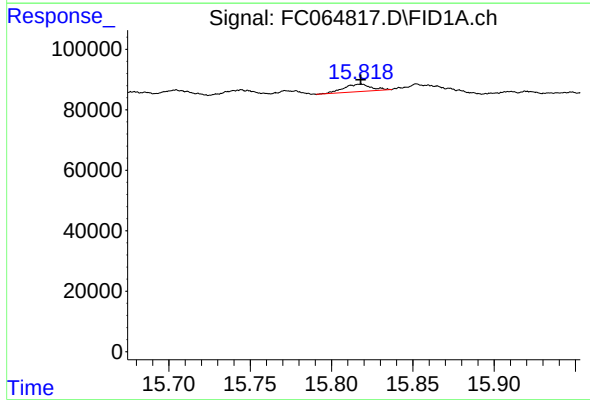

#15 n-Hexacosane (C26)

R.T.: 15.818 min
Delta R.T.: 0.000 min
Response: 28470
Conc: 0.19 ug/ml