

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101323AL\
 Data File : FC064826.D
 Signal(s) : FID1A.ch
 Acq On : 14 Oct 2023 05:18
 Operator : YP/AJ
 Sample : 04816-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 14 06:35:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 12:17:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.953	9102971	60.710 ug/ml
Spiked Amount 50.000		Recovery =	121.42%
Target Compounds			
20) T n-Hexatriacontane (C36)	19.992	47836	0.346 ug/ml
21) T n-Octatriacontane (C38)	20.711	95803	0.723 ug/ml
22) T n-Tetracontane (C40)	21.593	158610	1.267 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101323AL\
Data File : FC064826.D
Signal(s) : FID1A.ch
Acq On : 14 Oct 2023 05:18
Operator : YP/AJ
Sample : 04816-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 14 06:35:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 12:17:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

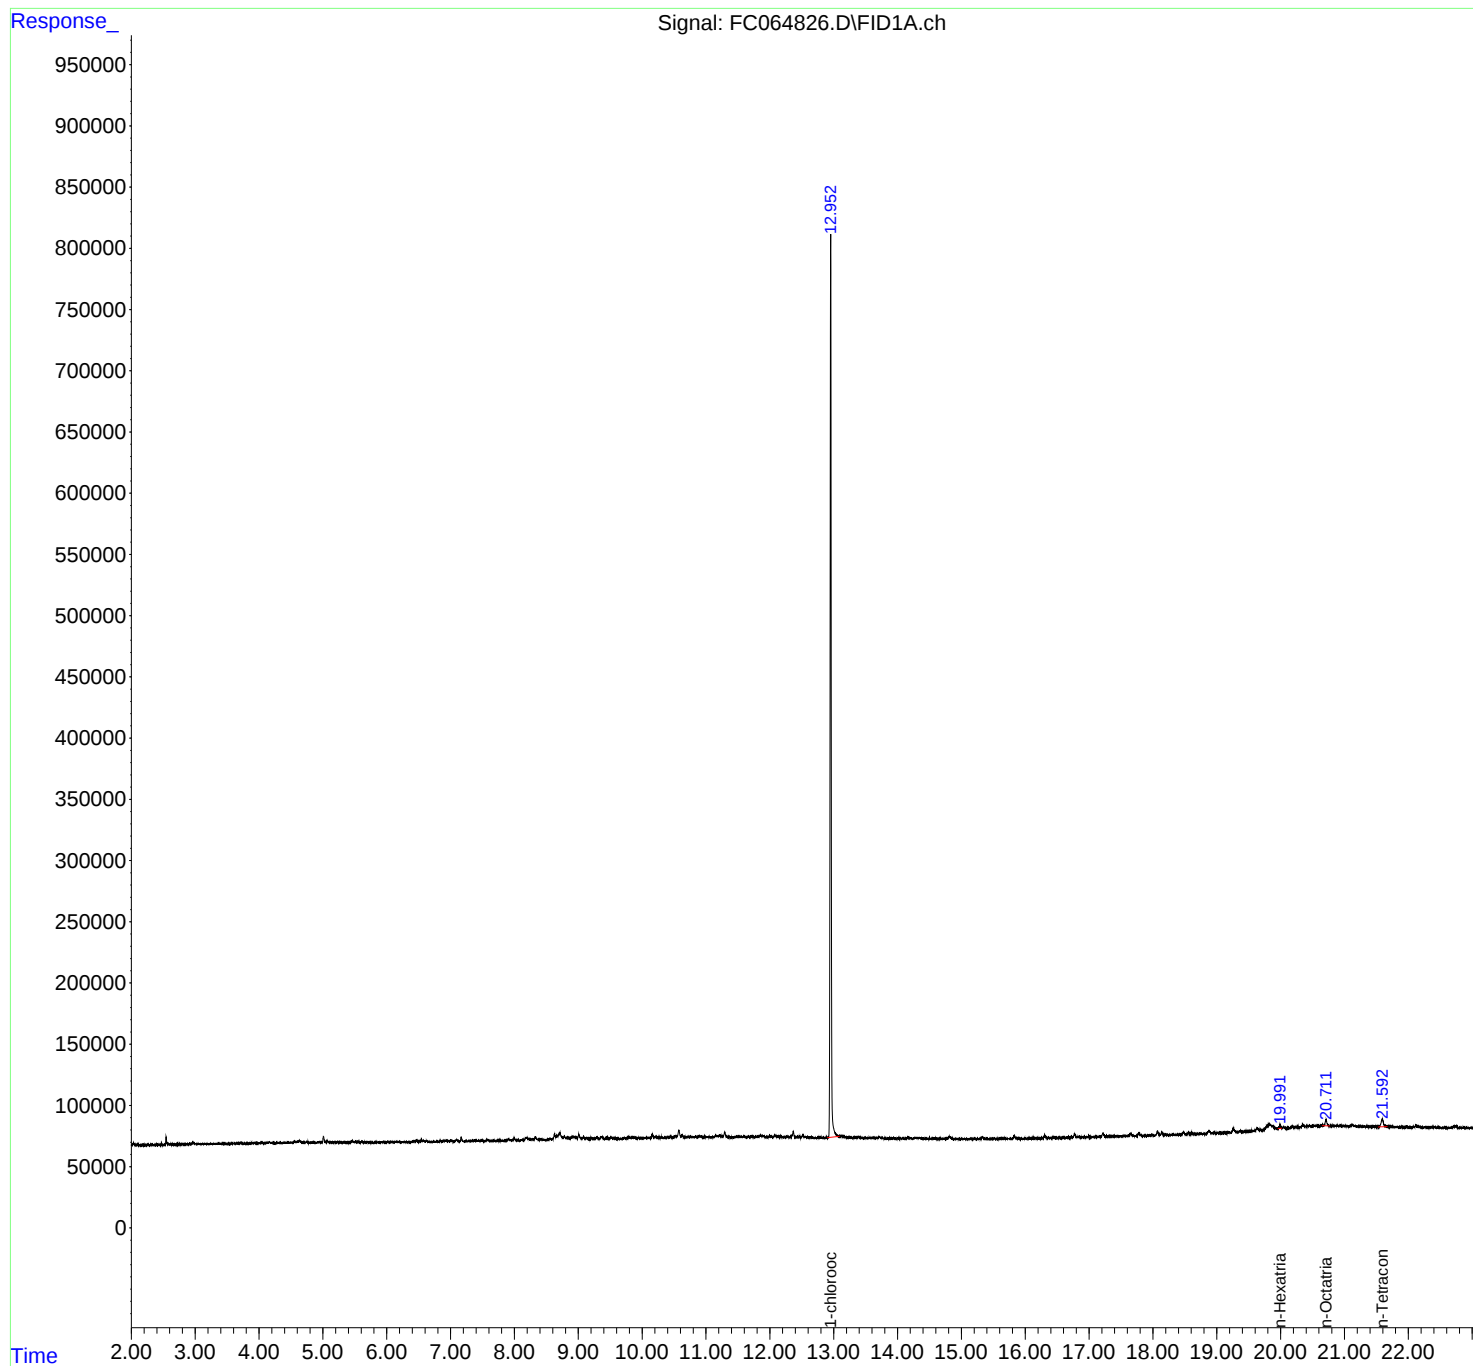


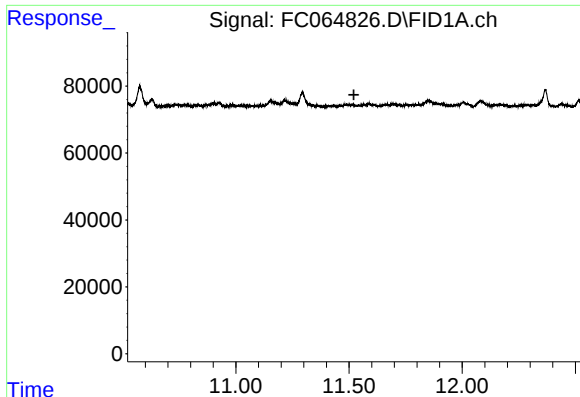

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.521 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

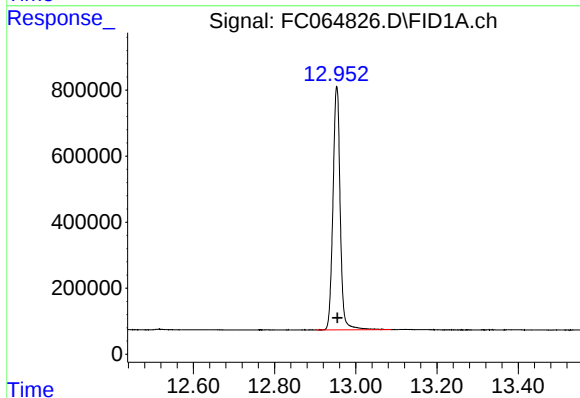


#12 1-chlorooctadecane (SURR)

R.T.: 12.953 min
Delta R.T.: -0.001 min
Response: 9102971
Conc: 60.71 ug/ml

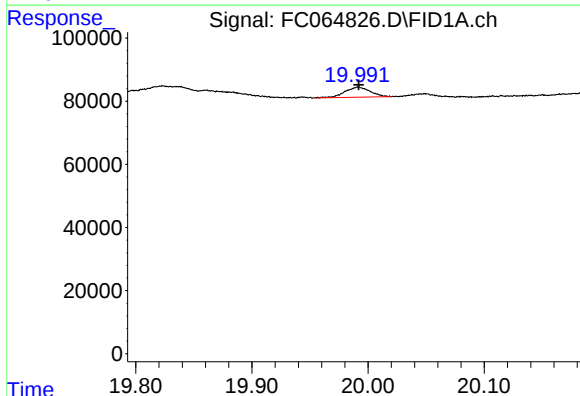


#20 n-Hexatriacontane (C36)

R.T.: 19.992 min
Delta R.T.: 0.000 min
Response: 47836
Conc: 0.35 ug/ml

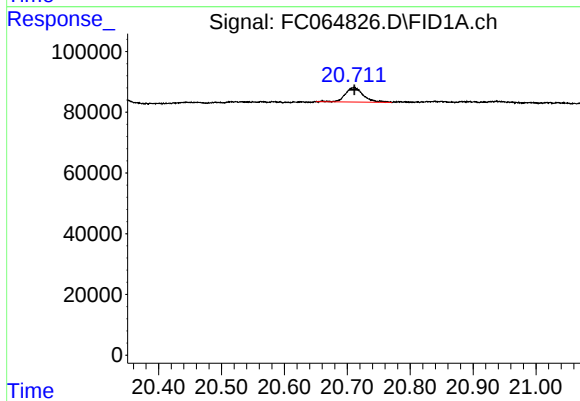

#21 n-Octatriacontane (C38)

R.T.: 20.711 min
Delta R.T.: 0.000 min
Response: 95803
Conc: 0.72 ug/ml

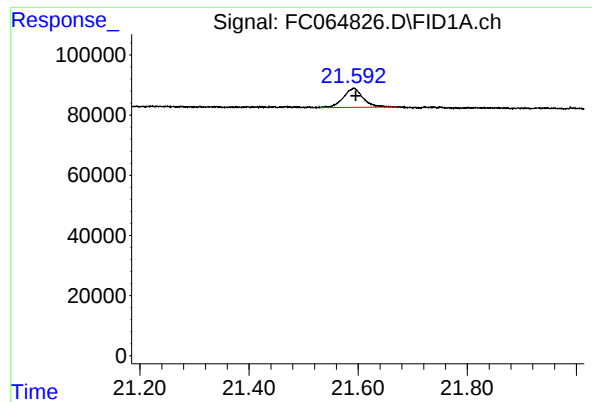

#22 n-Tetracontane (C40)

R.T.: 21.593 min
Delta R.T.: -0.003 min
Response: 158610
Conc: 1.27 ug/ml

Instrument :

FID_C

ClientSampleId :