

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101424AL\
Data File : FC067445.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2024 02:30
Operator : YP/AJ
Sample : P4396-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
WASTE-WATER-FRAC-TANK

Integration File: autoint1.e
Quant Time: Oct 15 04:34:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.939	3764572	33.258 ug/ml
Spiked Amount	50.000	Recovery	= 66.52%

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC101424AL\
Data File : FC067445.D
Signal(s) : FID1A.ch
Acq On : 15 Oct 2024 02:30
Operator : YP/AJ
Sample : P4396-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
WASTE-WATER-FRAC-TANK

Integration File: autoint1.e
Quant Time: Oct 15 04:34:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 100224.M
Quant Title : GC Extractables
QLast Update : Tue Oct 01 09:13:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

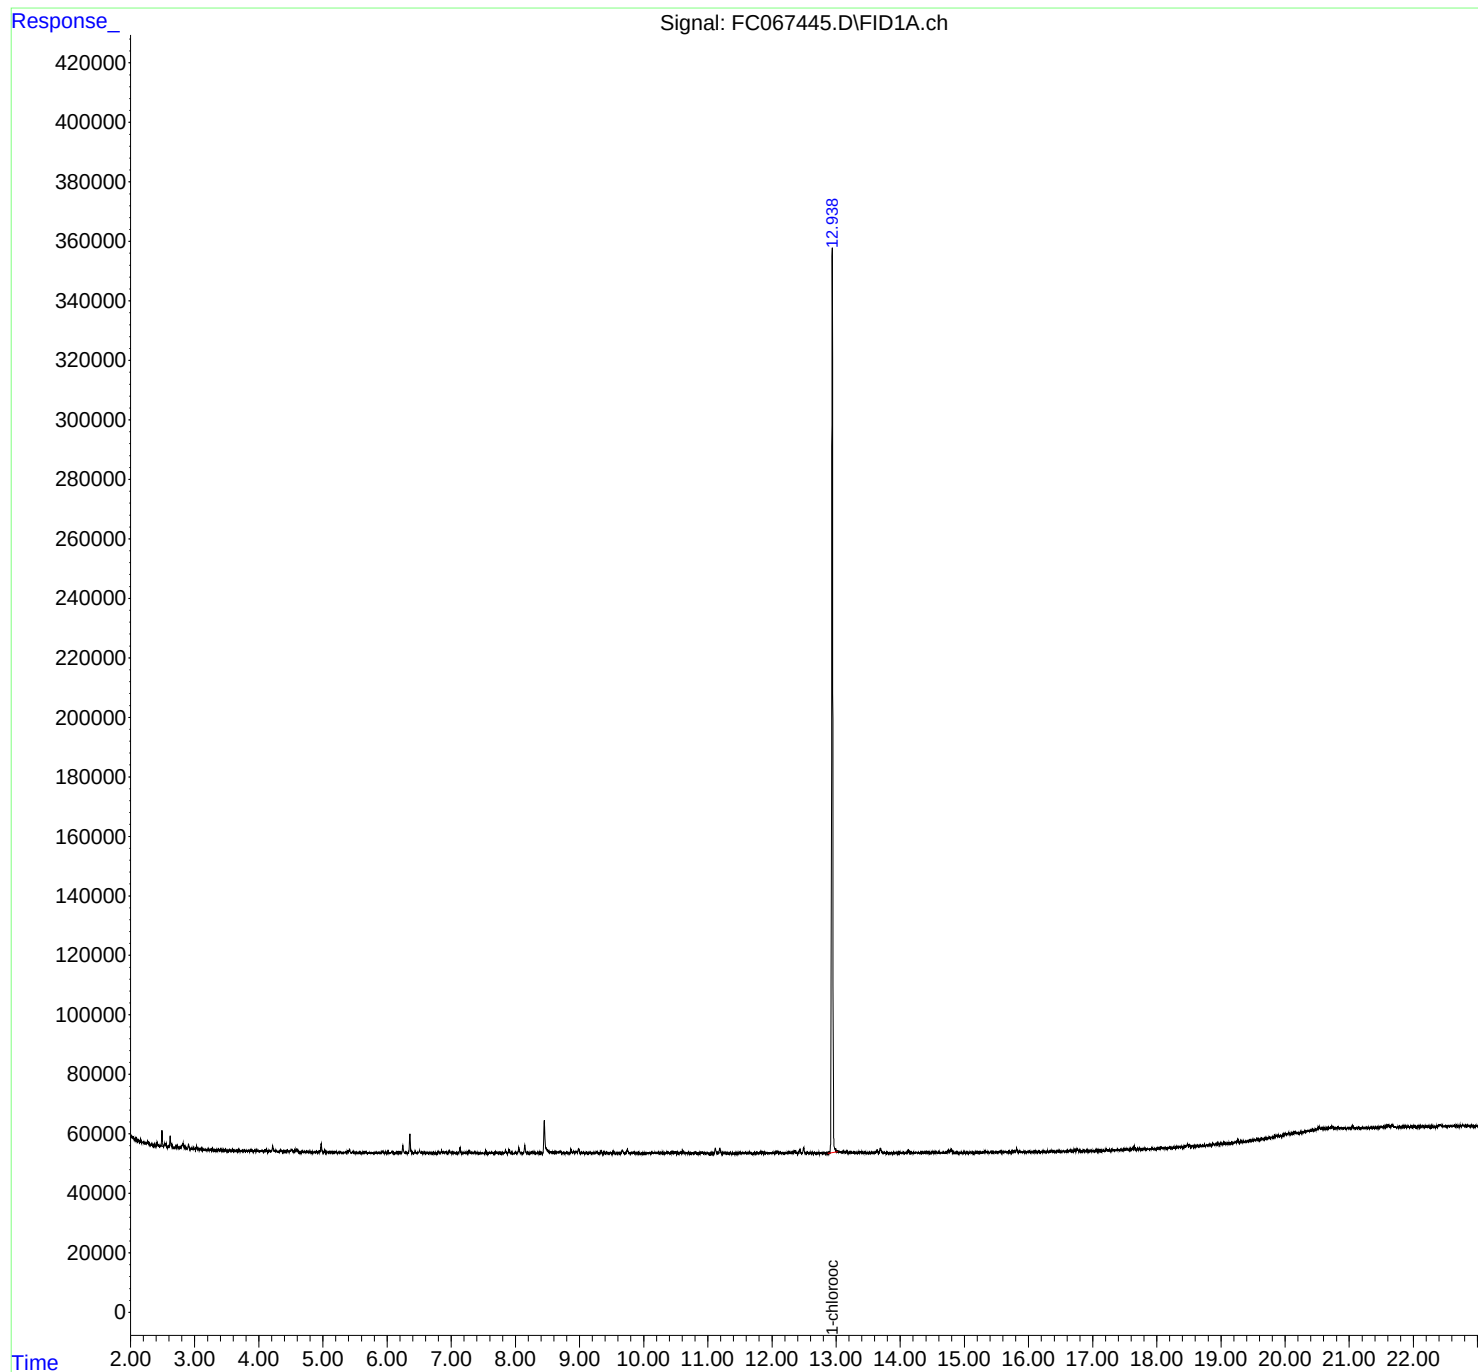


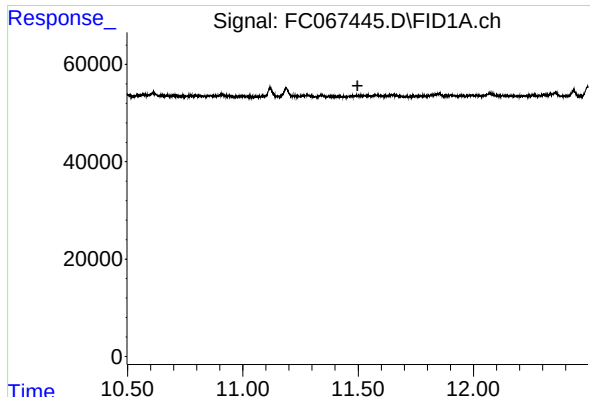

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.497 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
WASTE-WATER-FRAC-TANK

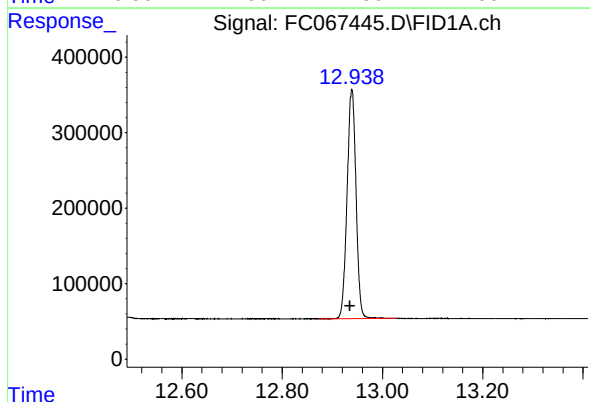

#12 1-chlorooctadecane (SURR)

R.T.: 12.939 min
Delta R.T.: 0.003 min
Response: 3764572
Conc: 33.26 ug/ml