

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC102224AL\  
Data File : FC067500.D  
Signal(s) : FID1A.ch  
Acq On : 23 Oct 2024 11:33  
Operator : YP/AJ  
Sample : P4456-01DL 50X  
Misc :  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
PAD-10182024DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 10/24/2024  
Supervised By :Ankita Jodhani 10/24/2024

Integration File: autoint1.e  
Quant Time: Oct 24 04:08:38 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 100224.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 01 09:13:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 12) S 1-chlorooctadecane (S... | 12.933 | 90718    | 0.801 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 1.60%      |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC102224AL\  
Data File : FC067500.D  
Signal(s) : FID1A.ch  
Acq On : 23 Oct 2024 11:33  
Operator : YP/AJ  
Sample : P4456-01DL 50X  
Misc :  
ALS Vial : 24 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
PAD-10182024DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 10/24/2024  
Supervised By :Ankita Jodhani 10/24/2024

Integration File: autoint1.e  
Quant Time: Oct 24 04:08:38 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 100224.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 01 09:13:32 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

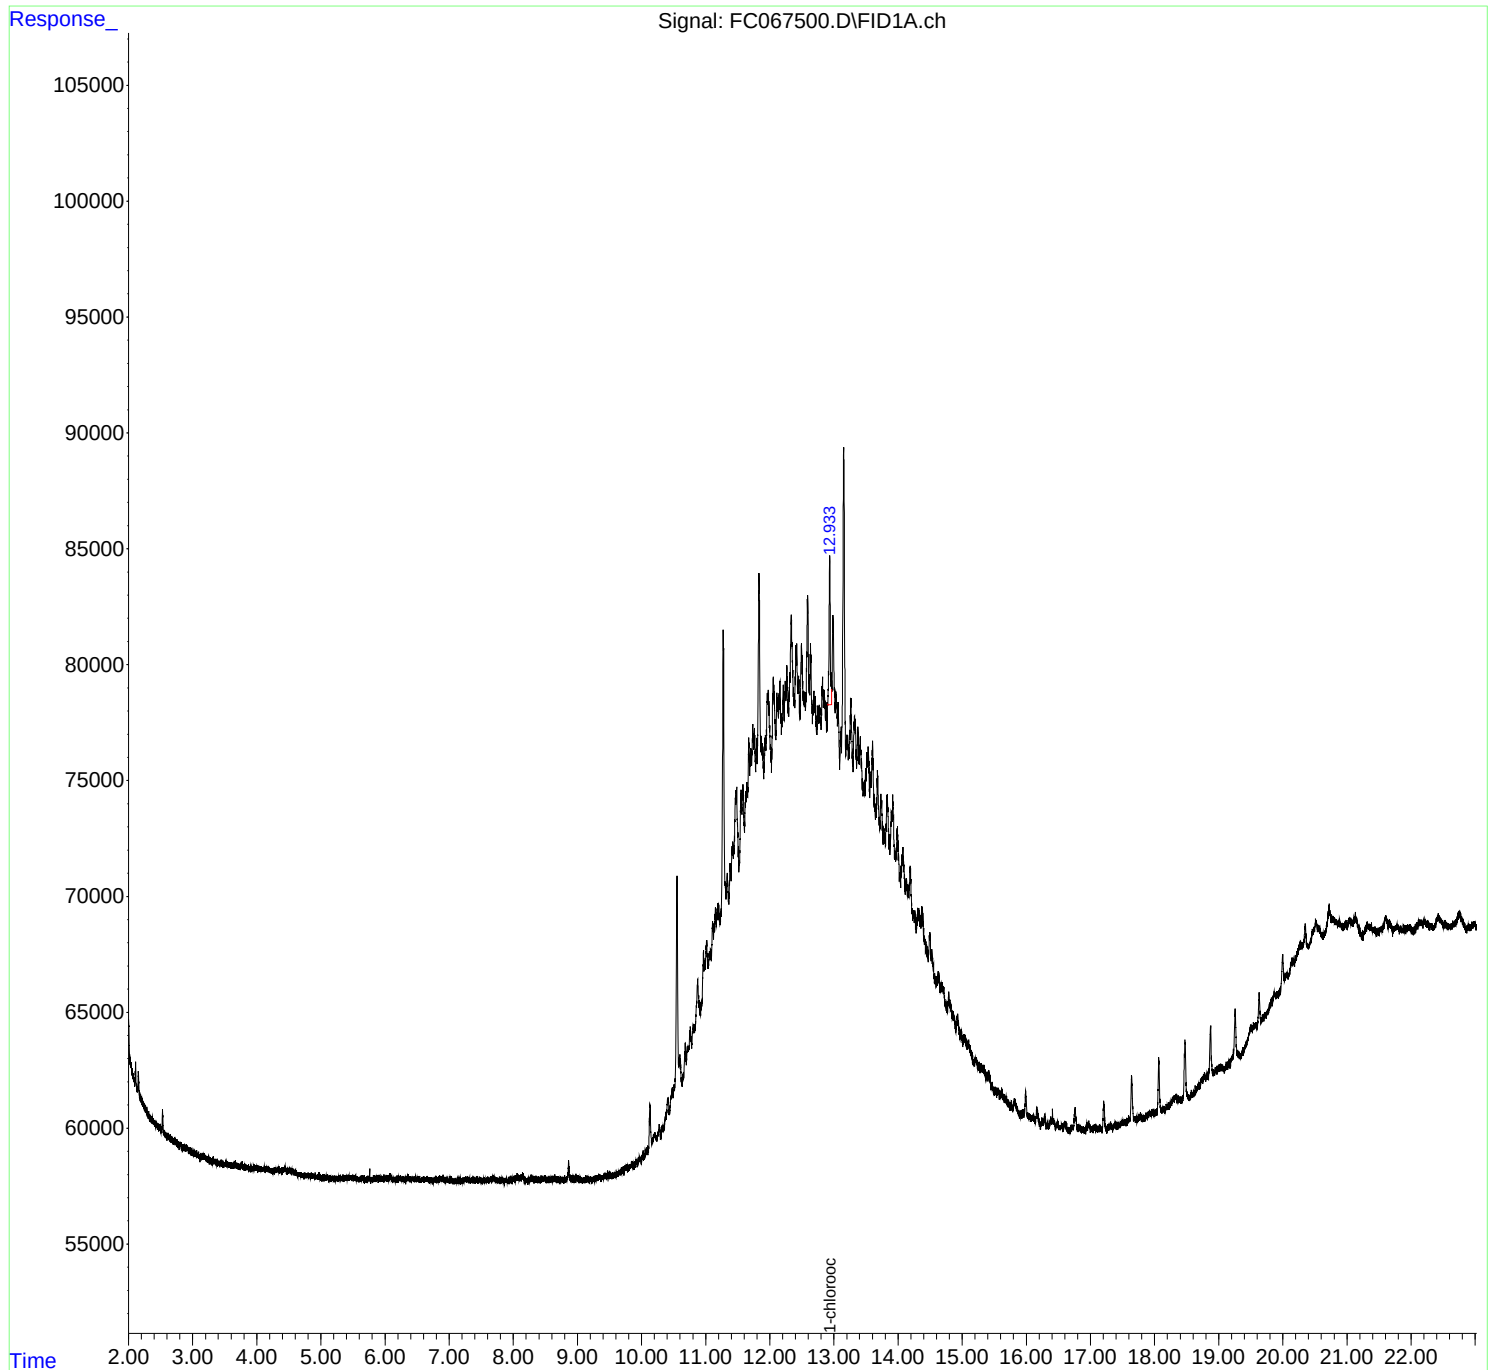

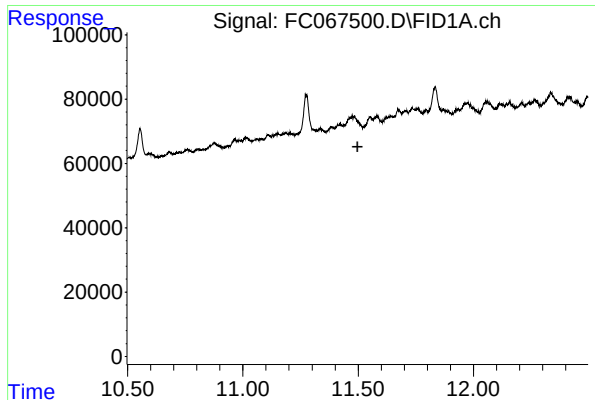


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.497 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :  
PAD-10182024DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 10/24/2024  
Supervised By :Ankita Jodhani 10/24/2024

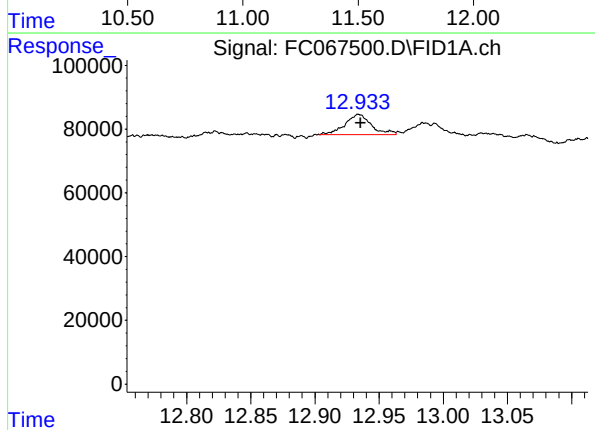

#12 1-chlorooctadecane (SURR)

R.T.: 12.933 min  
Delta R.T.: -0.003 min  
Response: 90718  
Conc: 0.80 ug/ml m