

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102320AL\
 Data File : FC050314.D
 Signal(s) : FID1A.CH
 Acq On : 23 Oct 2020 12:50
 Operator : DD\AJ
 Sample : PB132447BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 24 02:23:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 100620.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 07 04:53:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.062	3384530	39.071 ug/ml
Spiked Amount 50.000		Recovery =	78.14%
Target Compounds			
14) T n-Tetracosane (C24)	14.913	128734	1.239 ug/ml
15) T n-Hexacosane (C26)	15.934	155836	1.512 ug/ml
16) T n-Octacosane (C28)	16.882	203595	1.967 ug/ml
17) T n-Tricontane (C30)	17.769	235650	2.309 ug/ml
18) T n-Dotriacontane (C32)	18.600	195962	2.040 ug/ml
19) T n-Tetratriacontane (C34)	19.382	126565	1.380 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102320AL\
Data File : FC050314.D
Signal(s) : FID1A.CH
Acq On : 23 Oct 2020 12:50
Operator : DD\AJ
Sample : PB132447BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 24 02:23:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 100620.M
Quant Title : GC Extractables
QLast Update : Wed Oct 07 04:53:04 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

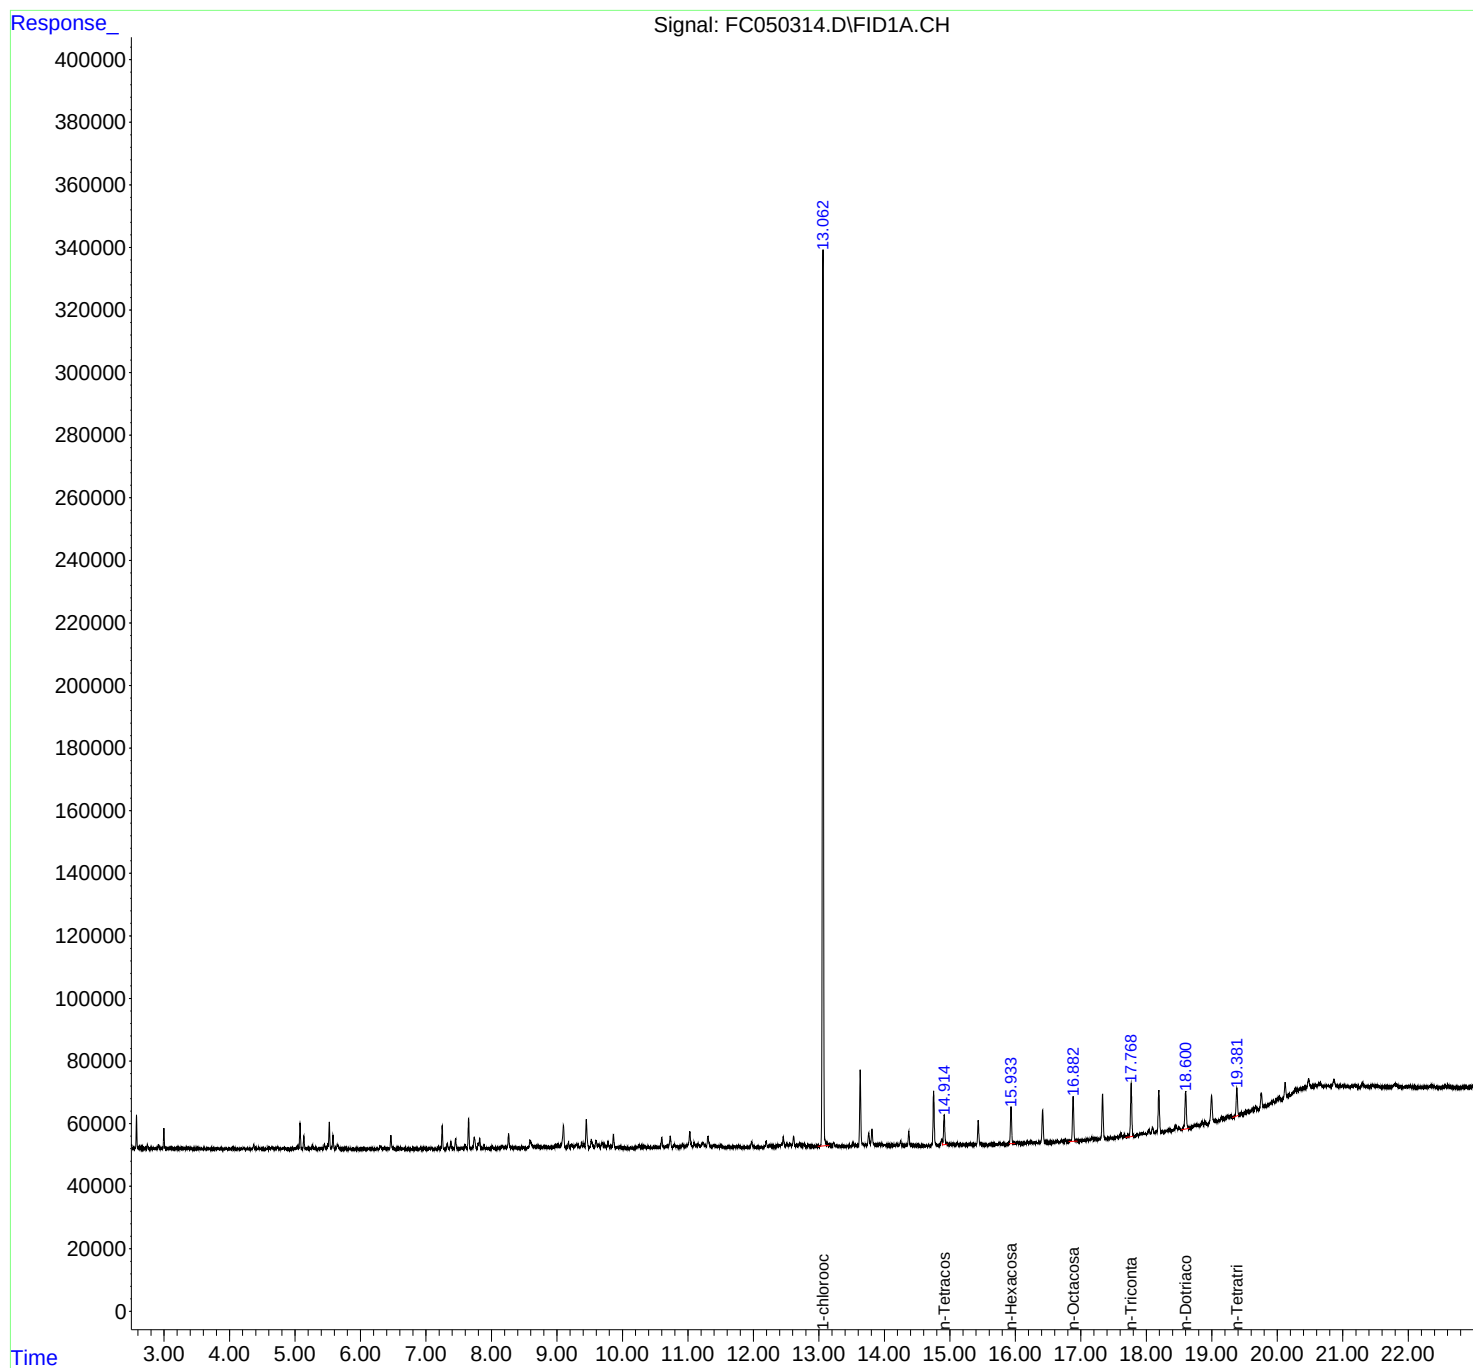


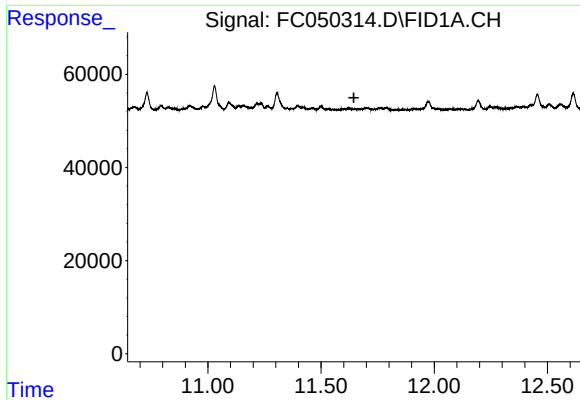

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.645 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

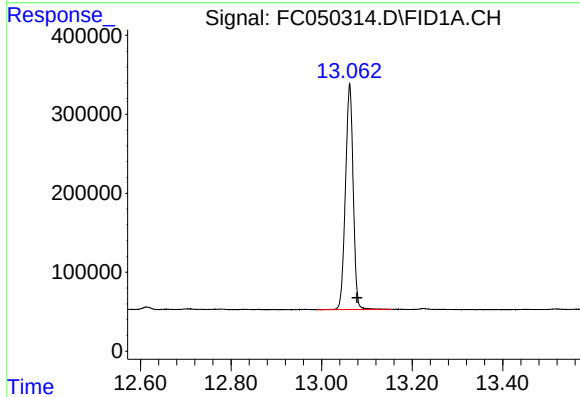


#12 1-chlorooctadecane (SURR)

R.T.: 13.062 min
Delta R.T.: -0.016 min
Response: 3384530
Conc: 39.07 ug/ml

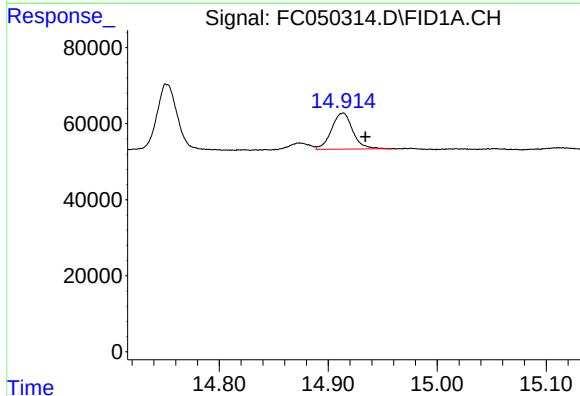


#14 n-Tetracosane (C24)

R.T.: 14.913 min
Delta R.T.: -0.021 min
Response: 128734
Conc: 1.24 ug/ml

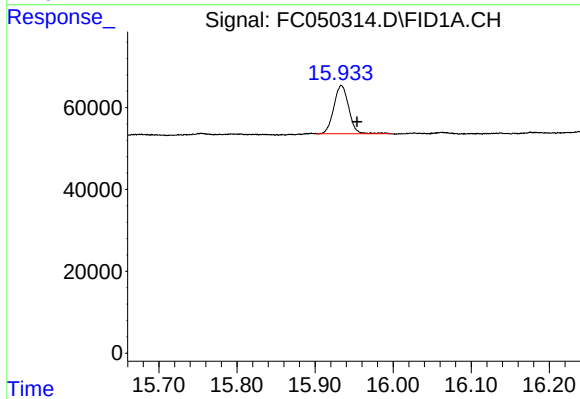

#15 n-Hexacosane (C26)


R.T.: 15.934 min
Delta R.T.: -0.020 min
Response: 155836
Conc: 1.51 ug/ml

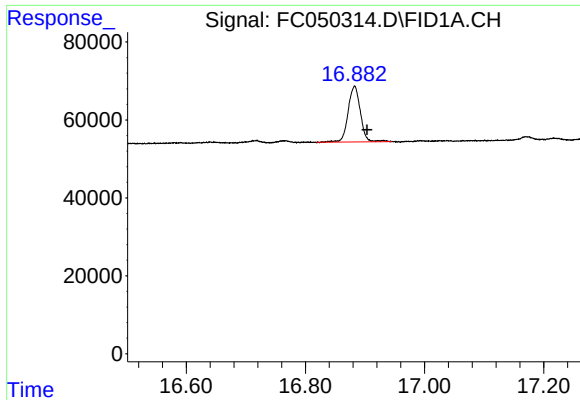

#16 n-Octacosane (C28)


R.T.: 16.882 min
Delta R.T.: -0.021 min
Response: 203595
Conc: 1.97 ug/ml

Instrument :
FID_C
ClientSampleId :

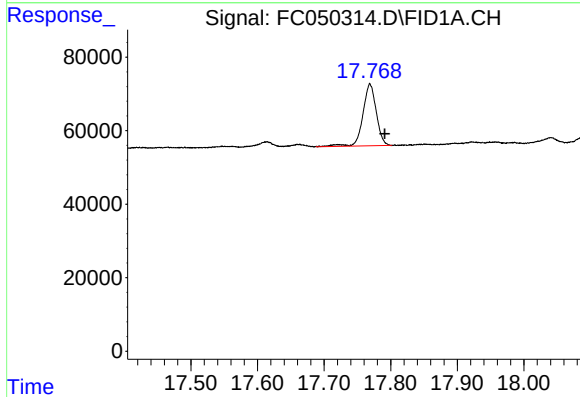


#17 n-Tricontane (C30)

R.T.: 17.769 min
Delta R.T.: -0.022 min
Response: 235650
Conc: 2.31 ug/ml

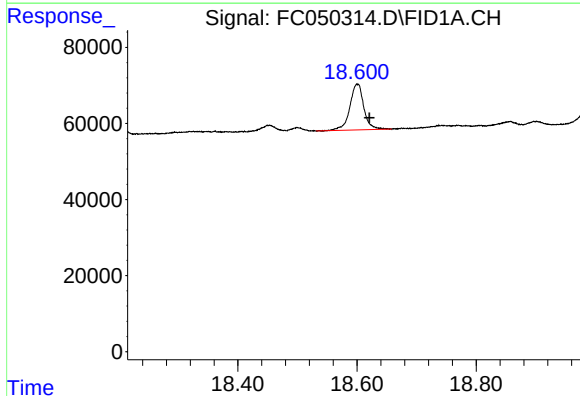

#18 n-Dotriacontane (C32)

R.T.: 18.600 min
Delta R.T.: -0.020 min
Response: 195962
Conc: 2.04 ug/ml

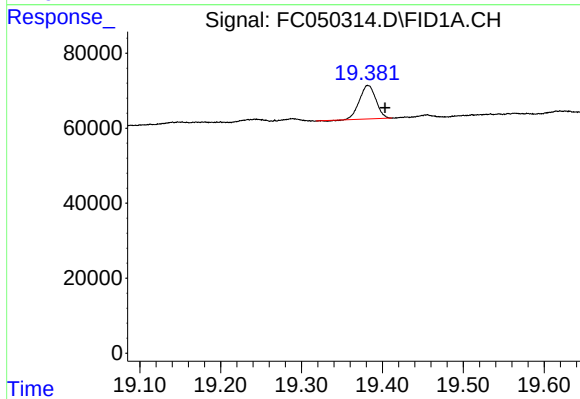

#19 n-Tetratriacontane (C34)

R.T.: 19.382 min
Delta R.T.: -0.021 min
Response: 126565
Conc: 1.38 ug/ml