

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102320AL\
 Data File : FC050315.D
 Signal(s) : FID1A.CH
 Acq On : 23 Oct 2020 13:27
 Operator : DD\AJ
 Sample : PB132448BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 24 02:24:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 100620.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 07 04:53:04 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.061	3362792	38.820 ug/ml
Spiked Amount 50.000		Recovery =	77.64%
Target Compounds			
14) T n-Tetracosane (C24)	14.913	127979	1.232 ug/ml
15) T n-Hexacosane (C26)	15.934	159739	1.550 ug/ml
16) T n-Octacosane (C28)	16.882	216711	2.094 ug/ml
17) T n-Tricontane (C30)	17.769	250038	2.450 ug/ml
18) T n-Dotriacontane (C32)	18.600	210958	2.196 ug/ml
19) T n-Tetratriacontane (C34)	19.382	143325	1.563 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102320AL\
Data File : FC050315.D
Signal(s) : FID1A.CH
Acq On : 23 Oct 2020 13:27
Operator : DD\AJ
Sample : PB132448BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 24 02:24:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Alaphatic EPH 100620.M
Quant Title : GC Extractables
QLast Update : Wed Oct 07 04:53:04 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

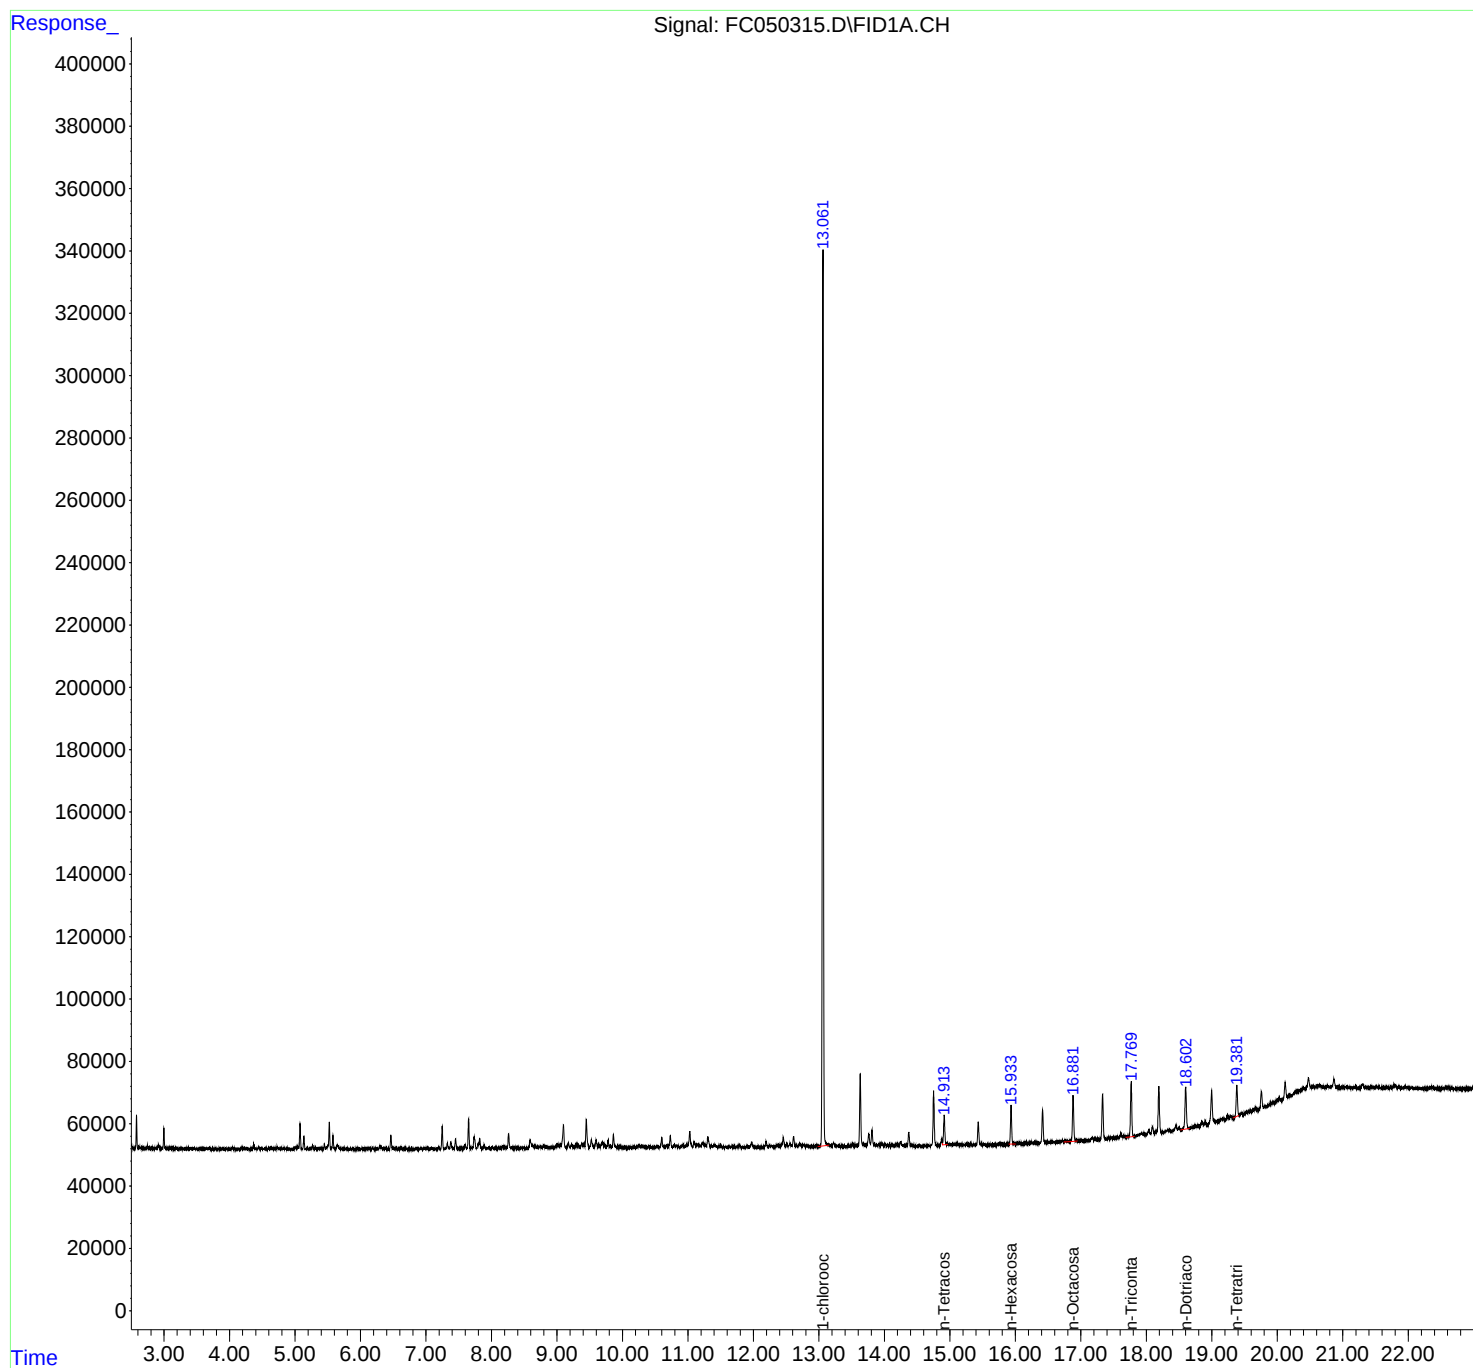


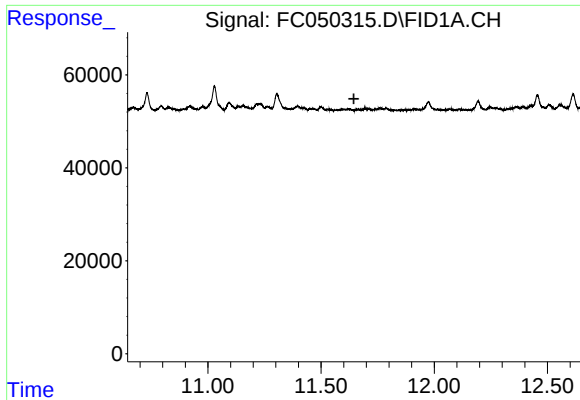

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.645 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

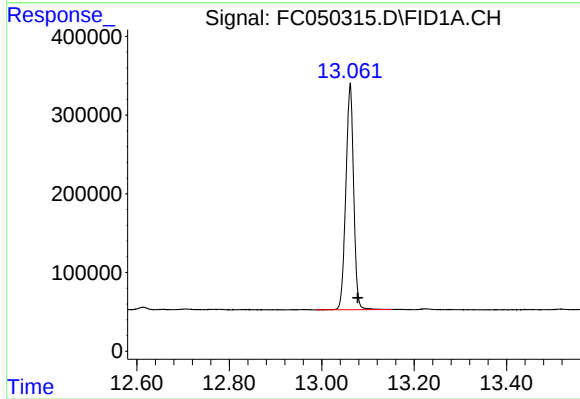


#12 1-chlorooctadecane (SURR)

R.T.: 13.061 min
Delta R.T.: -0.017 min
Response: 3362792
Conc: 38.82 ug/ml

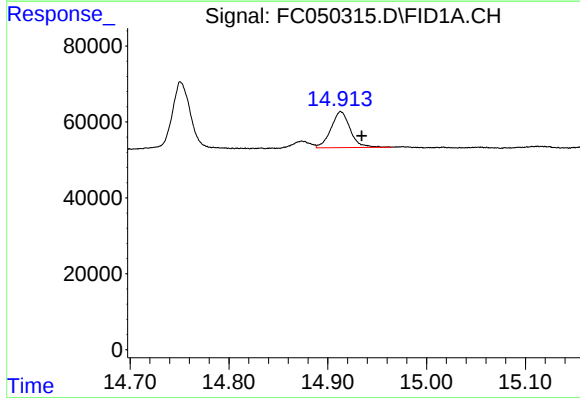


#14 n-Tetracosane (C24)

R.T.: 14.913 min
Delta R.T.: -0.021 min
Response: 127979
Conc: 1.23 ug/ml

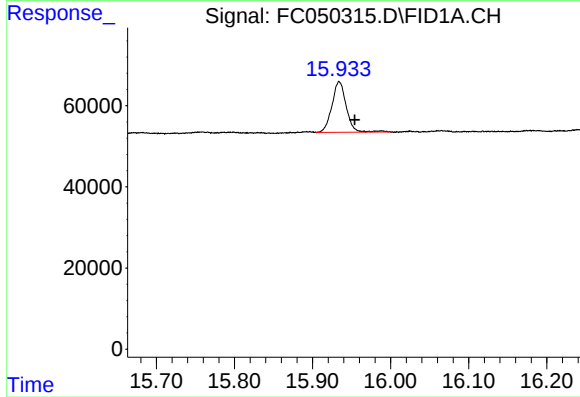

#15 n-Hexacosane (C26)


R.T.: 15.934 min
Delta R.T.: -0.020 min
Response: 159739
Conc: 1.55 ug/ml

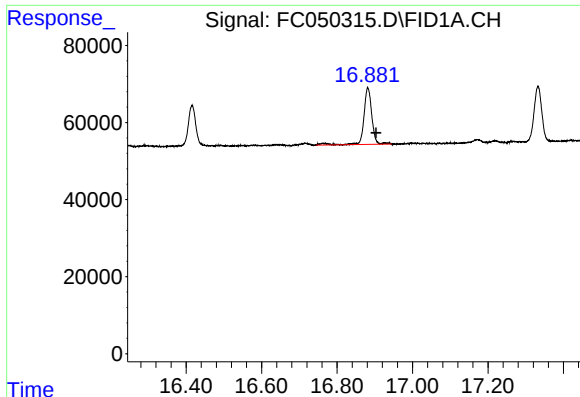

#16 n-Octacosane (C28)


R.T.: 16.882 min
Delta R.T.: -0.022 min
Response: 216711
Conc: 2.09 ug/ml

Instrument :
FID_C
ClientSampleId :

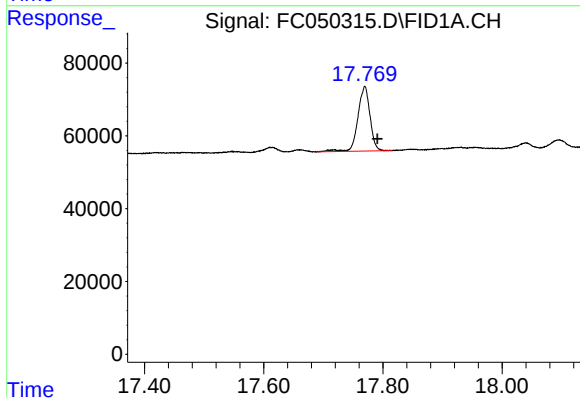


#17 n-Tricontane (C30)

R.T.: 17.769 min
Delta R.T.: -0.022 min
Response: 250038
Conc: 2.45 ug/ml

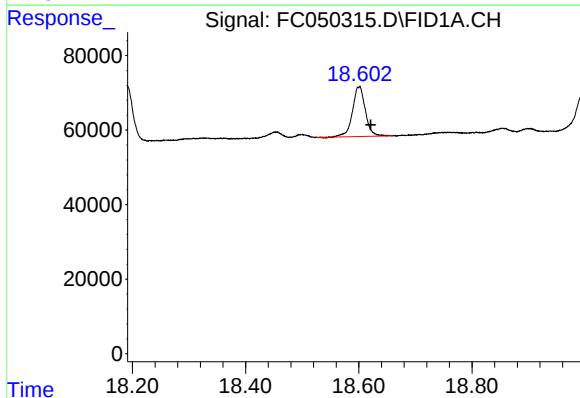

#18 n-Dotriacontane (C32)

R.T.: 18.600 min
Delta R.T.: -0.021 min
Response: 210958
Conc: 2.20 ug/ml

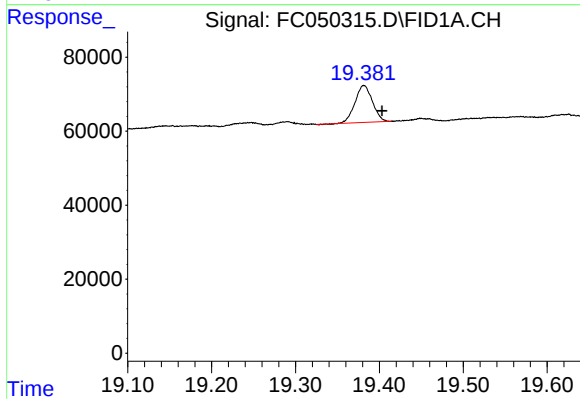

#19 n-Tetratriacontane (C34)

R.T.: 19.382 min
Delta R.T.: -0.022 min
Response: 143325
Conc: 1.56 ug/ml