

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC102325AL\  
Data File : FC070010.D  
Signal(s) : FID1A.ch  
Acq On : 23 Oct 2025 08:07  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 24 01:30:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 100725.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 07 09:35:40 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|       |                          |        |       |             |
|-------|--------------------------|--------|-------|-------------|
| 17) T | n-Tricontane (C30)       | 17.796 | 45724 | 0.335 ug/ml |
| 18) T | n-Dotriacontane (C32)    | 18.631 | 77980 | 0.605 ug/ml |
| 19) T | n-Tetratriacontane (C34) | 19.416 | 63805 | 0.559 ug/ml |
| 20) T | n-Hexatriacontane (C36)  | 20.155 | 61680 | 0.638 ug/ml |

-----  
(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC102325AL\  
Data File : FC070010.D  
Signal(s) : FID1A.ch  
Acq On : 23 Oct 2025 08:07  
Operator : YP/AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Oct 24 01:30:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 100725.M  
Quant Title : GC Extractables  
QLast Update : Tue Oct 07 09:35:40 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

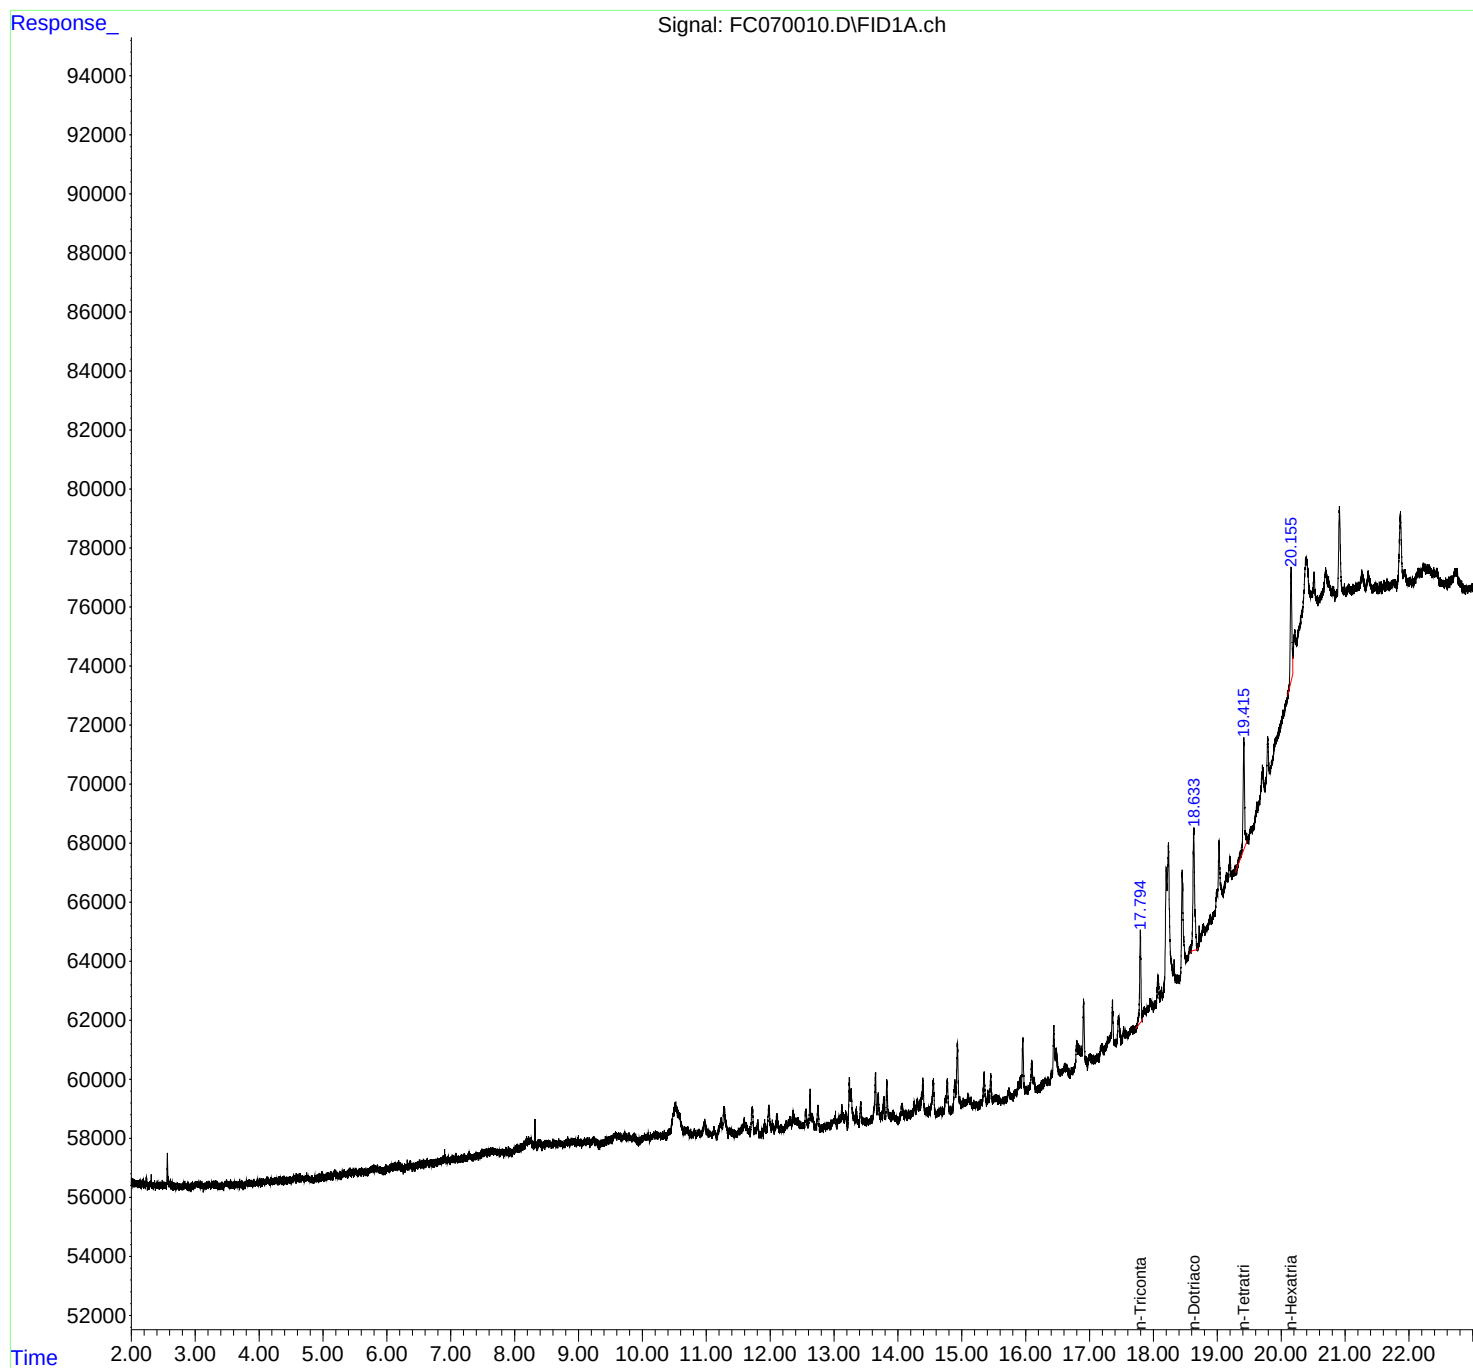


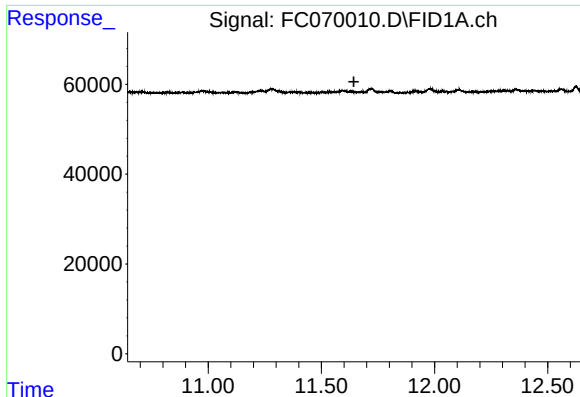

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 11.644 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_C  
ClientSampleId :

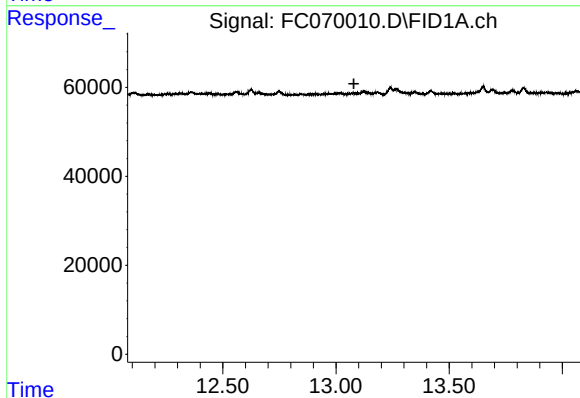


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T.: 13.079 min  
Response: 0  
Conc: N.D.

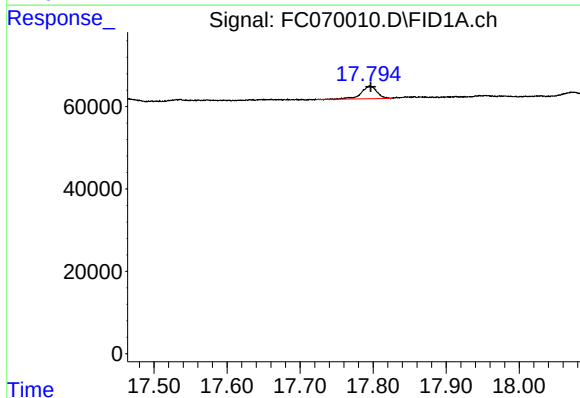


#17 n-Tricontane (C30)

R.T.: 17.796 min  
Delta R.T.: -0.001 min  
Response: 45724  
Conc: 0.33 ug/ml

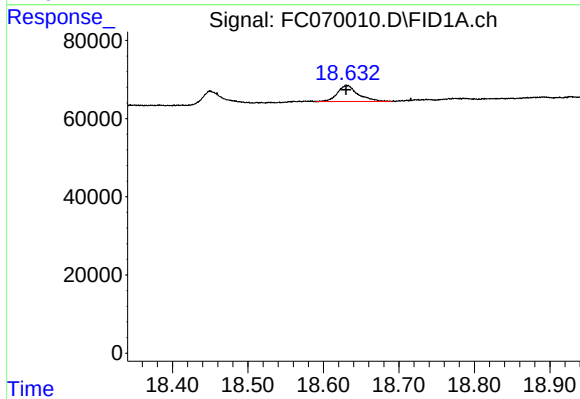

#18 n-Dotriacontane (C32)


R.T.: 18.631 min  
Delta R.T.: 0.001 min  
Response: 77980  
Conc: 0.60 ug/ml

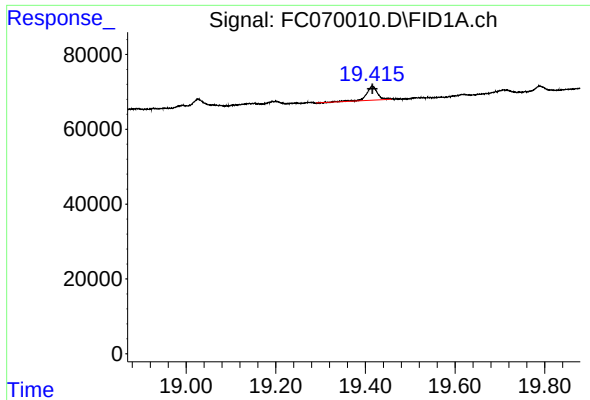

#19 n-Tetratriacontane (C34)

R.T.: 19.416 min  
Delta R.T.: 0.000 min  
Response: 63805  
Conc: 0.56 ug/ml

Instrument :  
FID\_C  
ClientSampleId :

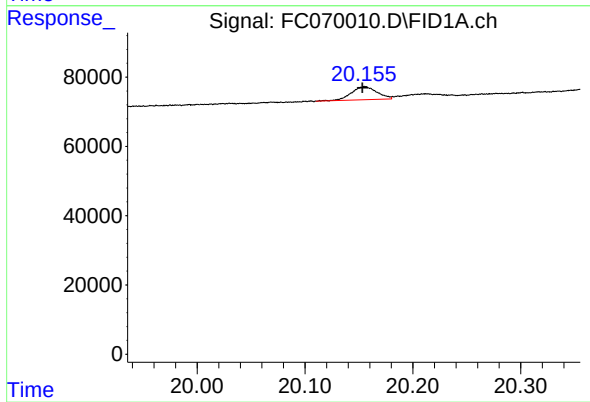

#20 n-Hexatriacontane (C36)

R.T.: 20.155 min  
Delta R.T.: 0.002 min  
Response: 61680  
Conc: 0.64 ug/ml