

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102422AL\
 Data File : FC061877.D
 Signal(s) : FID1A.ch
 Acq On : 24 Oct 2022 09:05
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 25 04:41:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101722.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 17 23:26:31 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.574	146437	1.038 ug/ml
11) T	n-Heneicosane (C21)	13.186	321512	2.317 ug/ml
13) T	n-Docosane (C22)	13.769	226771	1.654 ug/ml
14) T	n-Tetracosane (C24)	14.872	115261	0.872 ug/ml
15) T	n-Hexacosane (C26)	15.894	118426	0.940 ug/ml
16) T	n-Octacosane (C28)	16.844	135328	1.122 ug/ml
17) T	n-Tricontane (C30)	17.732	192608	1.619 ug/ml
18) T	n-Dotriacontane (C32)	18.564	266199	2.259 ug/ml
19) T	n-Tetratriacontane (C34)	19.347	204503	1.810 ug/ml
20) T	n-Hexatriacontane (C36)	20.087	147592	1.301 ug/ml
21) T	n-Octatriacontane (C38)	20.822	106943	0.950 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102422AL\
Data File : FC061877.D
Signal(s) : FID1A.ch
Acq On : 24 Oct 2022 09:05
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 04:41:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101722.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 23:26:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

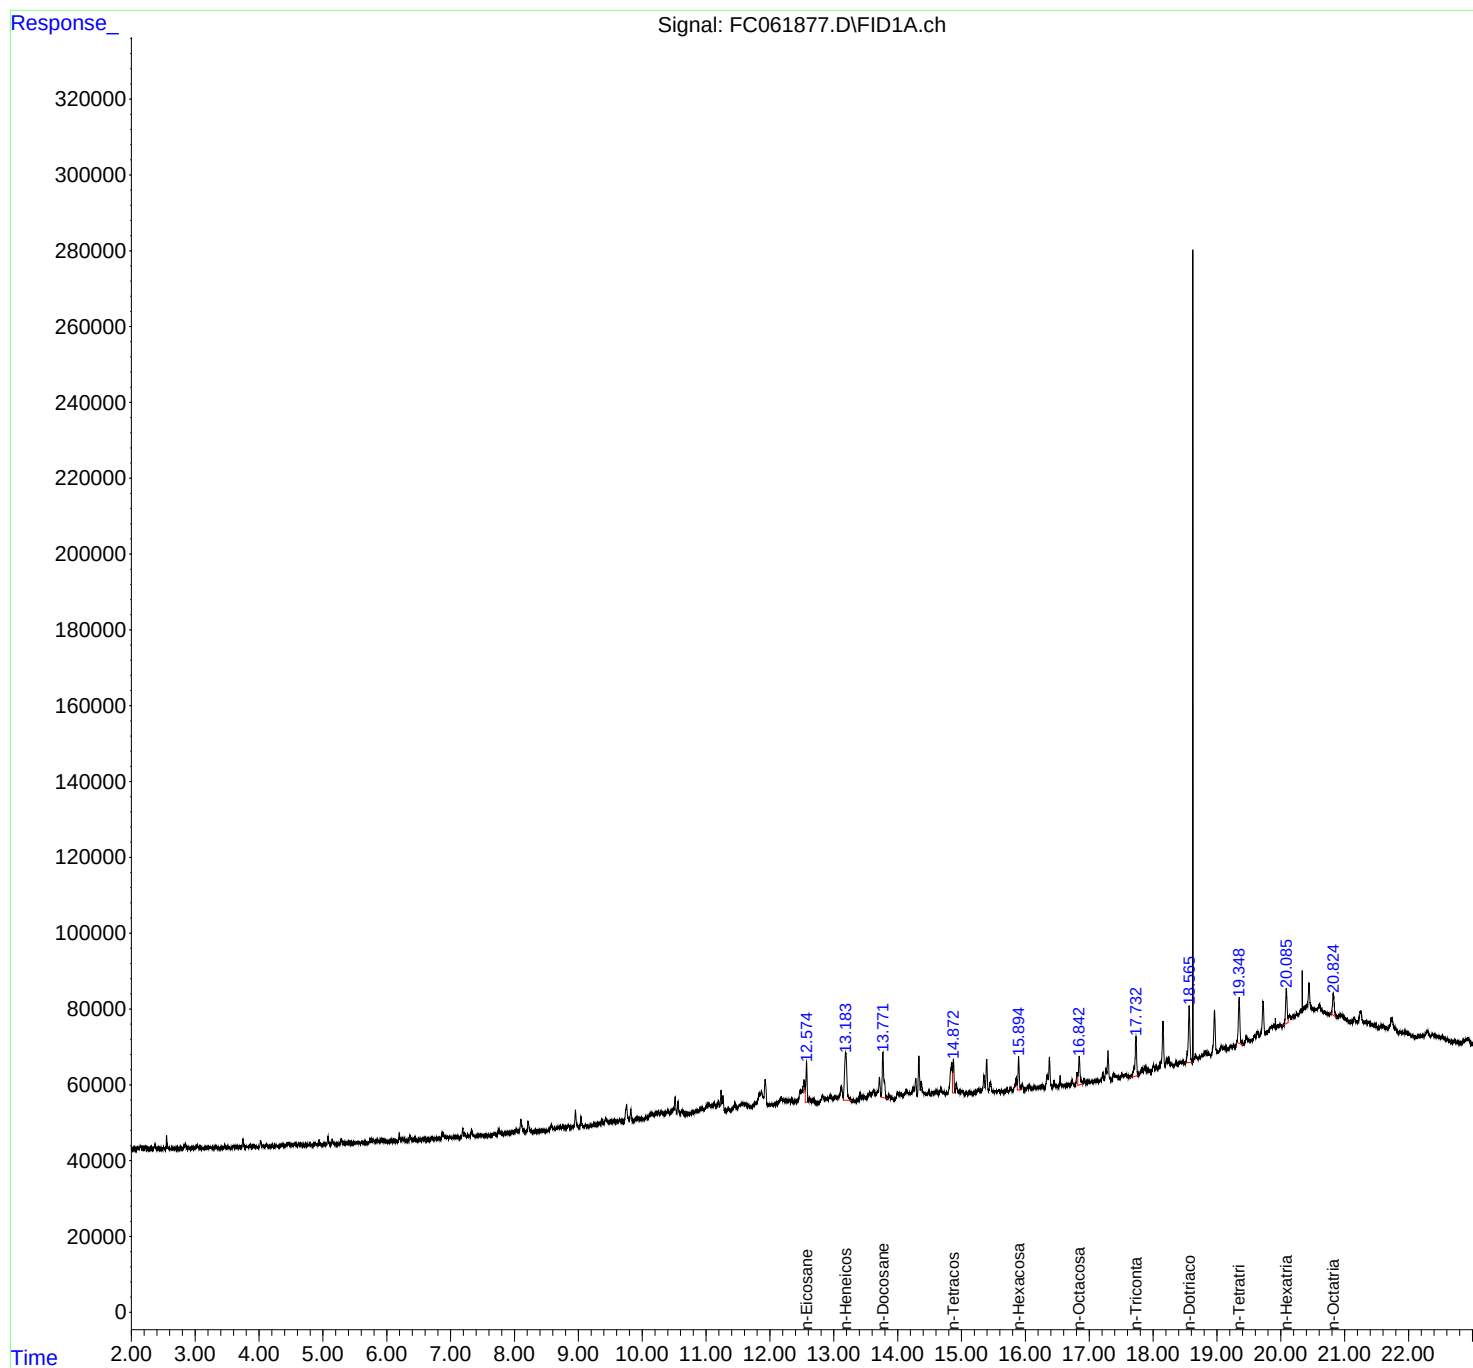


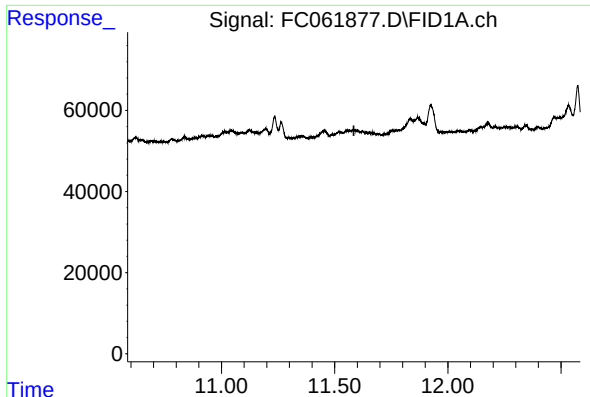

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.585 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

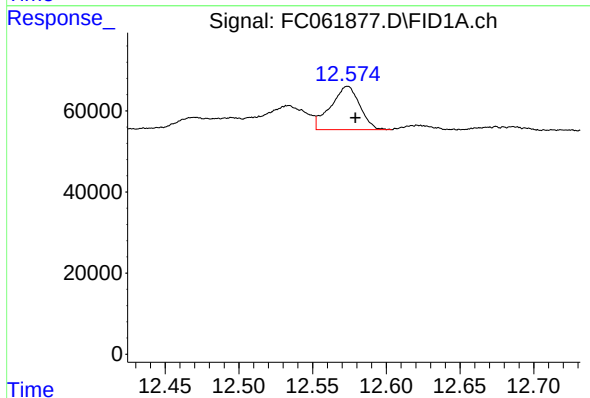


#10 n-Eicosane (C20)

R.T.: 12.574 min
Delta R.T.: -0.005 min
Response: 146437
Conc: 1.04 ug/ml

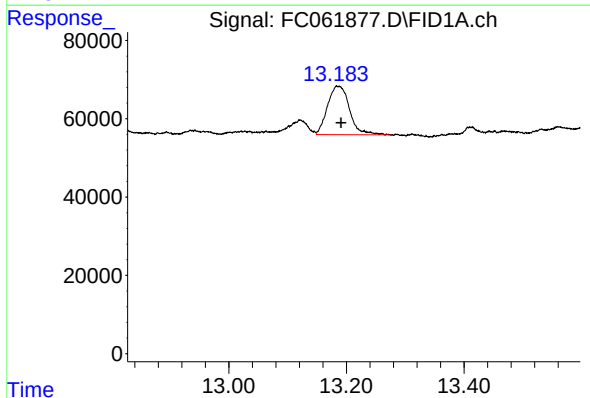


#11 n-Heneicosane (C21)

R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 321512
Conc: 2.32 ug/ml

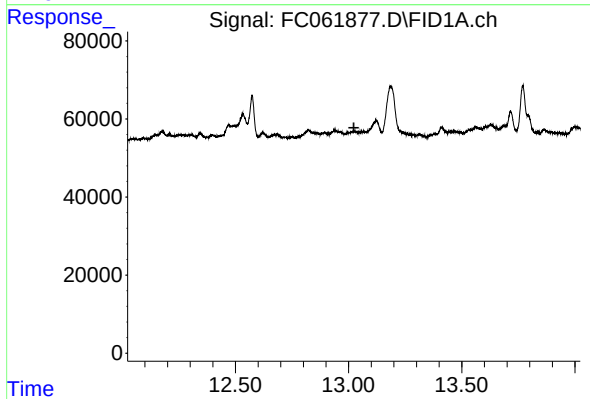

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.023 min
Response: 0
Conc: N.D.

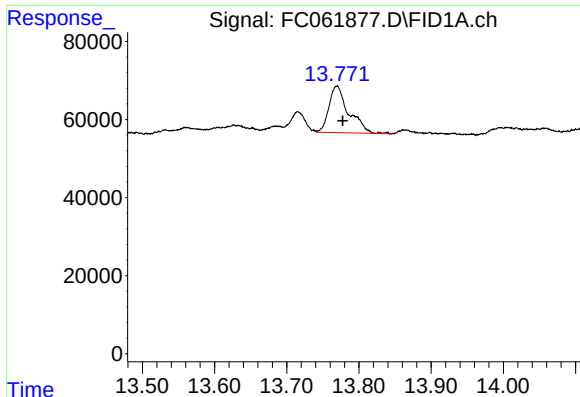

#13 n-Docosane (C22)


R.T.: 13.769 min
Delta R.T.: -0.008 min
Response: 226771
Conc: 1.65 ug/ml

Instrument :
FID_C
ClientSampleId :

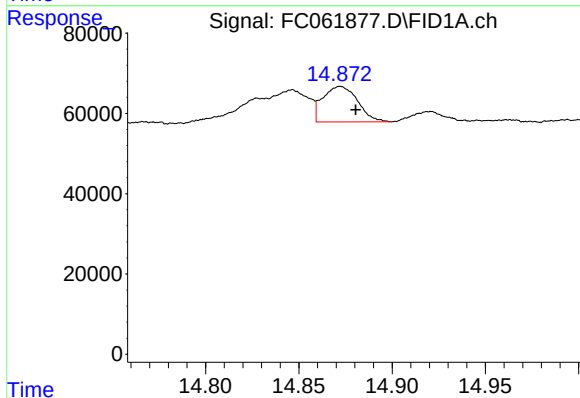


#14 n-Tetracosane (C24)

R.T.: 14.872 min
Delta R.T.: -0.008 min
Response: 115261
Conc: 0.87 ug/ml

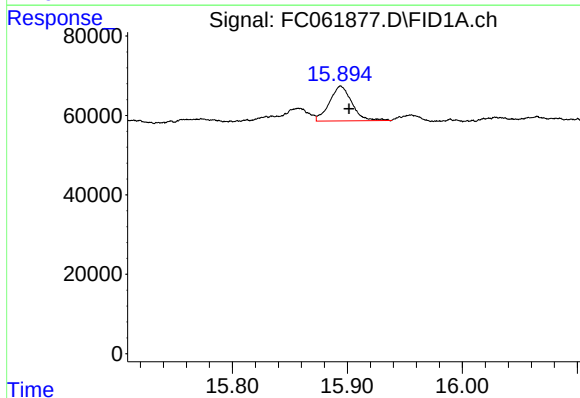


#15 n-Hexacosane (C26)

R.T.: 15.894 min
Delta R.T.: -0.007 min
Response: 118426
Conc: 0.94 ug/ml

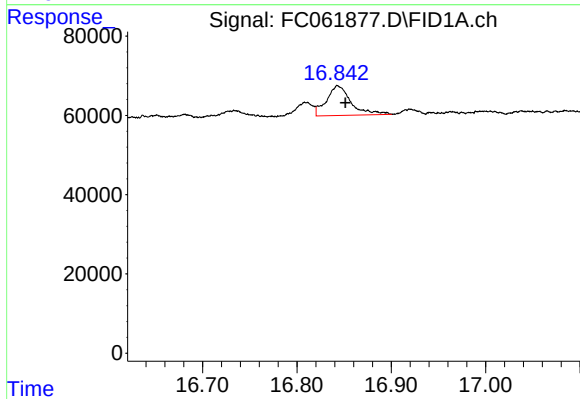

#16 n-Octacosane (C28)


R.T.: 16.844 min
Delta R.T.: -0.007 min
Response: 135328
Conc: 1.12 ug/ml

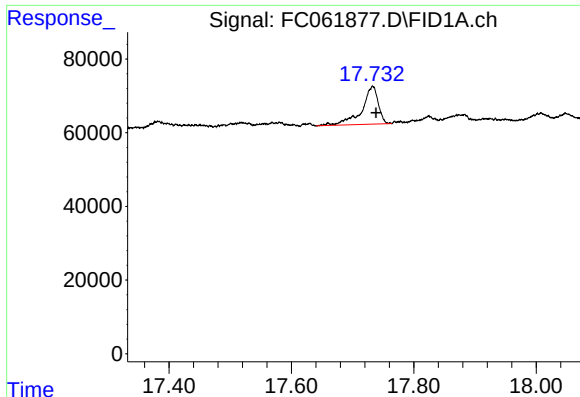

#17 n-Tricontane (C30)


R.T.: 17.732 min
Delta R.T.: -0.006 min
Response: 192608
Conc: 1.62 ug/ml

Instrument :
FID_C
ClientSampleId :

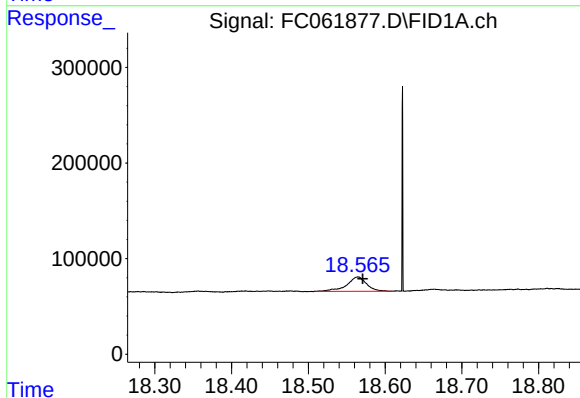


#18 n-Dotriacontane (C32)

R.T.: 18.564 min
Delta R.T.: -0.007 min
Response: 266199
Conc: 2.26 ug/ml

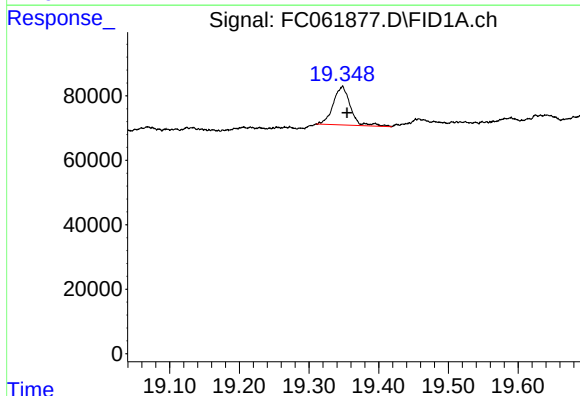


#19 n-Tetratriacontane (C34)

R.T.: 19.347 min
Delta R.T.: -0.007 min
Response: 204503
Conc: 1.81 ug/ml

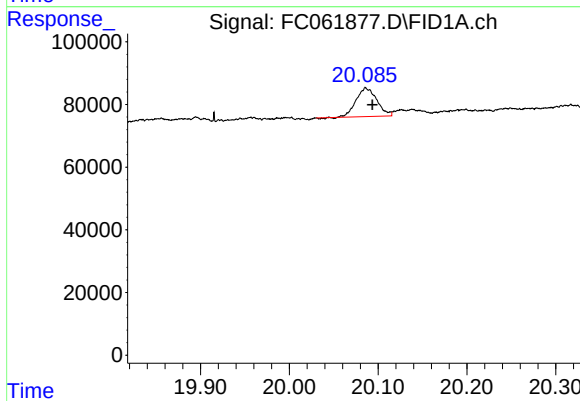

#20 n-Hexatriacontane (C36)

R.T.: 20.087 min
Delta R.T.: -0.007 min
Response: 147592
Conc: 1.30 ug/ml

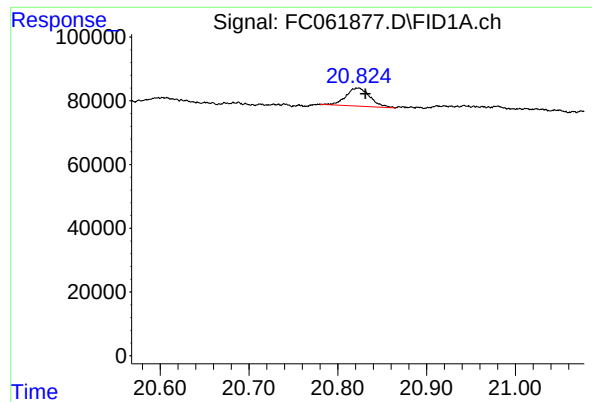

#21 n-Octatriacontane (C38)

R.T.: 20.822 min
Delta R.T.: -0.009 min
Response: 106943
Conc: 0.95 ug/ml

Instrument :

FID_C

ClientSampleId :