

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102422AL\
Data File : FC061898.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 01:01
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 04:43:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101722.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 23:26:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	17.730	58180	0.489 ug/ml
18) T	n-Dotriacontane (C32)	18.563	80133	0.680 ug/ml
19) T	n-Tetratriacontane (C34)	19.345	63370	0.561 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102422AL\
Data File : FC061898.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2022 01:01
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 04:43:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101722.M
Quant Title : GC Extractables
QLast Update : Mon Oct 17 23:26:31 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

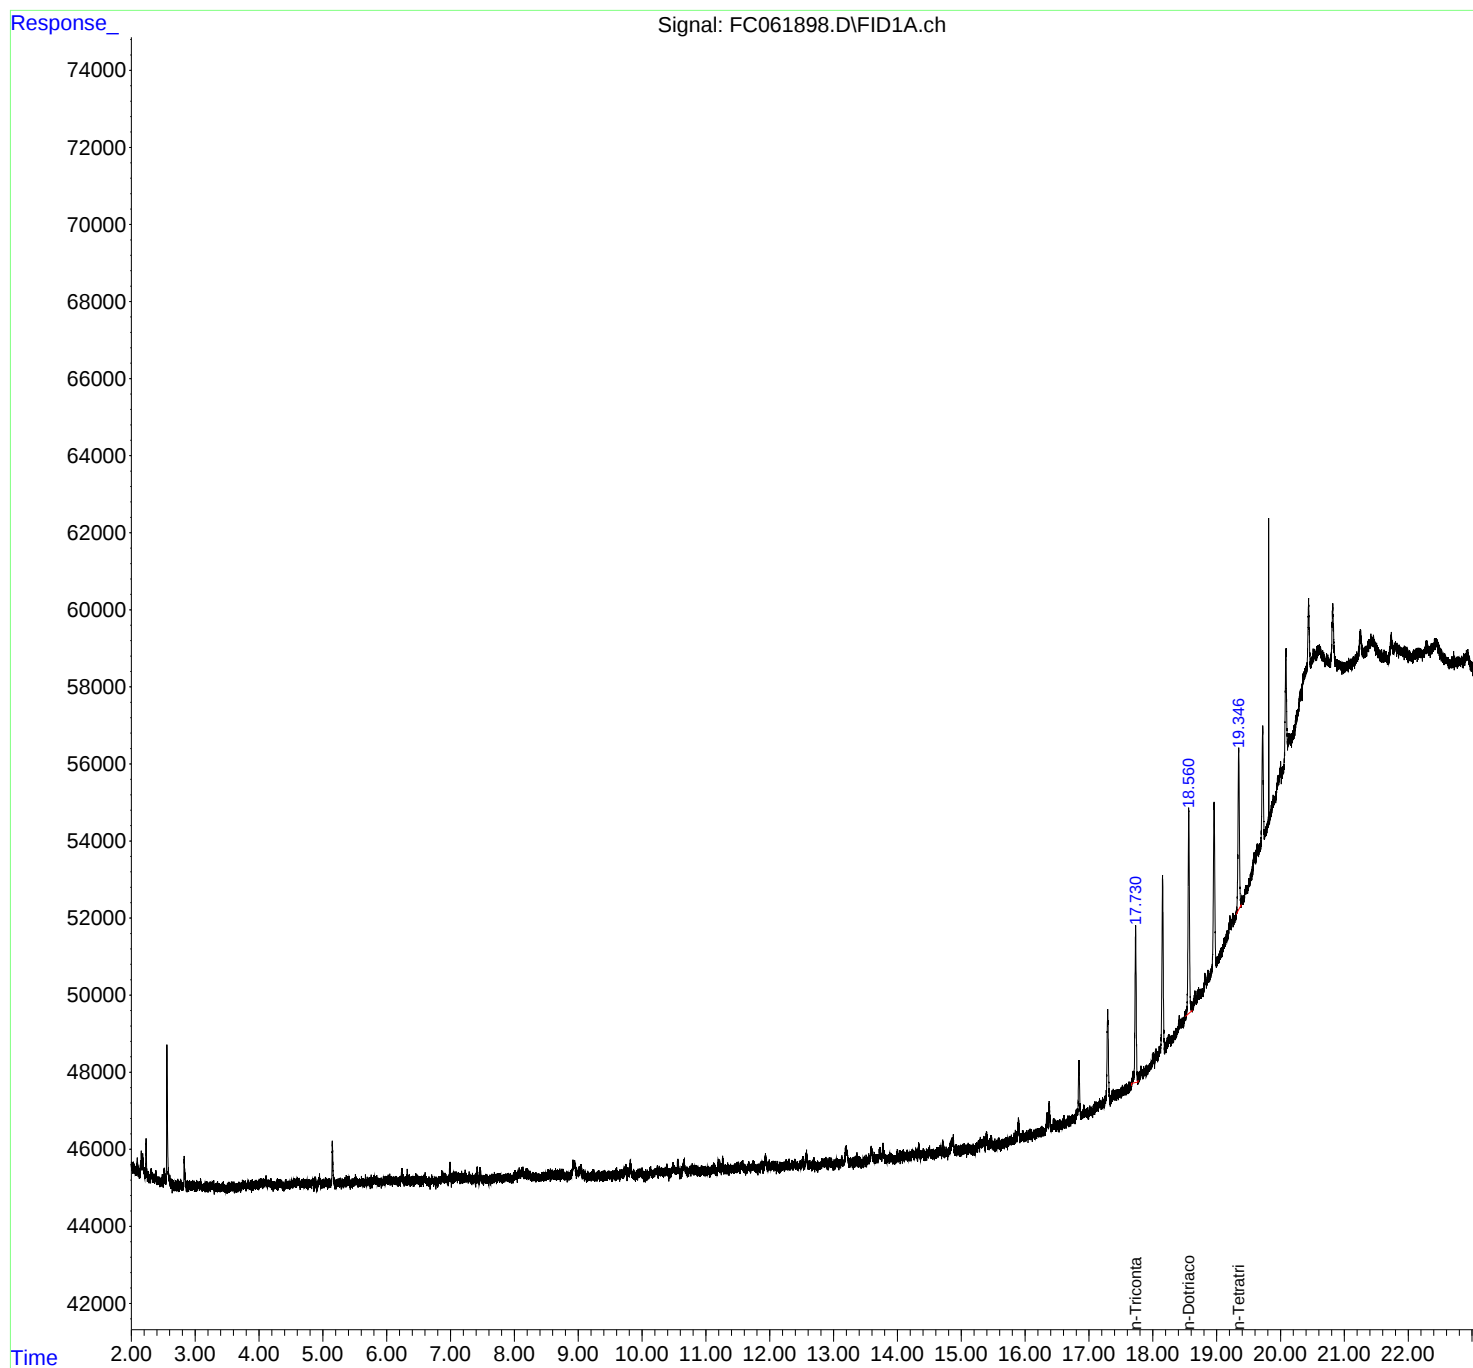


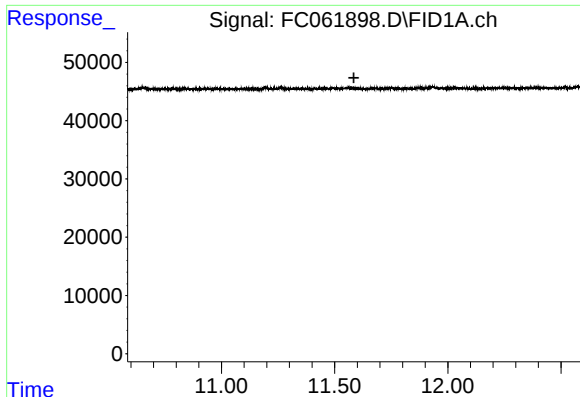

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.585 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

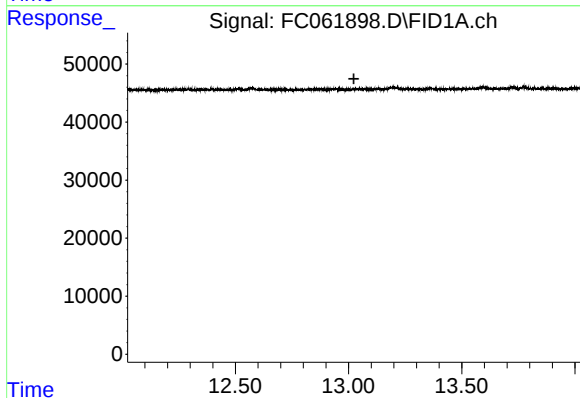


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.023 min
Response: 0
Conc: N.D.

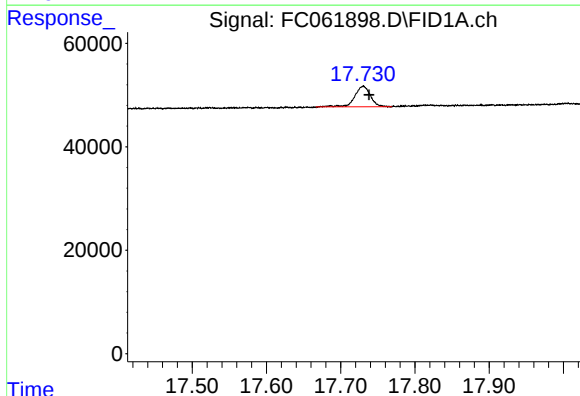


#17 n-Tricontane (C30)

R.T.: 17.730 min
Delta R.T.: -0.008 min
Response: 58180
Conc: 0.49 ug/ml

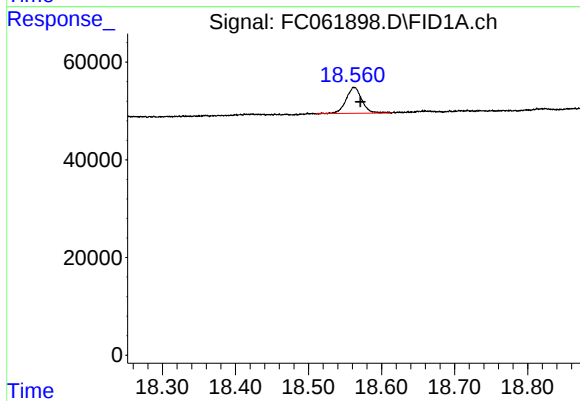

#18 n-Dotriacontane (C32)

R.T.: 18.563 min
Delta R.T.: -0.008 min
Response: 80133
Conc: 0.68 ug/ml

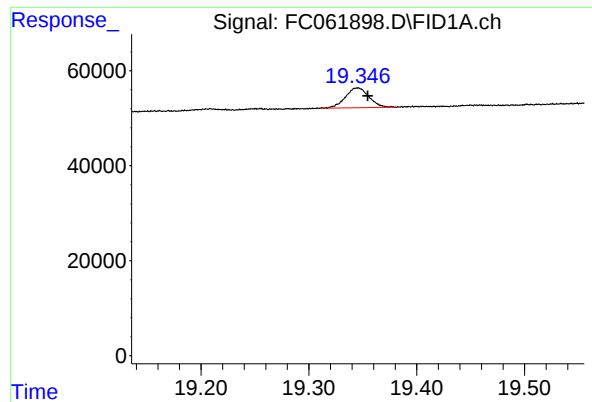

#19 n-Tetratriacontane (C34)

R.T.: 19.345 min
Delta R.T.: -0.009 min
Response: 63370
Conc: 0.56 ug/ml

Instrument :

FID_C

ClientSampleId :