

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102524AL\
Data File : FC067528.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2024 17:30
Operator : YP/AJ
Sample : P4518-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
EX-5-TPH-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

Integration File: autoint1.e
Quant Time: Oct 26 00:48:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.939	2448698	22.676 ug/mlm
Spiked Amount 50.000		Recovery =	45.35%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102524AL\
Data File : FC067528.D
Signal(s) : FID1A.ch
Acq On : 25 Oct 2024 17:30
Operator : YP/AJ
Sample : P4518-03
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
FID_C
ClientSampleId :
EX-5-TPH-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

Integration File: autoint1.e
Quant Time: Oct 26 00:48:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

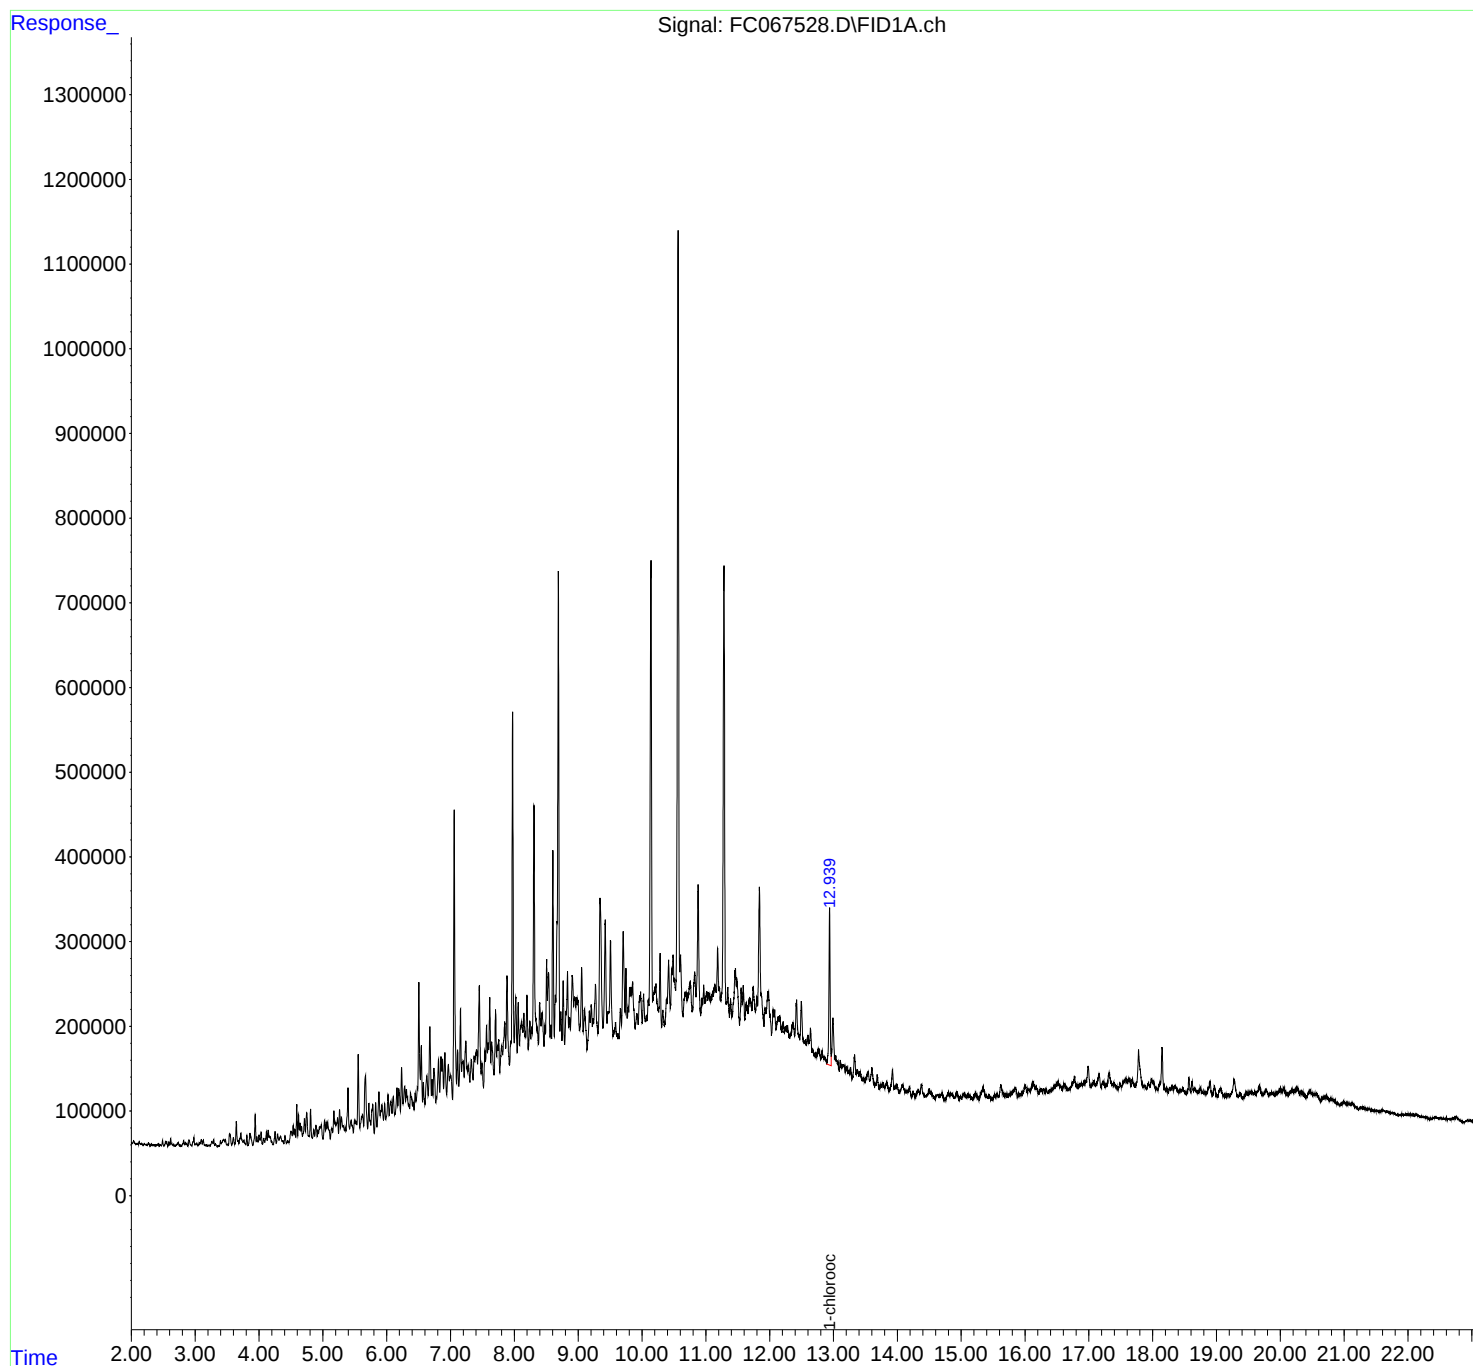

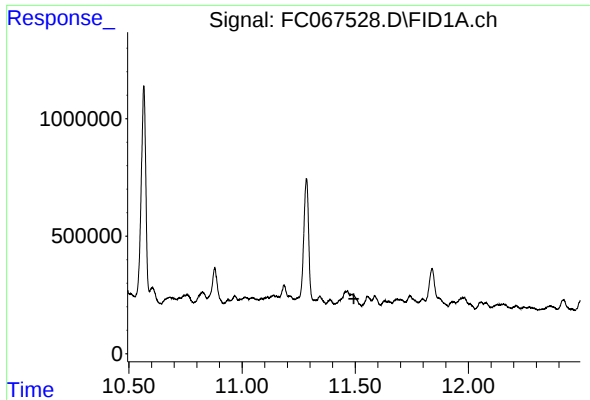


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.494 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :
EX-5-TPH-3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/28/2024
Supervised By :Ankita Jodhani 10/28/2024

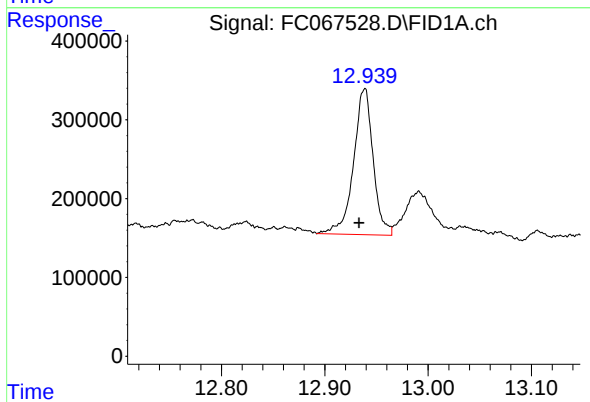

#12 1-chlorooctadecane (SURR)

R.T.: 12.939 min
Delta R.T.: 0.006 min
Response: 2448698
Conc: 22.68 ug/ml m