

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102623AL\
 Data File : FC064915.D
 Signal(s) : FID1A.ch
 Acq On : 26 Oct 2023 10:05
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 27 01:03:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 10 12:17:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rx1-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.442f	782461	4.544 ug/ml
11) T	n-Heneicosane (C21)	13.102	639481	3.776 ug/ml
13) T	n-Docosane (C22)	13.694	639585	3.882 ug/ml
14) T	n-Tetracosane (C24)	14.798	458399	2.880 ug/ml
15) T	n-Hexacosane (C26)	15.816	385969	2.520 ug/ml
16) T	n-Octacosane (C28)	16.762	254249	1.725 ug/ml
17) T	n-Tricontane (C30)	17.645	237291	1.622 ug/ml
18) T	n-Dotriacontane (C32)	18.476	239794	1.661 ug/ml
19) T	n-Tetratriacontane (C34)	19.256	251904	1.790 ug/ml
20) T	n-Hexatriacontane (C36)	19.989	262783	1.899 ug/ml
21) T	n-Octatriacontane (C38)	20.708	121242	0.915 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC102623AL\
Data File : FC064915.D
Signal(s) : FID1A.ch
Acq On : 26 Oct 2023 10:05
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:03:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 101023.M
Quant Title : GC Extractables
QLast Update : Tue Oct 10 12:17:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

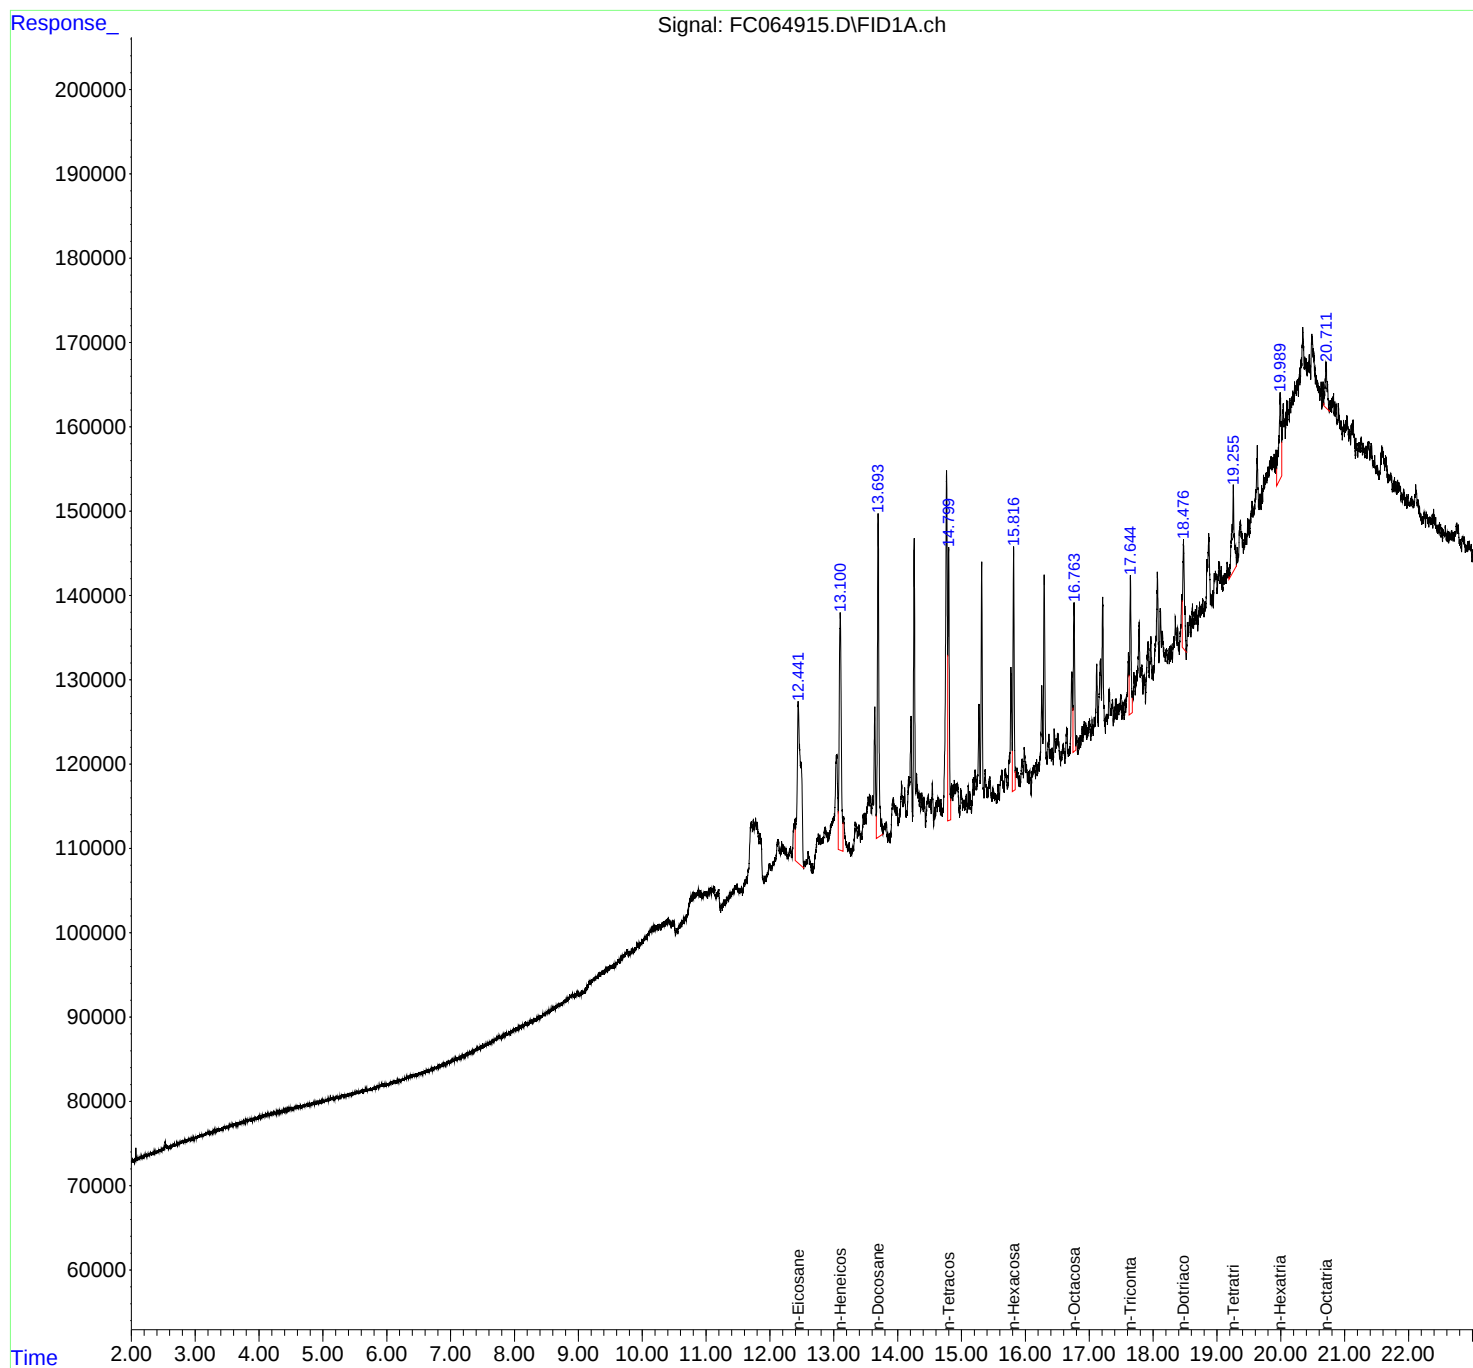


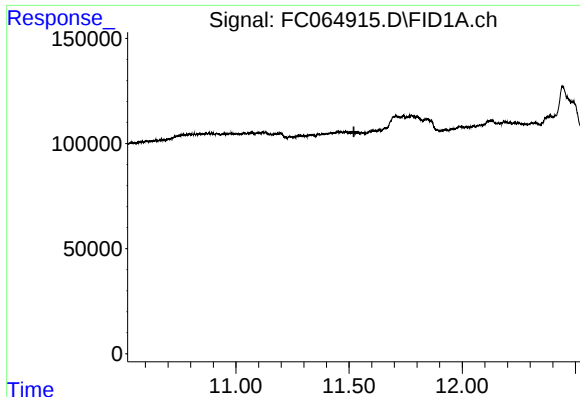

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.521 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

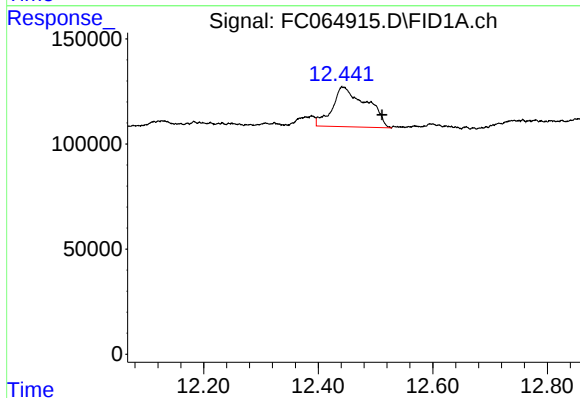


#10 n-Eicosane (C20)

R.T.: 12.442 min
Delta R.T.: -0.070 min
Response: 782461
Conc: 4.54 ug/ml

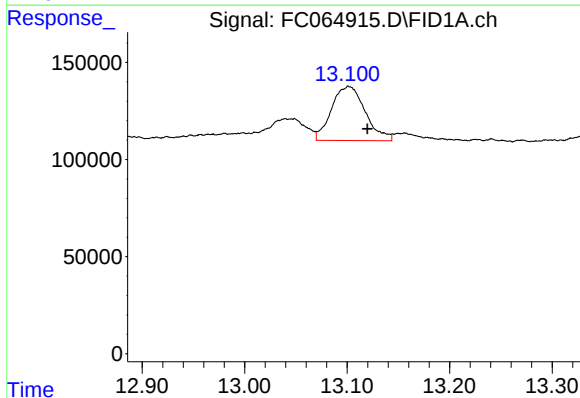


#11 n-Heneicosane (C21)

R.T.: 13.102 min
Delta R.T.: -0.018 min
Response: 639481
Conc: 3.78 ug/ml

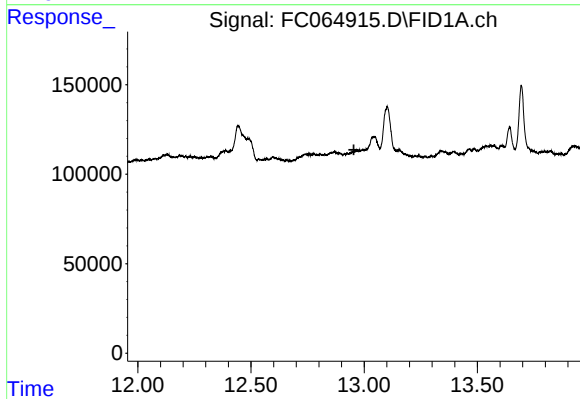

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

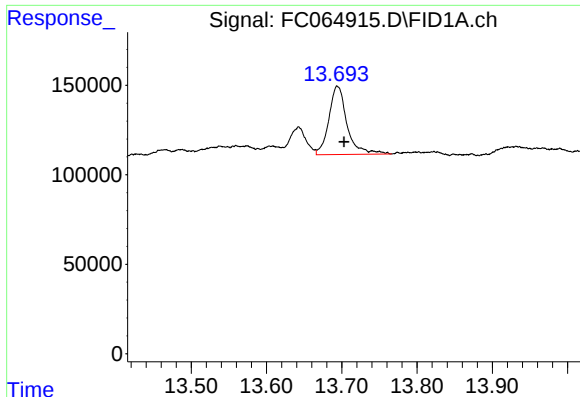

#13 n-Docosane (C22)


R.T.: 13.694 min
Delta R.T.: -0.009 min
Response: 639585
Conc: 3.88 ug/ml

Instrument :
FID_C
ClientSampleId :

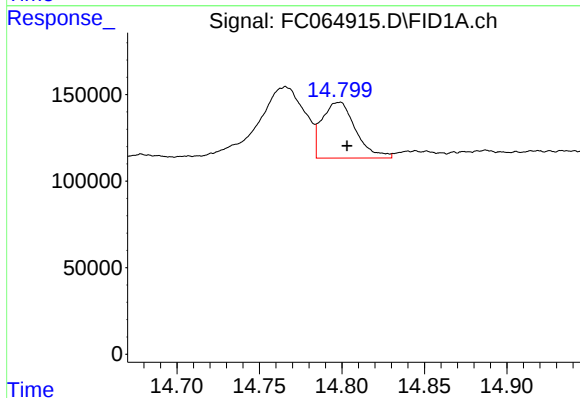


#14 n-Tetracosane (C24)

R.T.: 14.798 min
Delta R.T.: -0.005 min
Response: 458399
Conc: 2.88 ug/ml

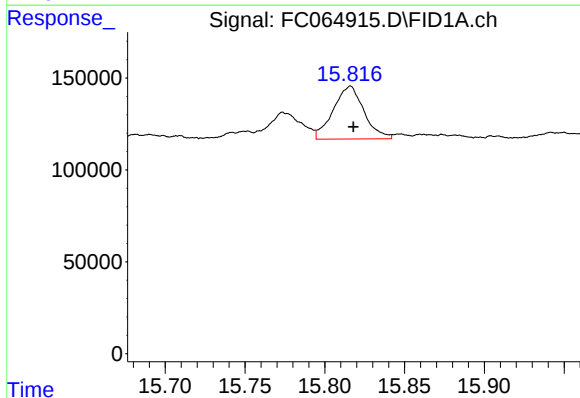


#15 n-Hexacosane (C26)

R.T.: 15.816 min
Delta R.T.: -0.002 min
Response: 385969
Conc: 2.52 ug/ml

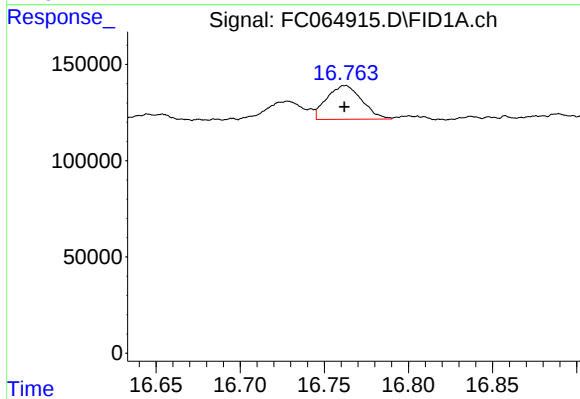

#16 n-Octacosane (C28)


R.T.: 16.762 min
Delta R.T.: 0.000 min
Response: 254249
Conc: 1.73 ug/ml

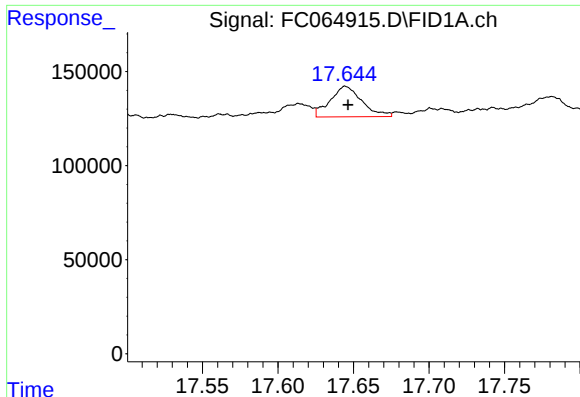

#17 n-Tricontane (C30)


R.T.: 17.645 min
Delta R.T.: -0.002 min
Response: 237291
Conc: 1.62 ug/ml

Instrument :
FID_C
ClientSampleId :

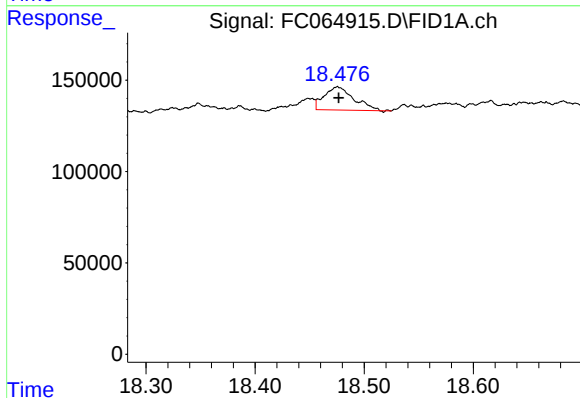


#18 n-Dotriacontane (C32)

R.T.: 18.476 min
Delta R.T.: -0.001 min
Response: 239794
Conc: 1.66 ug/ml

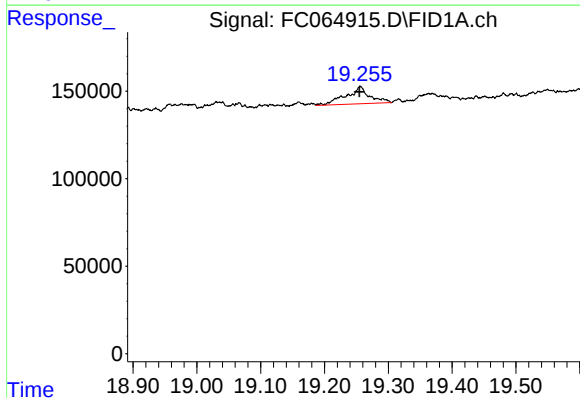


#19 n-Tetratriacontane (C34)

R.T.: 19.256 min
Delta R.T.: 0.002 min
Response: 251904
Conc: 1.79 ug/ml

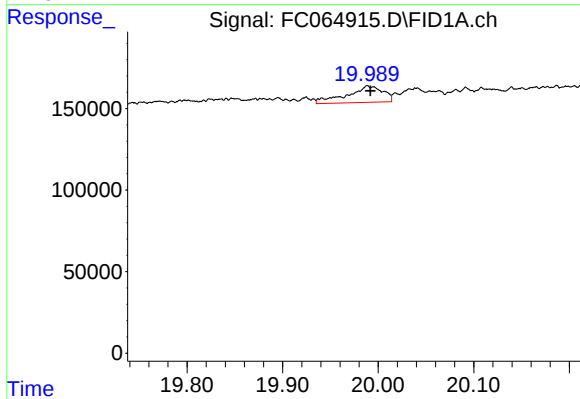

#20 n-Hexatriacontane (C36)

R.T.: 19.989 min
Delta R.T.: -0.003 min
Response: 262783
Conc: 1.90 ug/ml

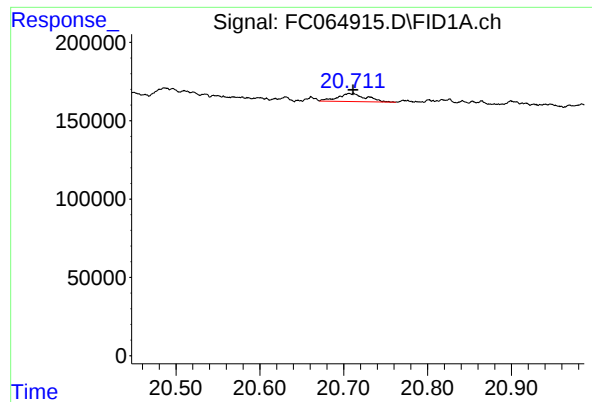

#21 n-Octatriacontane (C38)

R.T.: 20.708 min
Delta R.T.: -0.003 min
Response: 121242
Conc: 0.92 ug/ml

Instrument :

FID_C

ClientSampleId :