

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC103023AL\
 Data File : FC064945.D
 Signal(s) : FID1A.ch
 Acq On : 30 Oct 2023 09:07
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 30 23:35:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.488	146372	0.814 ug/ml
11) T n-Heneicosane (C21)	13.106	265874	1.514 ug/ml
13) T n-Docosane (C22)	13.695	308922	1.798 ug/ml
14) T n-Tetracosane (C24)	14.800	167519	1.006 ug/ml
15) T n-Hexacosane (C26)	15.816	182440	1.137 ug/ml
16) T n-Octacosane (C28)	16.764	157584	1.007 ug/ml
17) T n-Tricontane (C30)	17.645	97341	0.615 ug/ml
18) T n-Dotriacontane (C32)	18.477	194760	1.233 ug/ml
19) T n-Tetratriacontane (C34)	19.255	143517	0.940 ug/ml
20) T n-Hexatriacontane (C36)	19.995	54451	0.361 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC103023AL\
Data File : FC064945.D
Signal(s) : FID1A.ch
Acq On : 30 Oct 2023 09:07
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 23:35:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

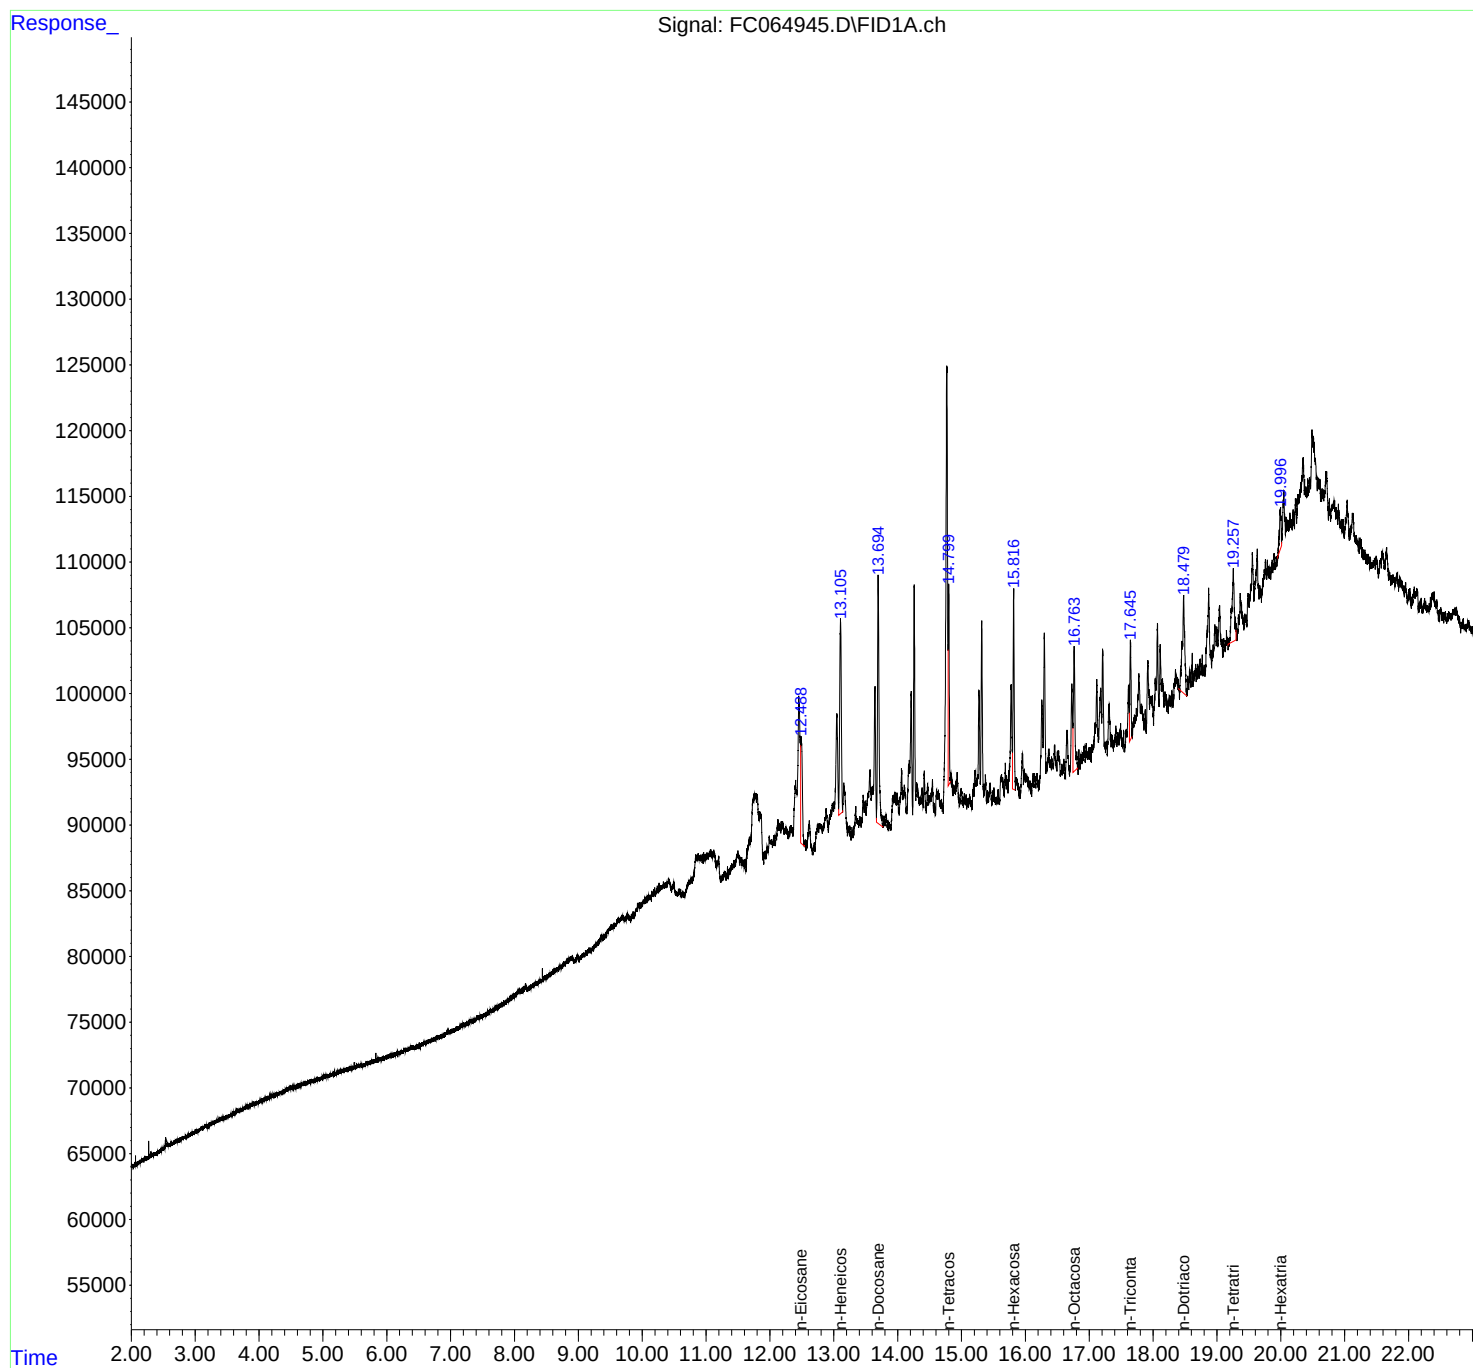


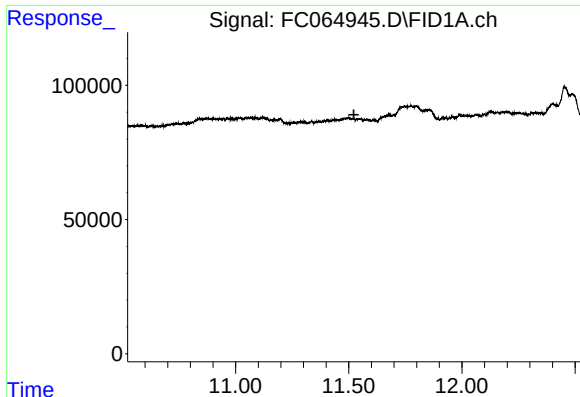

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

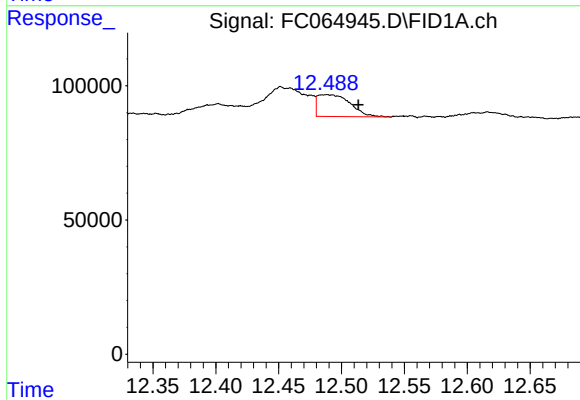


#10 n-Eicosane (C20)

R.T.: 12.488 min
Delta R.T.: -0.025 min
Response: 146372
Conc: 0.81 ug/ml

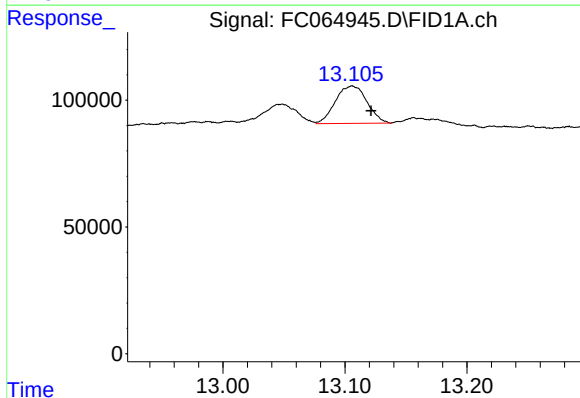


#11 n-Heneicosane (C21)

R.T.: 13.106 min
Delta R.T.: -0.016 min
Response: 265874
Conc: 1.51 ug/ml

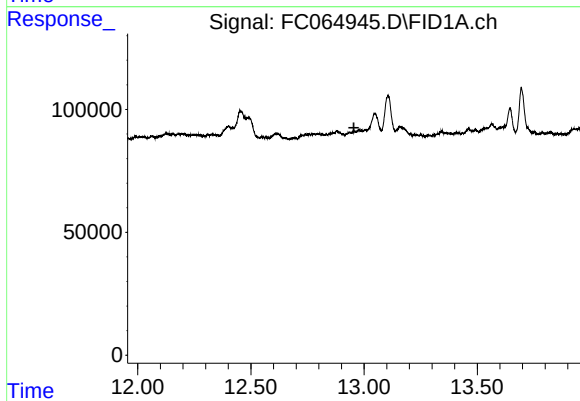

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

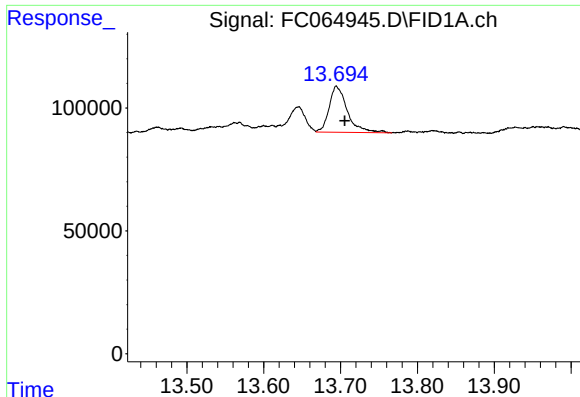

#13 n-Docosane (C22)


R.T.: 13.695 min
Delta R.T.: -0.011 min
Response: 308922
Conc: 1.80 ug/ml

Instrument :
FID_C
ClientSampleId :

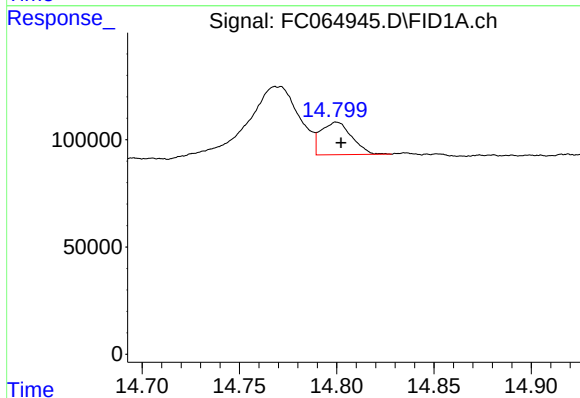


#14 n-Tetracosane (C24)

R.T.: 14.800 min
Delta R.T.: -0.002 min
Response: 167519
Conc: 1.01 ug/ml

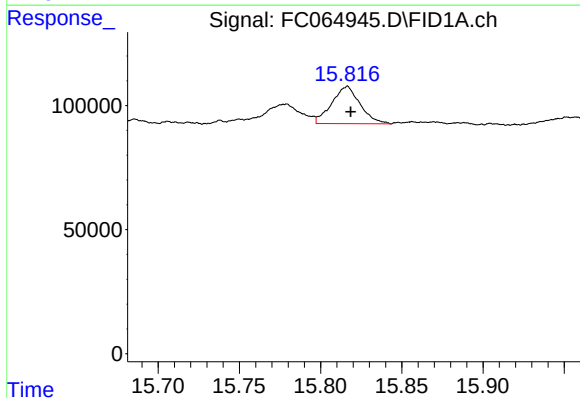


#15 n-Hexacosane (C26)

R.T.: 15.816 min
Delta R.T.: -0.002 min
Response: 182440
Conc: 1.14 ug/ml

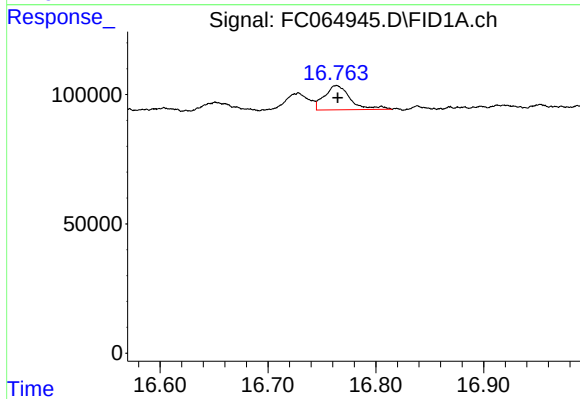

#16 n-Octacosane (C28)


R.T.: 16.764 min
Delta R.T.: -0.001 min
Response: 157584
Conc: 1.01 ug/ml

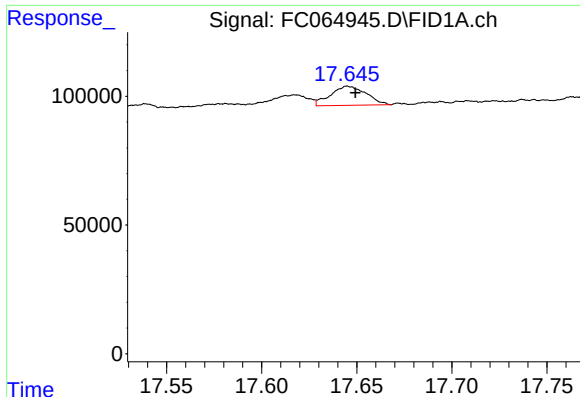

#17 n-Tricontane (C30)


R.T.: 17.645 min
Delta R.T.: -0.004 min
Response: 97341
Conc: 0.61 ug/ml

Instrument :
FID_C
ClientSampleId :

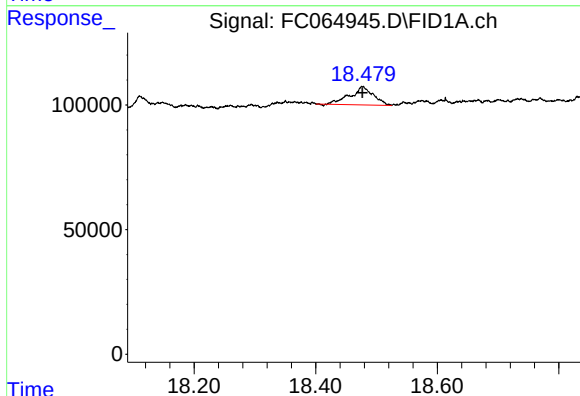


#18 n-Dotriacontane (C32)

R.T.: 18.477 min
Delta R.T.: 0.000 min
Response: 194760
Conc: 1.23 ug/ml

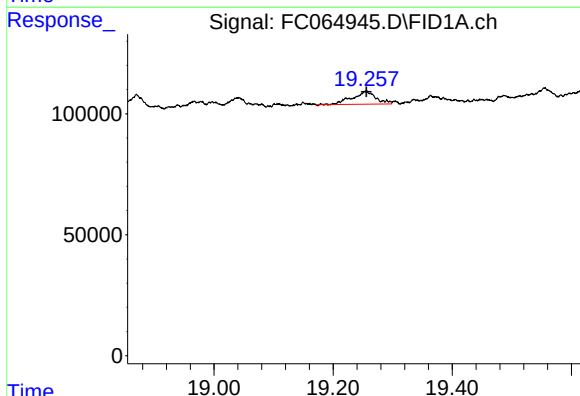

#19 n-Tetratriacontane (C34)

R.T.: 19.255 min
Delta R.T.: 0.000 min
Response: 143517
Conc: 0.94 ug/ml

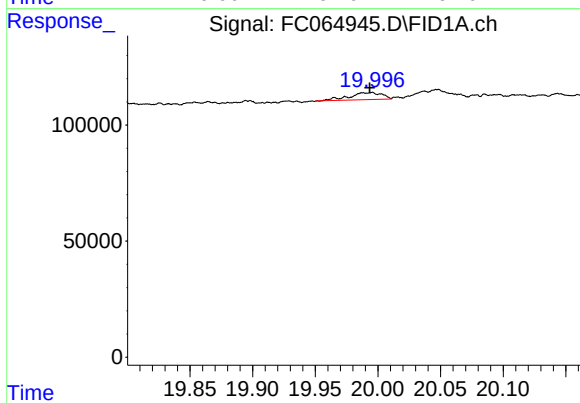

#20 n-Hexatriacontane (C36)

R.T.: 19.995 min
Delta R.T.: 0.001 min
Response: 54451
Conc: 0.36 ug/ml