

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103118\
 Data File : PS002224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 10:51
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:20:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	11.436	10.925	142.5E6	137.0E6	452.818	381.419
Target Compounds							
1) T	Dalapon	0.000	2.360	0	136624	N.D.	0.303 #
6) T	MCPD	0.000	11.483	0	645615	N.D.	0.750 #
7) T	MCPA	0.000	11.815	0	835355	N.D.	0.617 #
10) T	Pentachlo...	0.000	13.288	0	70177	N.D.	0.015 #
12) T	2,4,5-T	0.000	14.538	0	10988085	N.D.	7.338 #
15) T	Picloram	16.938	16.784	5683798	537292	2.383	0.238 #
16) T	DCPA	0.000	16.845	0	20210638	N.D.	8.535 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103118\
Data File : PS002224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 10:51
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:20:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

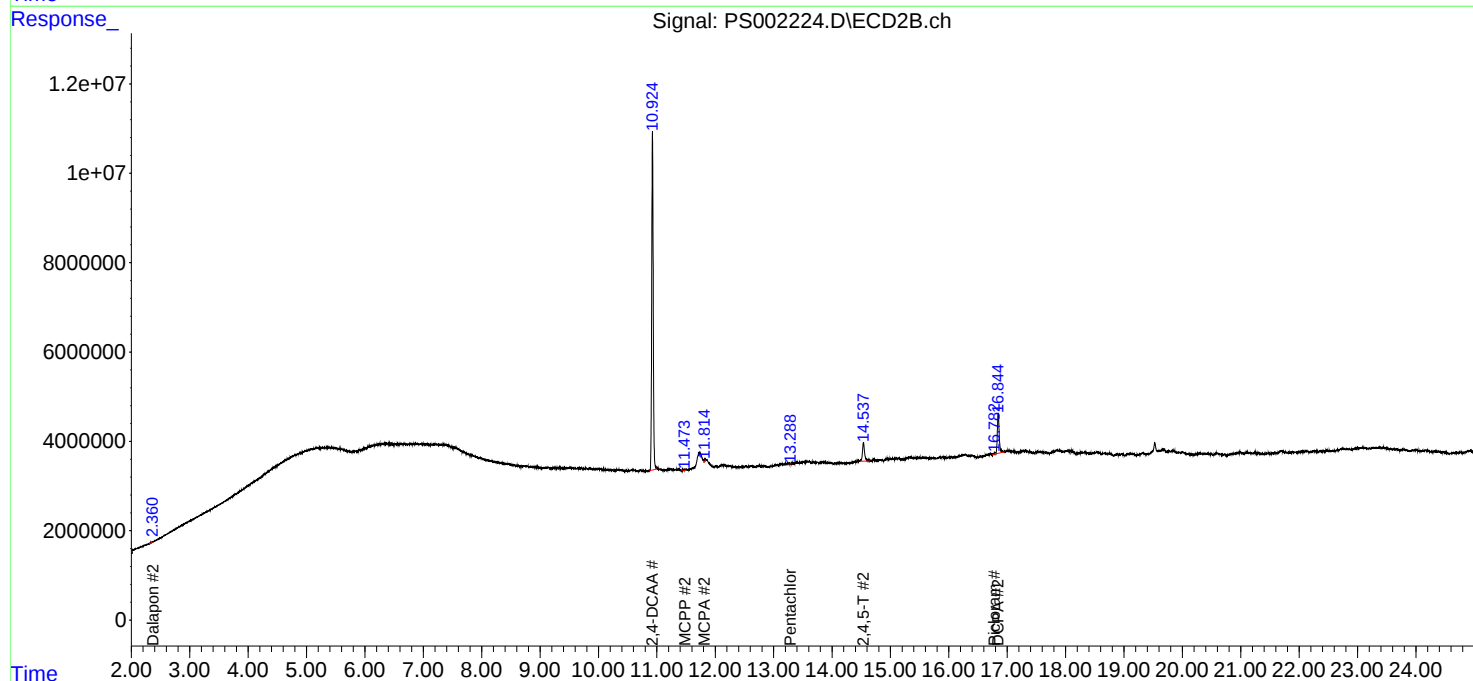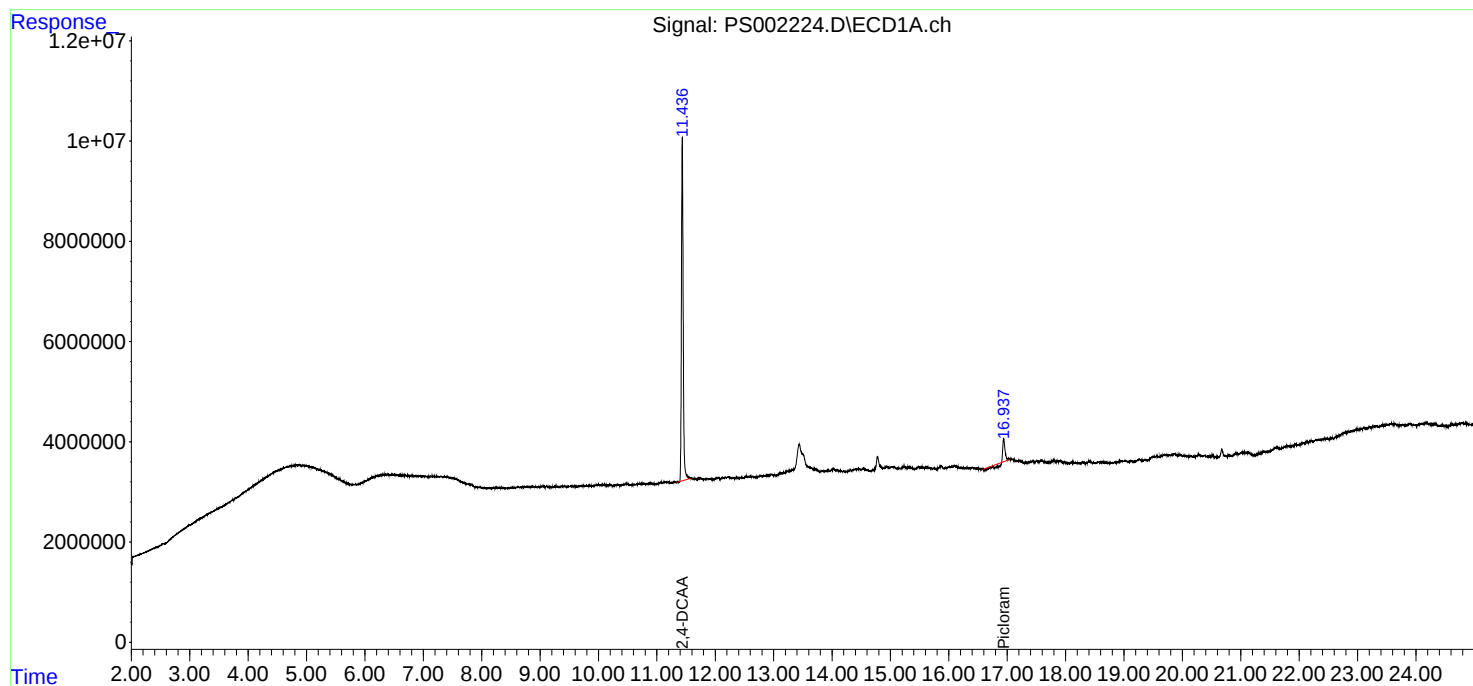

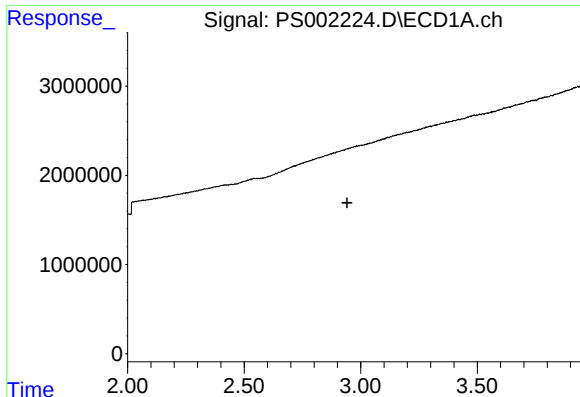


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

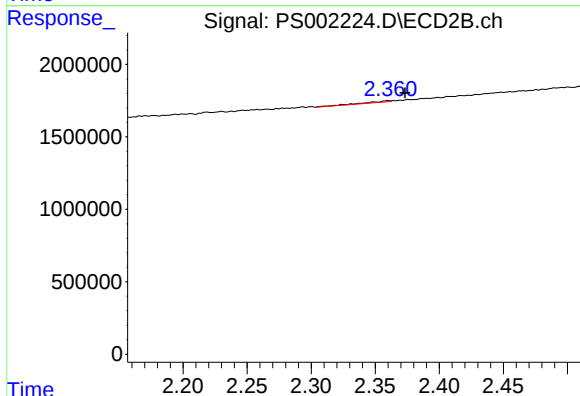


#1 Dalapon

R.T.: 2.360 min
Delta R.T.: -0.013 min
Response: 136624
Conc: 0.30 ng/ml

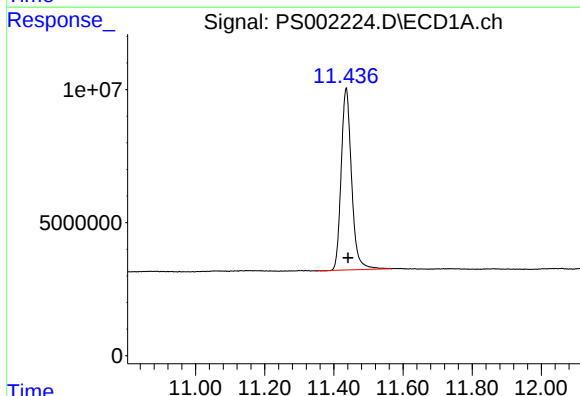


#4 2,4-DCAA

R.T.: 11.436 min
Delta R.T.: -0.006 min
Response: 142495465
Conc: 452.82 ng/ml

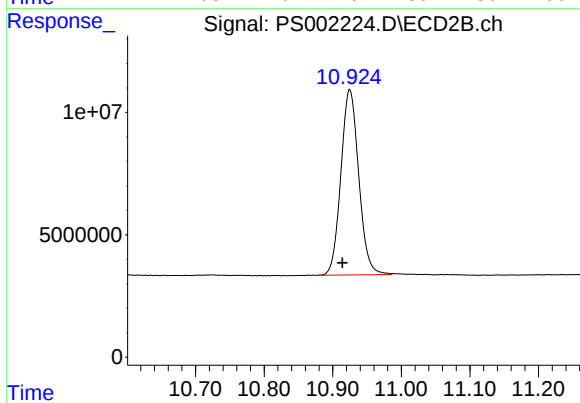


#4 2,4-DCAA

R.T.: 10.925 min
Delta R.T.: 0.010 min
Response: 136966772
Conc: 381.42 ng/ml

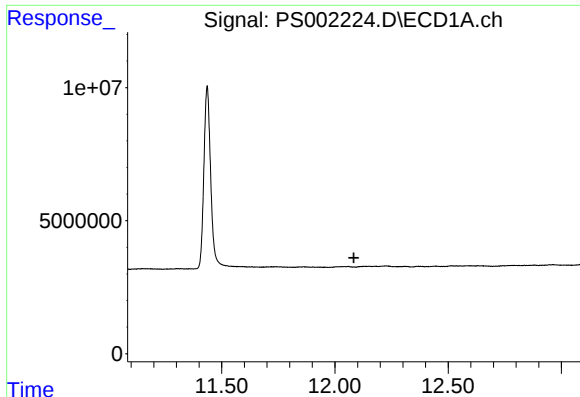


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

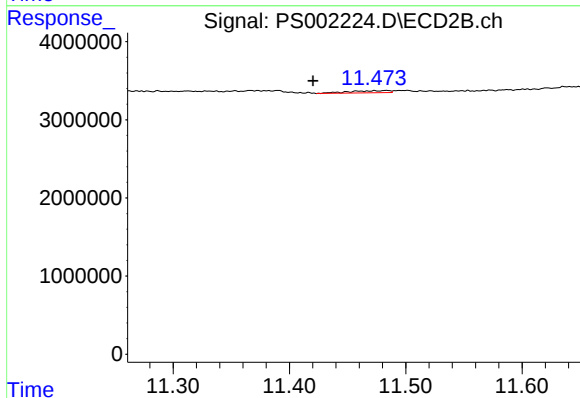


#6 MCPP

R.T.: 11.483 min
Delta R.T.: 0.063 min
Response: 645615
Conc: 0.75 ug/ml

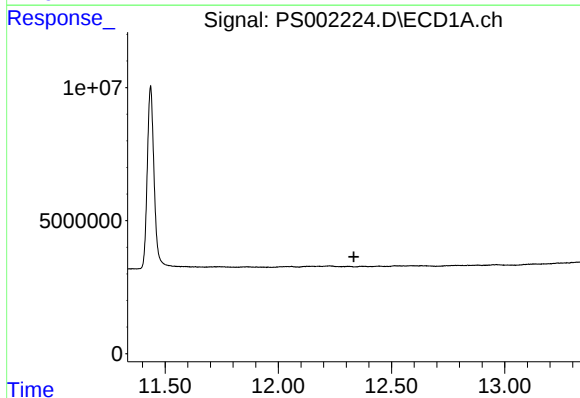


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

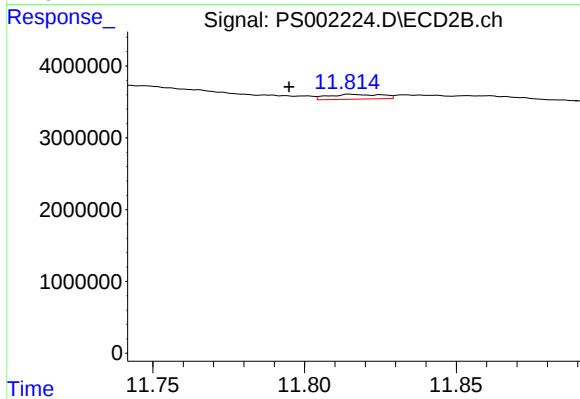


#7 MCPA

R.T.: 11.815 min
Delta R.T.: 0.020 min
Response: 835355
Conc: 0.62 ug/ml

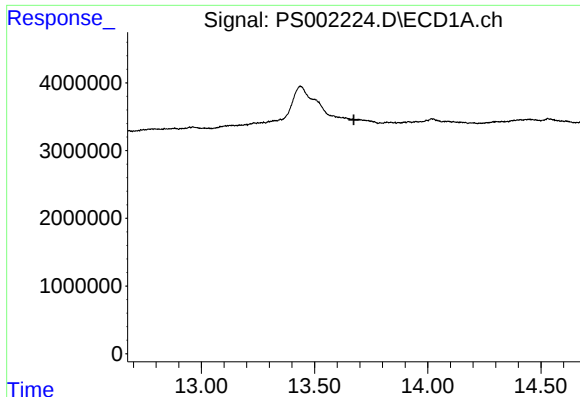


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

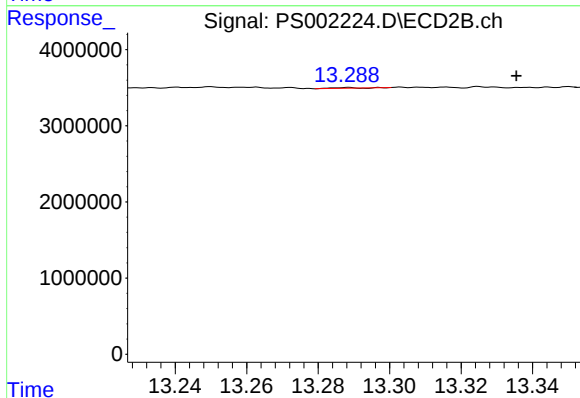


#10 Pentachlorophenol

R.T.: 13.288 min
Delta R.T.: -0.047 min
Response: 70177
Conc: 0.01 ng/ml

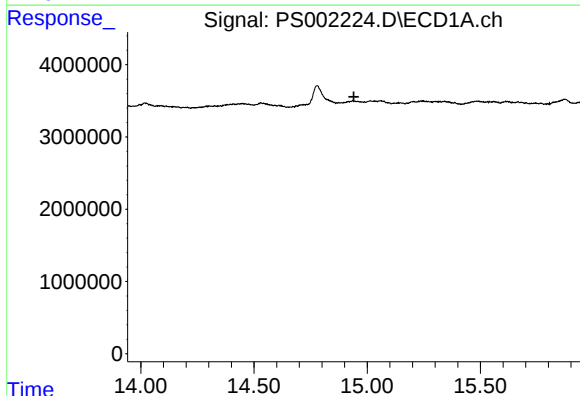


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.941 min
Response: 0
Conc: N.D.

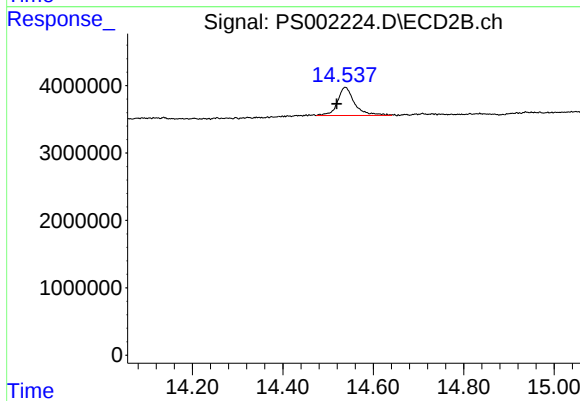


#12 2,4,5-T

R.T.: 14.538 min
Delta R.T.: 0.019 min
Response: 10988085
Conc: 7.34 ng/ml

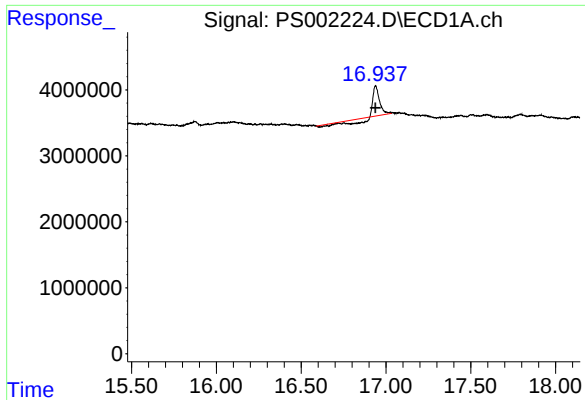


#15 Picloram

R.T.: 16.938 min
Delta R.T.: 0.001 min
Response: 5683798
Conc: 2.38 ng/ml

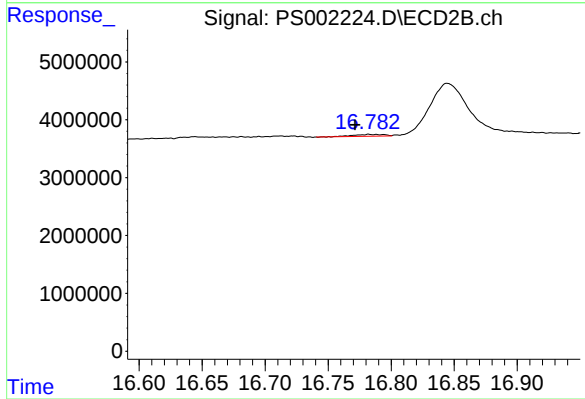


#15 Picloram

R.T.: 16.784 min
Delta R.T.: 0.013 min
Response: 537292
Conc: 0.24 ng/ml

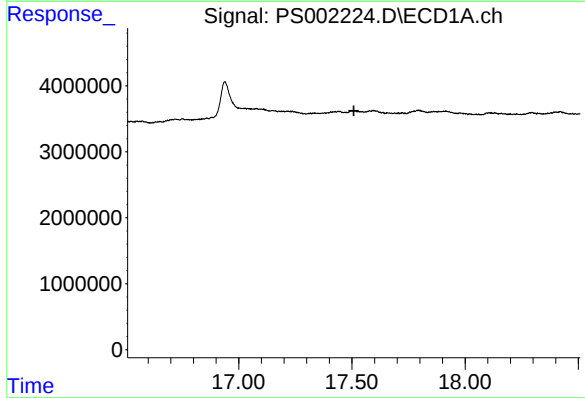

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

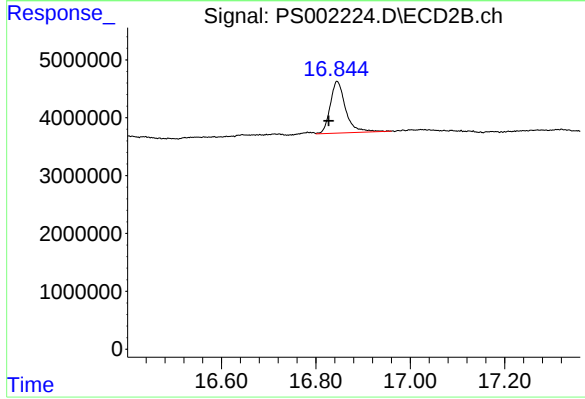

#16 DCPA

R.T.: 16.845 min
Delta R.T.: 0.018 min
Response: 20210638
Conc: 8.54 ng/ml