

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110323AL\
 Data File : FC064989.D
 Signal(s) : FID1A.ch
 Acq On : 03 Nov 2023 10:05
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 04 00:25:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.491	59608	0.332 ug/ml
11) T n-Heneicosane (C21)	13.105	62496	0.356 ug/ml
13) T n-Docosane (C22)	13.689	53254	0.310 ug/ml
14) T n-Tetracosane (C24)	14.763	184621	1.108 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110323AL\
Data File : FC064989.D
Signal(s) : FID1A.ch
Acq On : 03 Nov 2023 10:05
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 04 00:25:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

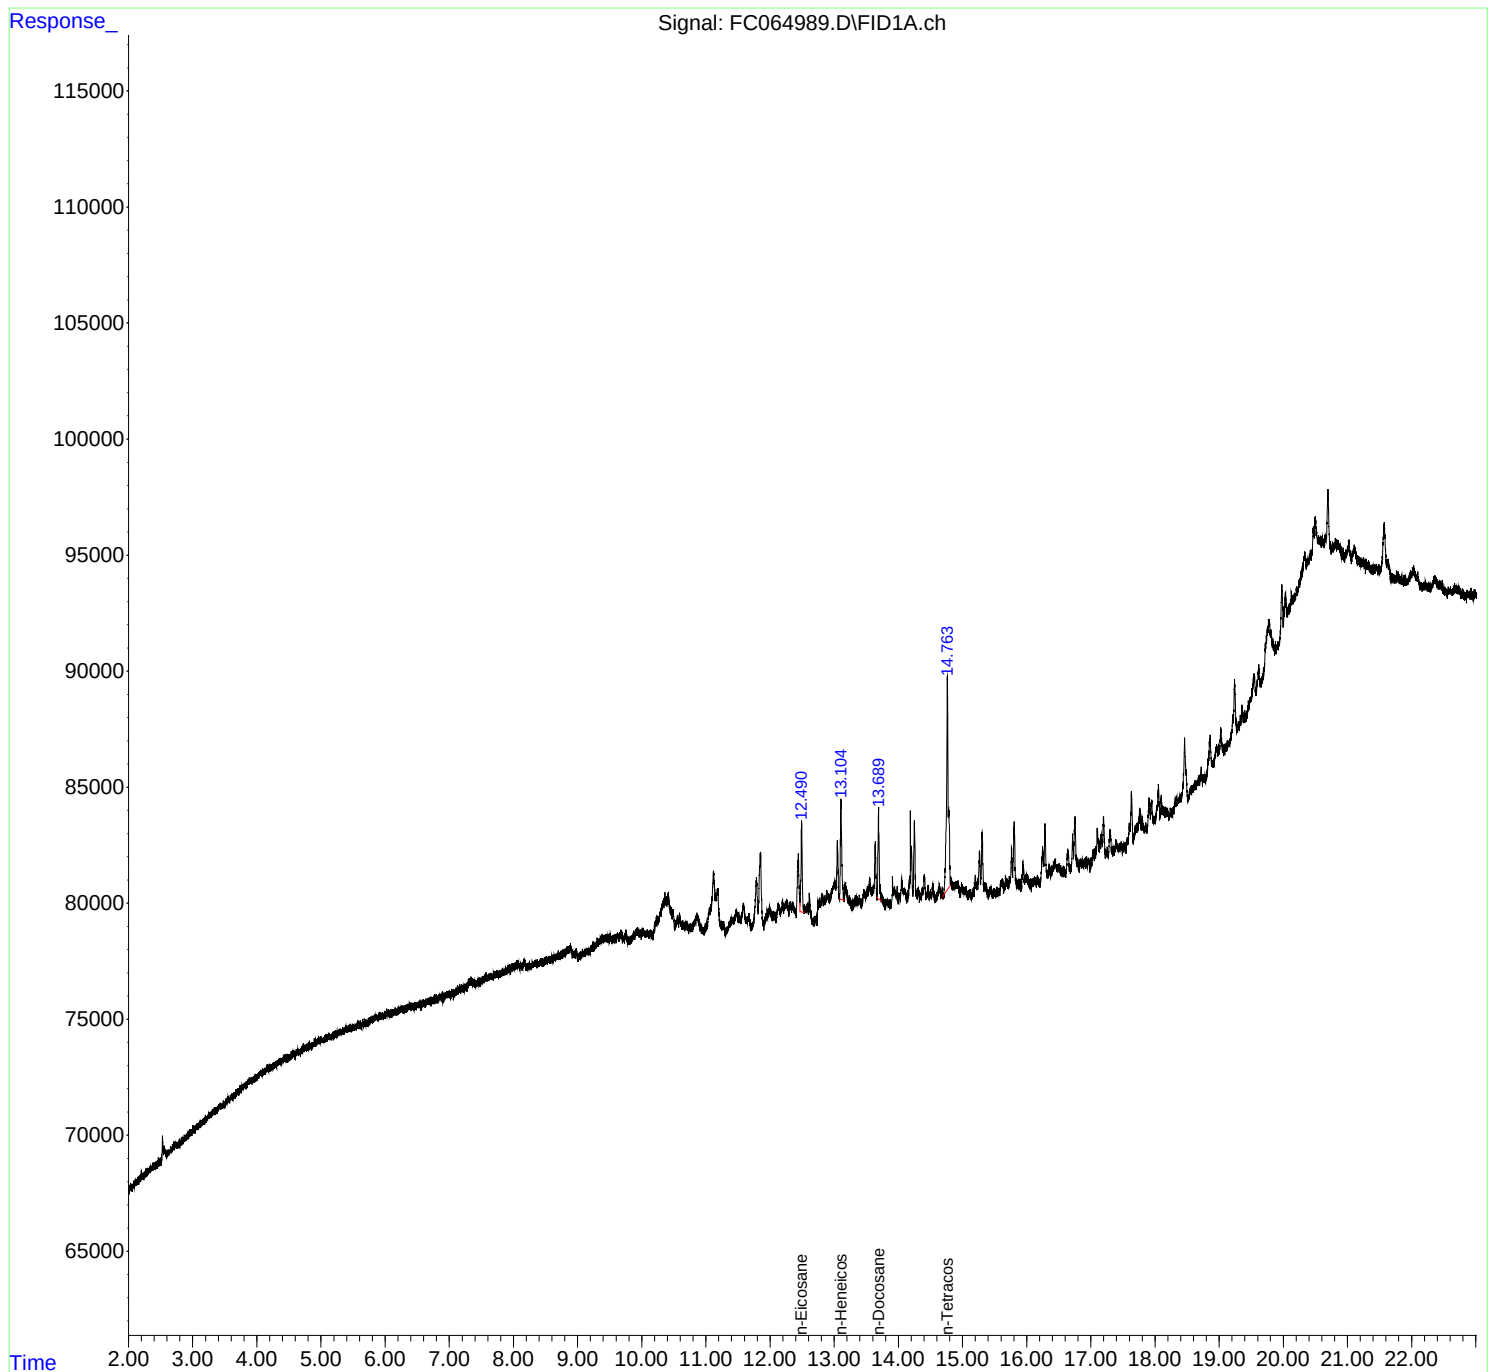


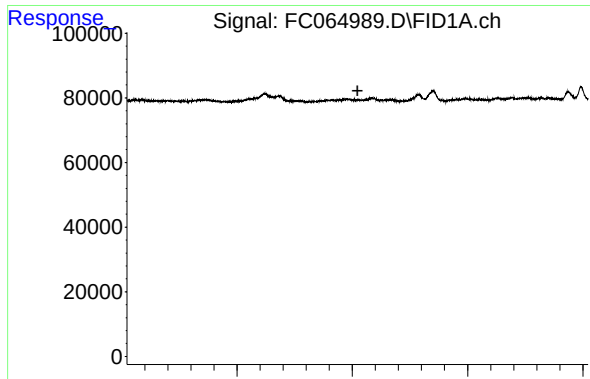

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

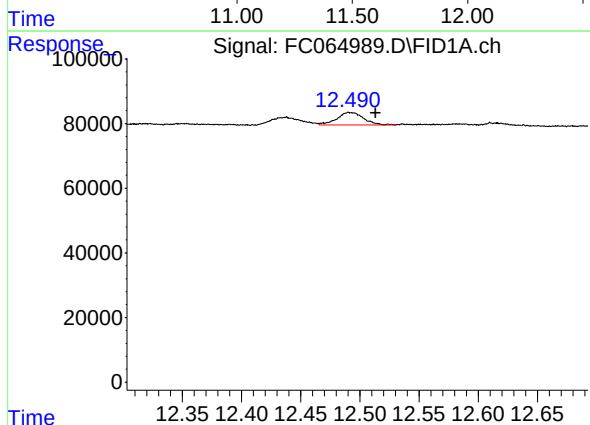


#10 n-Eicosane (C20)

R.T.: 12.491 min
Delta R.T.: -0.023 min
Response: 59608
Conc: 0.33 ug/ml

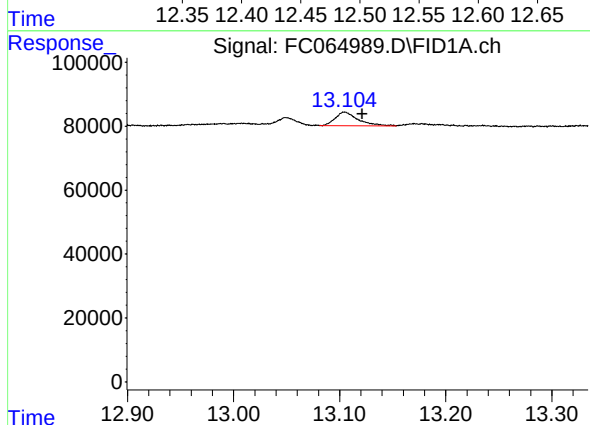


#11 n-Heneicosane (C21)

R.T.: 13.105 min
Delta R.T.: -0.017 min
Response: 62496
Conc: 0.36 ug/ml

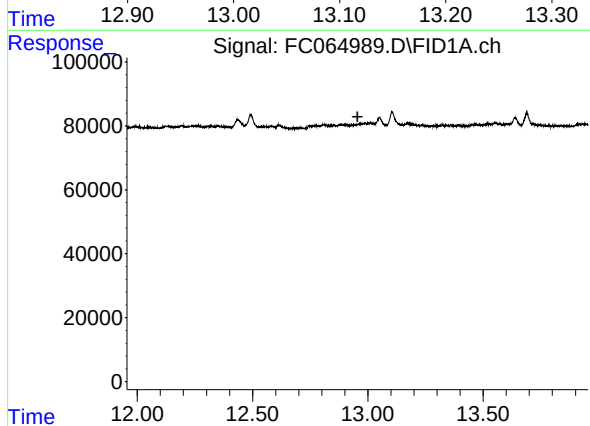

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

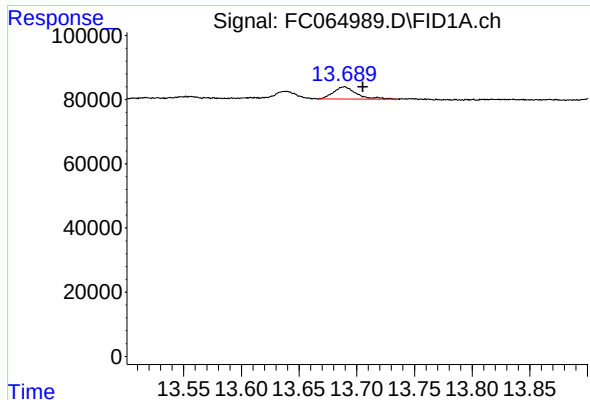

#13 n-Docosane (C22)

R.T.: 13.689 min
Delta R.T.: -0.016 min
Response: 53254
Conc: 0.31 ug/ml

Instrument :
FID_C
ClientSampleId :

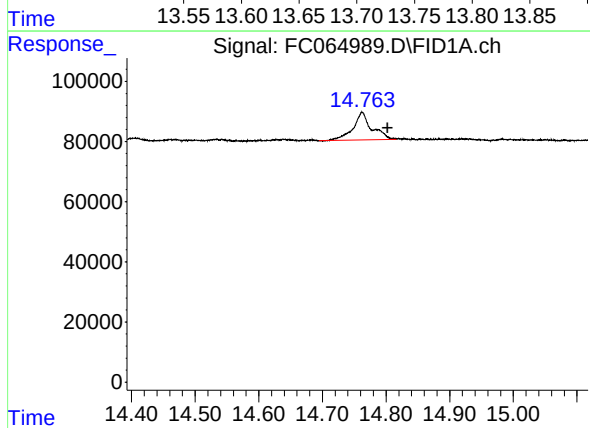

#14 n-Tetracosane (C24)

R.T.: 14.763 min
Delta R.T.: -0.039 min
Response: 184621
Conc: 1.11 ug/ml