

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110323AL\
Data File : FC065006.D
Signal(s) : FID1A.ch
Acq On : 03 Nov 2023 23:17
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 04 02:42:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
22) T n-Tetracontane (C40)	21.570	287822	1.957 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110323AL\
Data File : FC065006.D
Signal(s) : FID1A.ch
Acq On : 03 Nov 2023 23:17
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 04 02:42:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

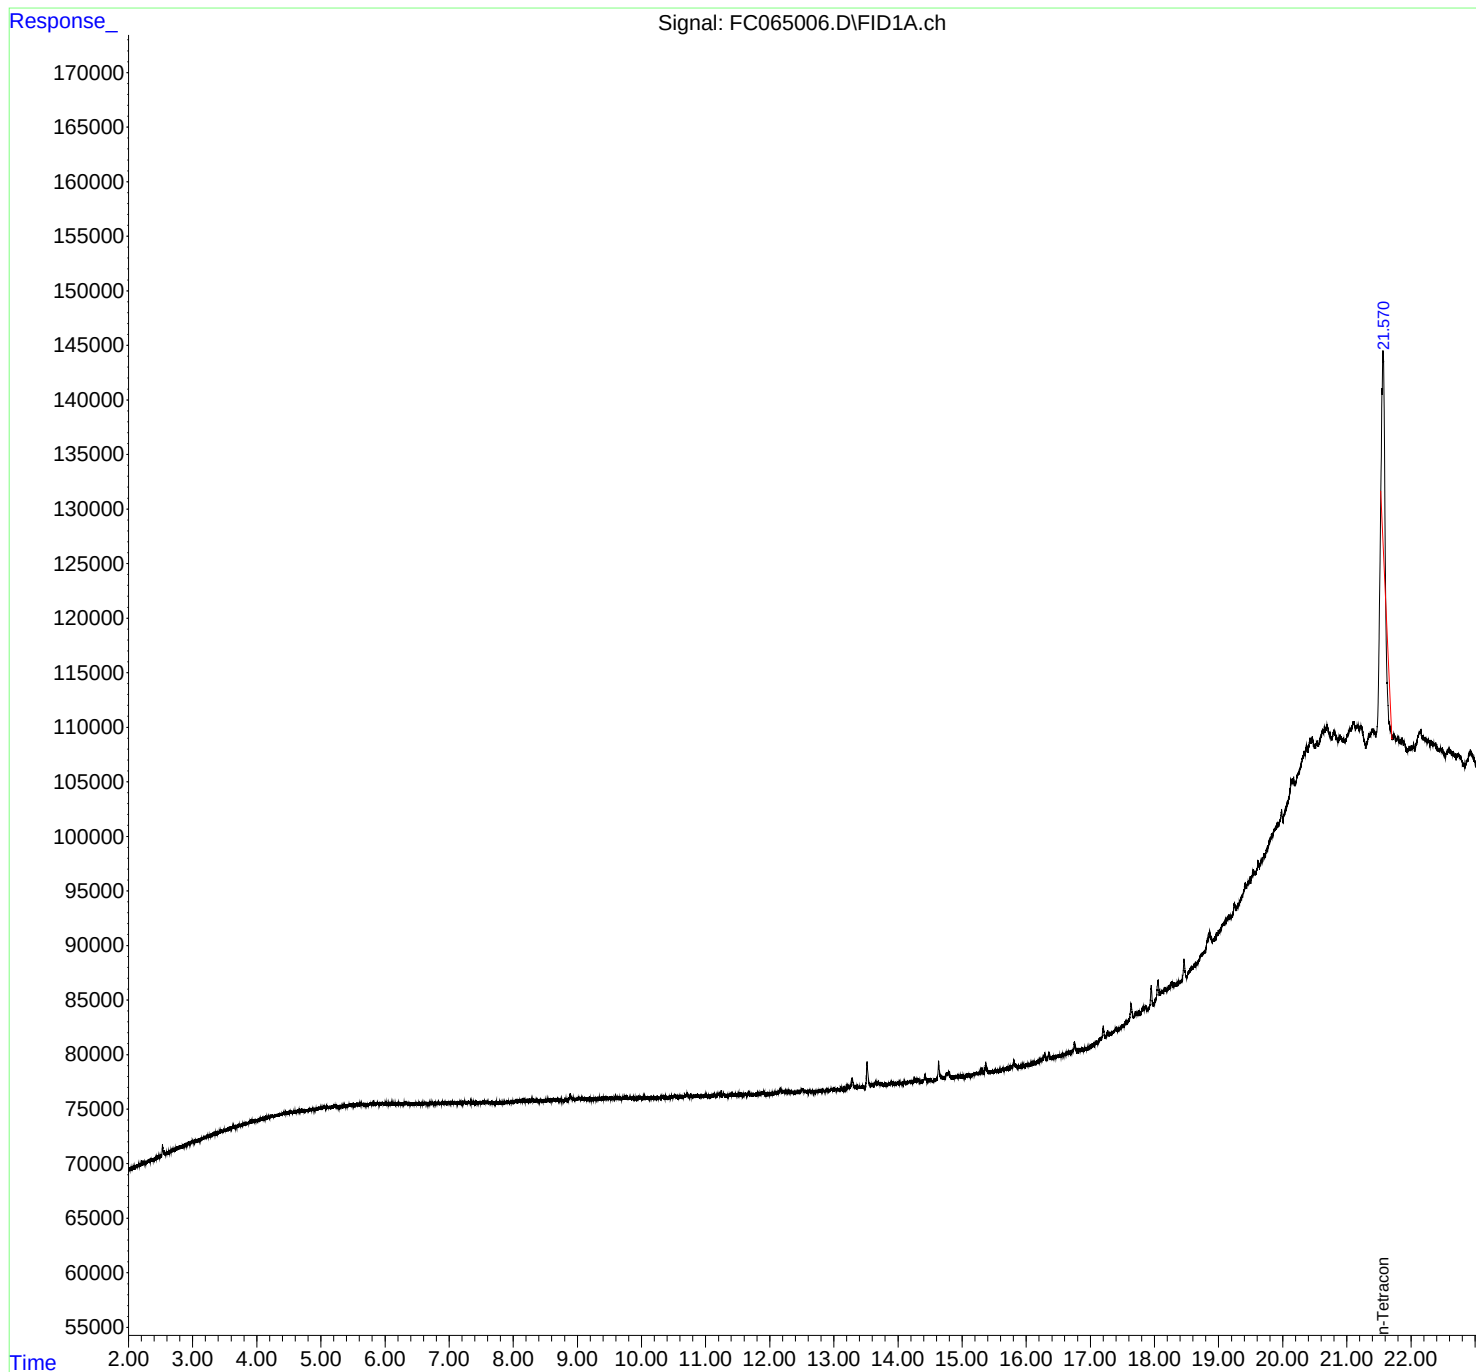


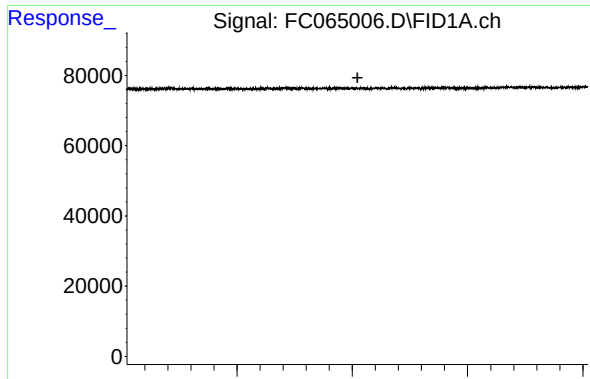

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

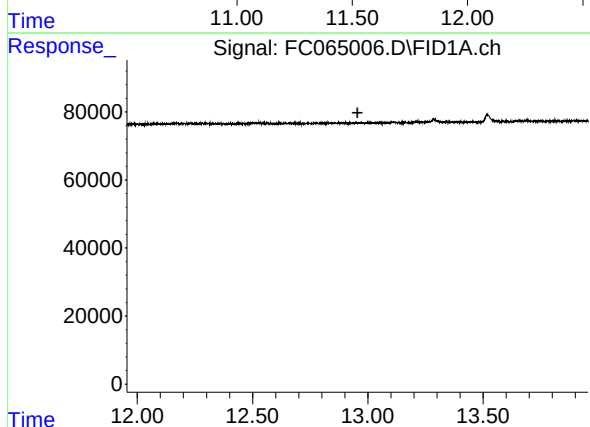

#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

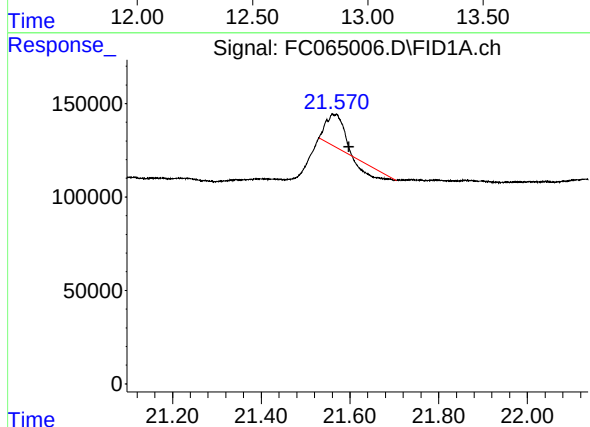

#22 n-Tetracontane (C40)

R.T.: 21.570 min
Delta R.T.: -0.028 min
Response: 287822
Conc: 1.96 ug/ml