

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110624AL\
Data File : FC067647.D
Signal(s) : FID1A.ch
Acq On : 06 Nov 2024 21:53
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 07 00:33:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

18) T	n-Dotriacontane (C32)	18.469	204513	1.728 ug/ml
19) T	n-Tetratriacontane (C34)	19.252	89035	0.850 ug/ml
20) T	n-Hexatriacontane (C36)	19.987	39136	0.430 ug/ml
21) T	n-Octatriacontane (C38)	20.718	556696	6.428 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110624AL\
Data File : FC067647.D
Signal(s) : FID1A.ch
Acq On : 06 Nov 2024 21:53
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 07 00:33:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102324.M
Quant Title : GC Extractables
QLast Update : Wed Oct 23 18:12:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

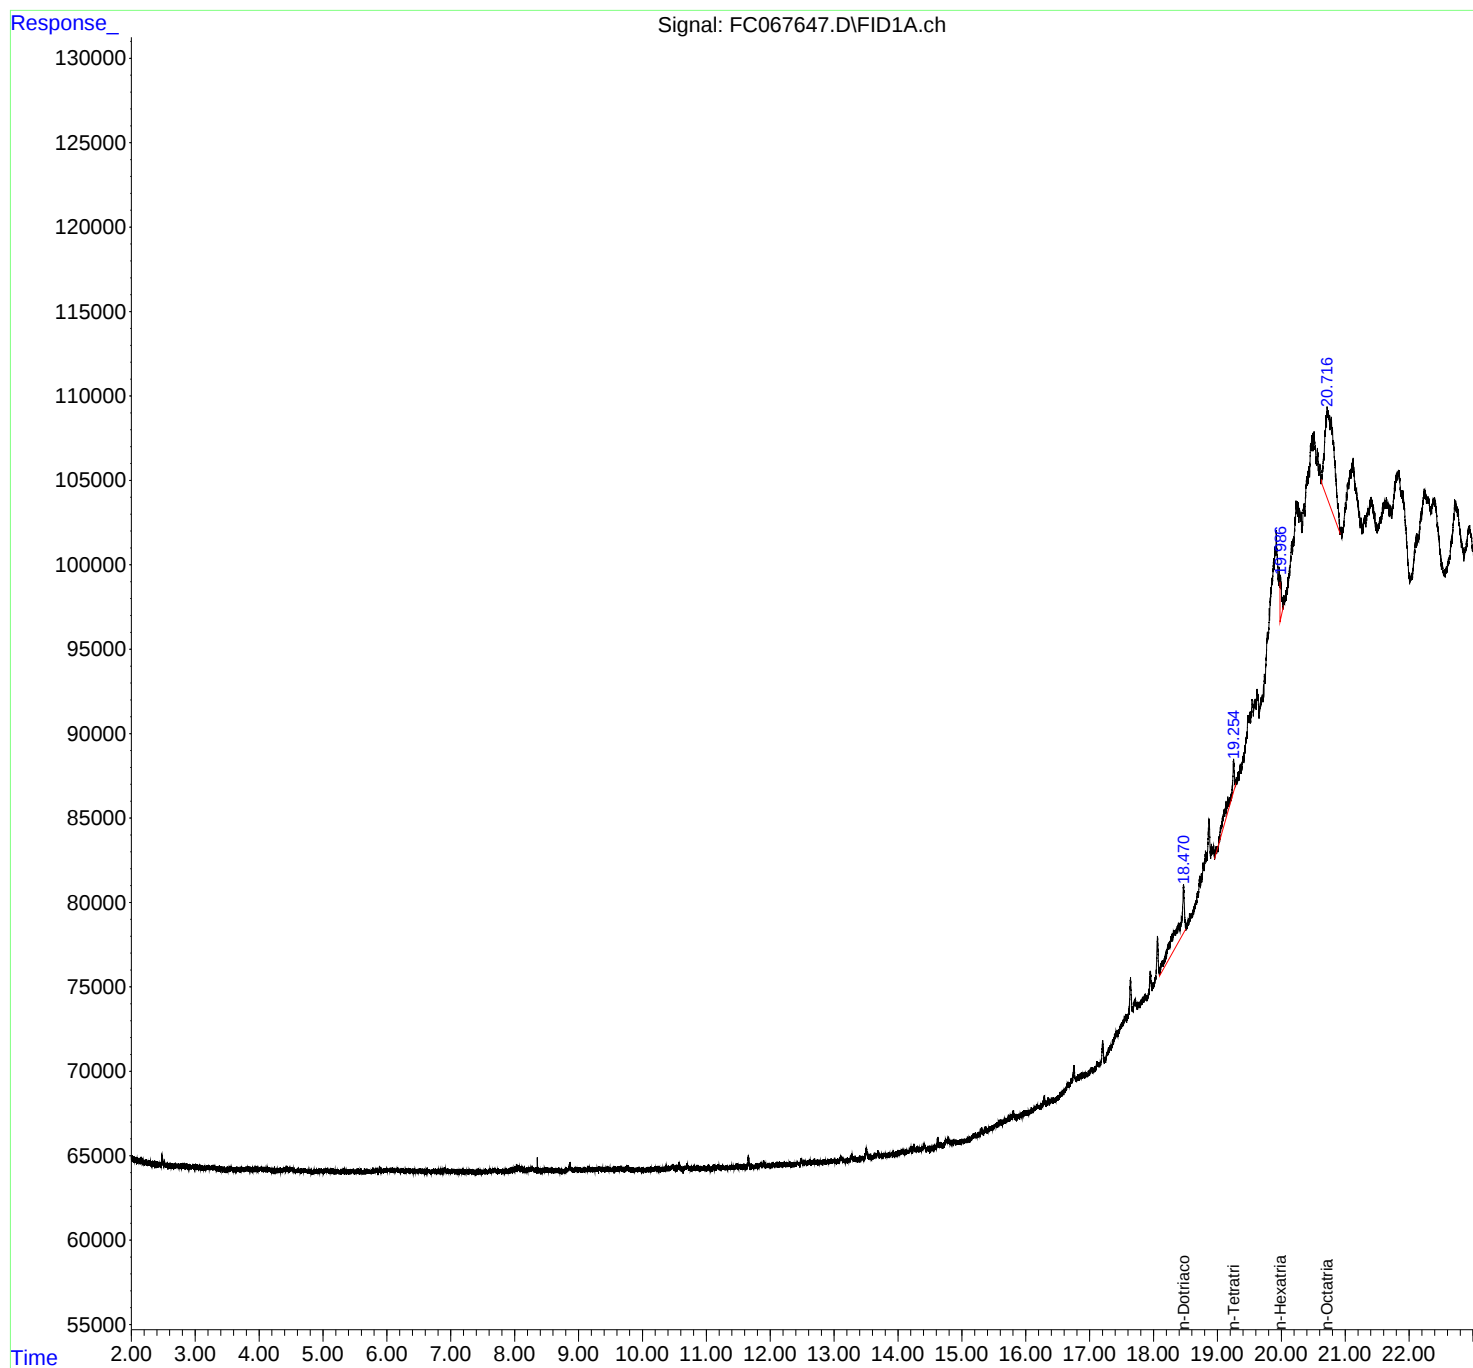


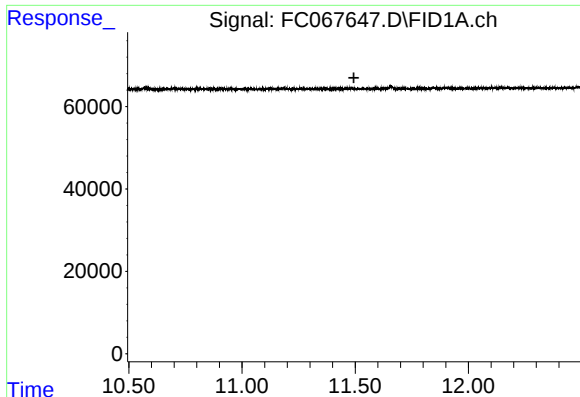

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.494 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

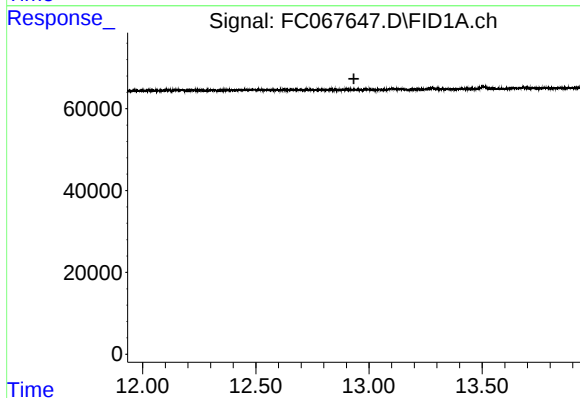


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.933 min
Response: 0
Conc: N.D.

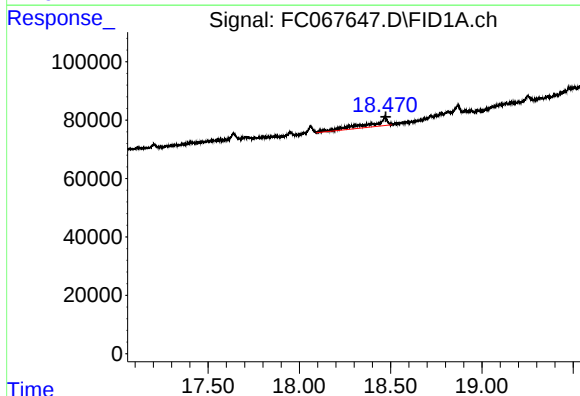


#18 n-Dotriacontane (C32)

R.T.: 18.469 min
Delta R.T.: -0.005 min
Response: 204513
Conc: 1.73 ug/ml

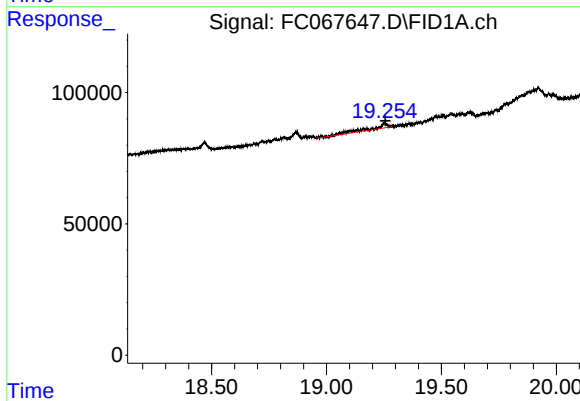

#19 n-Tetratriacontane (C34)


R.T.: 19.252 min
Delta R.T.: -0.004 min
Response: 89035
Conc: 0.85 ug/ml

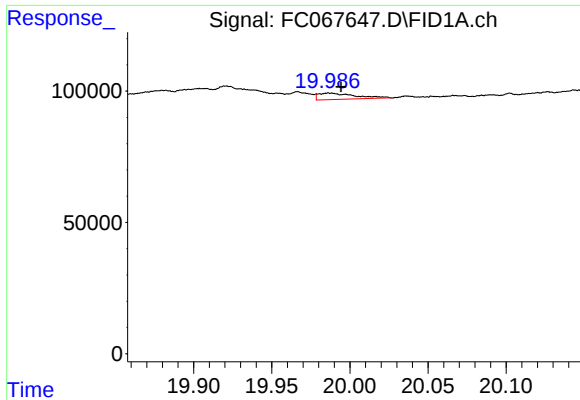

#20 n-Hexatriacontane (C36)

R.T.: 19.987 min
Delta R.T.: -0.008 min
Response: 39136
Conc: 0.43 ug/ml

Instrument :
FID_C
ClientSampleId :

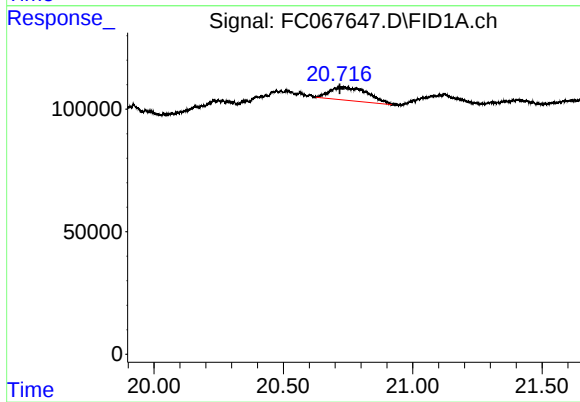

#21 n-Octatriacontane (C38)

R.T.: 20.718 min
Delta R.T.: 0.000 min
Response: 556696
Conc: 6.43 ug/ml