

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110625AL\
 Data File : FC070152.D
 Signal(s) : FID1A.ch
 Acq On : 06 Nov 2025 21:52
 Operator : YP/AJ
 Sample : Q3546-01D
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :
 TP-COMP

Integration File: autoint1.e
 Quant Time: Nov 07 03:05:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 110625.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 06 14:47:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.639	6576219	37.463 ug/ml
Spiked Amount 50.000		Recovery =	74.93%
12) S 1-chlorooctadecane (S...	13.074	5268112	39.402 ug/ml
Spiked Amount 50.000		Recovery =	78.80%
Target Compounds			
14) T n-Tetracosane (C24)	14.921	63180	0.405 ug/ml
16) T n-Octacosane (C28)	16.900	35019	0.241 ug/ml
17) T n-Tricontane (C30)	17.789	178642	1.204 ug/ml
18) T n-Dotriacontane (C32)	18.618	339903	2.336 ug/ml
19) T n-Tetratriacontane (C34)	19.407	95897	0.745 ug/ml
20) T n-Hexatriacontane (C36)	20.147	97519	0.905 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110625AL\
Data File : FC070152.D
Signal(s) : FID1A.ch
Acq On : 06 Nov 2025 21:52
Operator : YP/AJ
Sample : Q3546-01D
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :
TP-COMP

Integration File: autoint1.e
Quant Time: Nov 07 03:05:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 110625.M
Quant Title : GC Extractables
QLast Update : Thu Nov 06 14:47:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

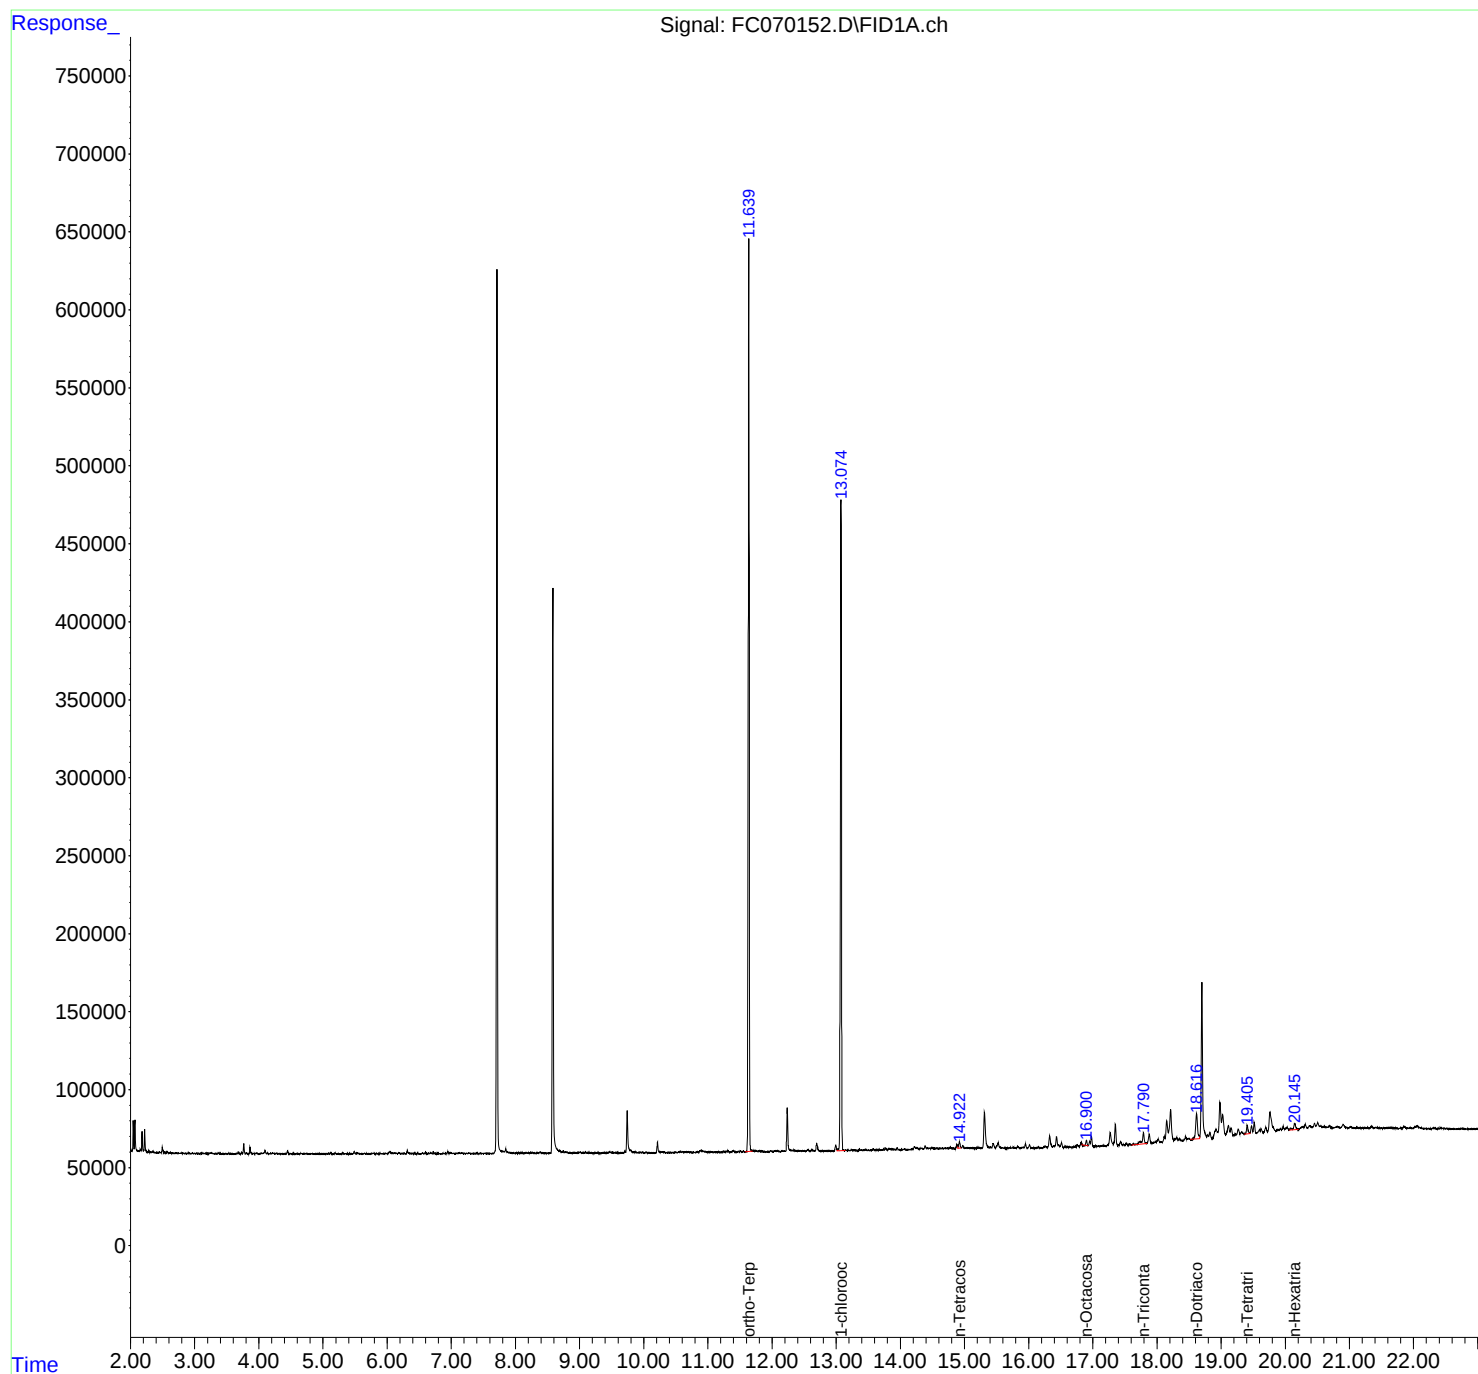


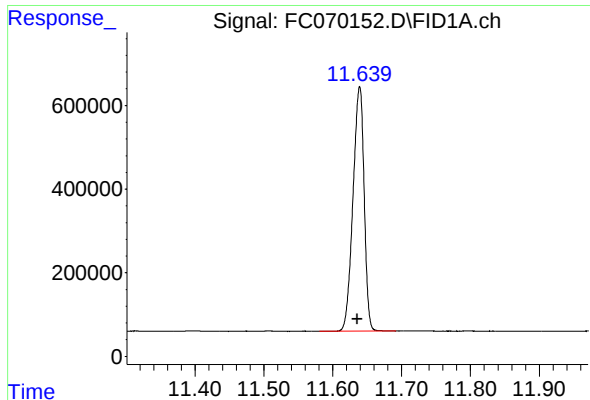

#9 ortho-Terphenyl (SURR)


R.T.: 11.639 min
Delta R.T.: 0.003 min
Response: 6576219
Conc: 37.46 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-COMP

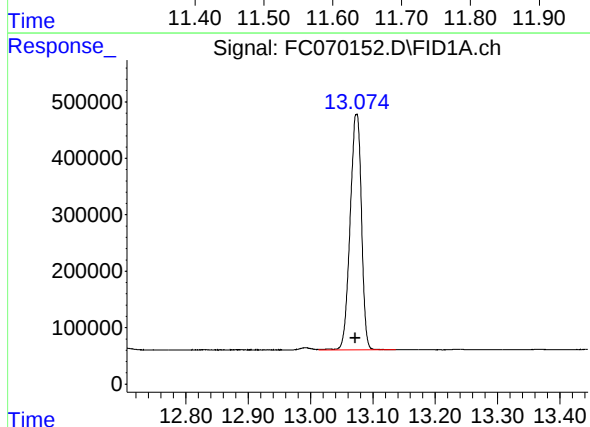


#12 1-chlorooctadecane (SURR)

R.T.: 13.074 min
Delta R.T.: 0.002 min
Response: 5268112
Conc: 39.40 ug/ml

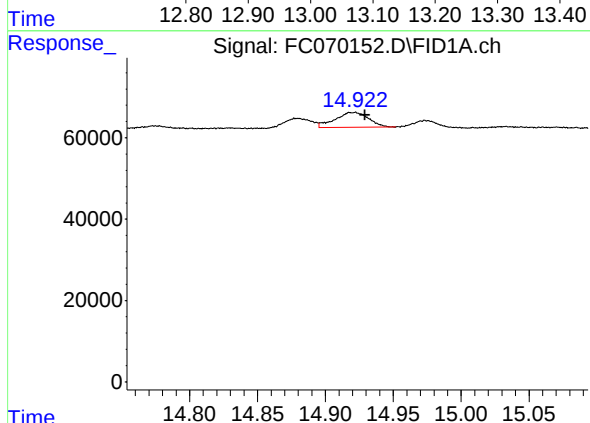


#14 n-Tetracosane (C24)

R.T.: 14.921 min
Delta R.T.: -0.008 min
Response: 63180
Conc: 0.41 ug/ml

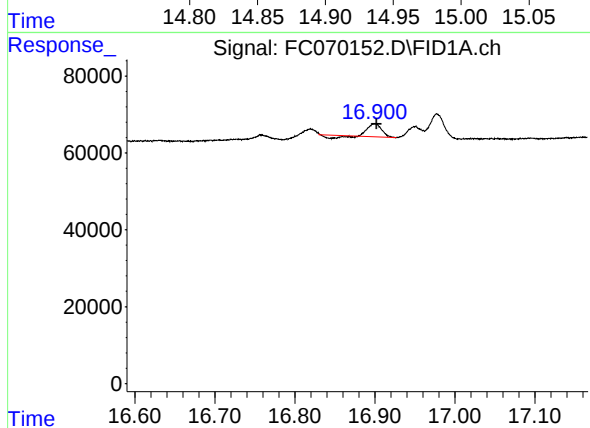

#16 n-Octacosane (C28)


R.T.: 16.900 min
Delta R.T.: -0.002 min
Response: 35019
Conc: 0.24 ug/ml

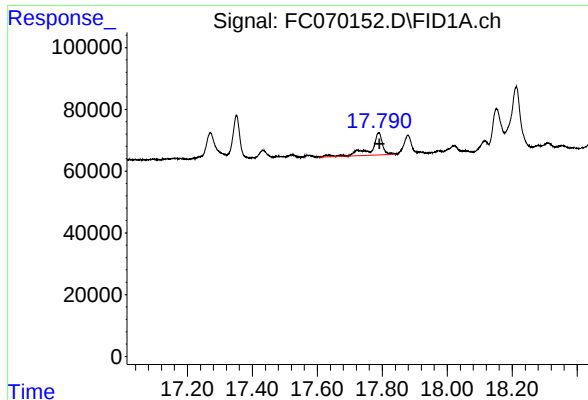

#17 n-Tricontane (C30)


R.T.: 17.789 min
Delta R.T.: -0.003 min
Response: 178642
Conc: 1.20 ug/ml

Instrument :
FID_C
ClientSampleId :
TP-COMP

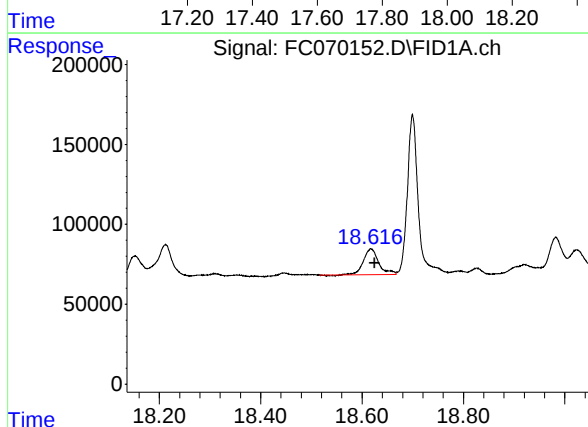


#18 n-Dotriacontane (C32)

R.T.: 18.618 min
Delta R.T.: -0.008 min
Response: 339903
Conc: 2.34 ug/ml

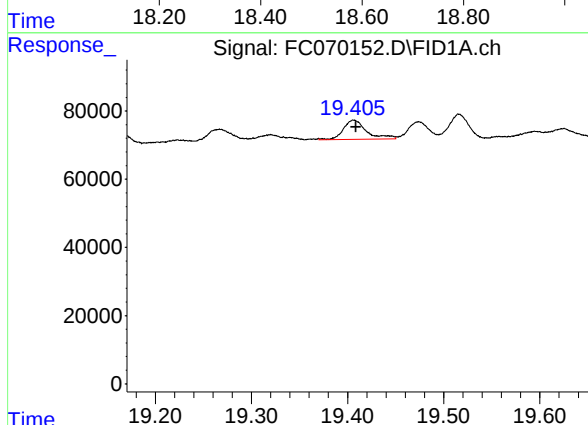

#19 n-Tetratriacontane (C34)

R.T.: 19.407 min
Delta R.T.: -0.002 min
Response: 95897
Conc: 0.75 ug/ml

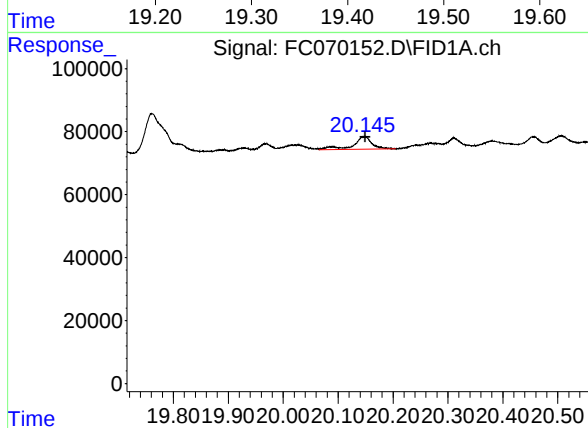

#20 n-Hexatriacontane (C36)

R.T.: 20.147 min
Delta R.T.: -0.002 min
Response: 97519
Conc: 0.90 ug/ml