

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110723AL\
 Data File : FC065025.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2023 10:23
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 07 22:01:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.497	85724	0.477 ug/ml
11) T n-Heneicosane (C21)	13.110	72921	0.415 ug/ml
13) T n-Docosane (C22)	13.693	70061	0.408 ug/ml
14) T n-Tetracosane (C24)	14.790	57655	0.346 ug/ml
15) T n-Hexacosane (C26)	15.808	54809	0.341 ug/ml
16) T n-Octacosane (C28)	16.754	55336	0.354 ug/ml
17) T n-Tricontane (C30)	17.639	70884	0.448 ug/ml
18) T n-Dotriacontane (C32)	18.464	99876	0.633 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110723AL\
Data File : FC065025.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2023 10:23
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 07 22:01:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

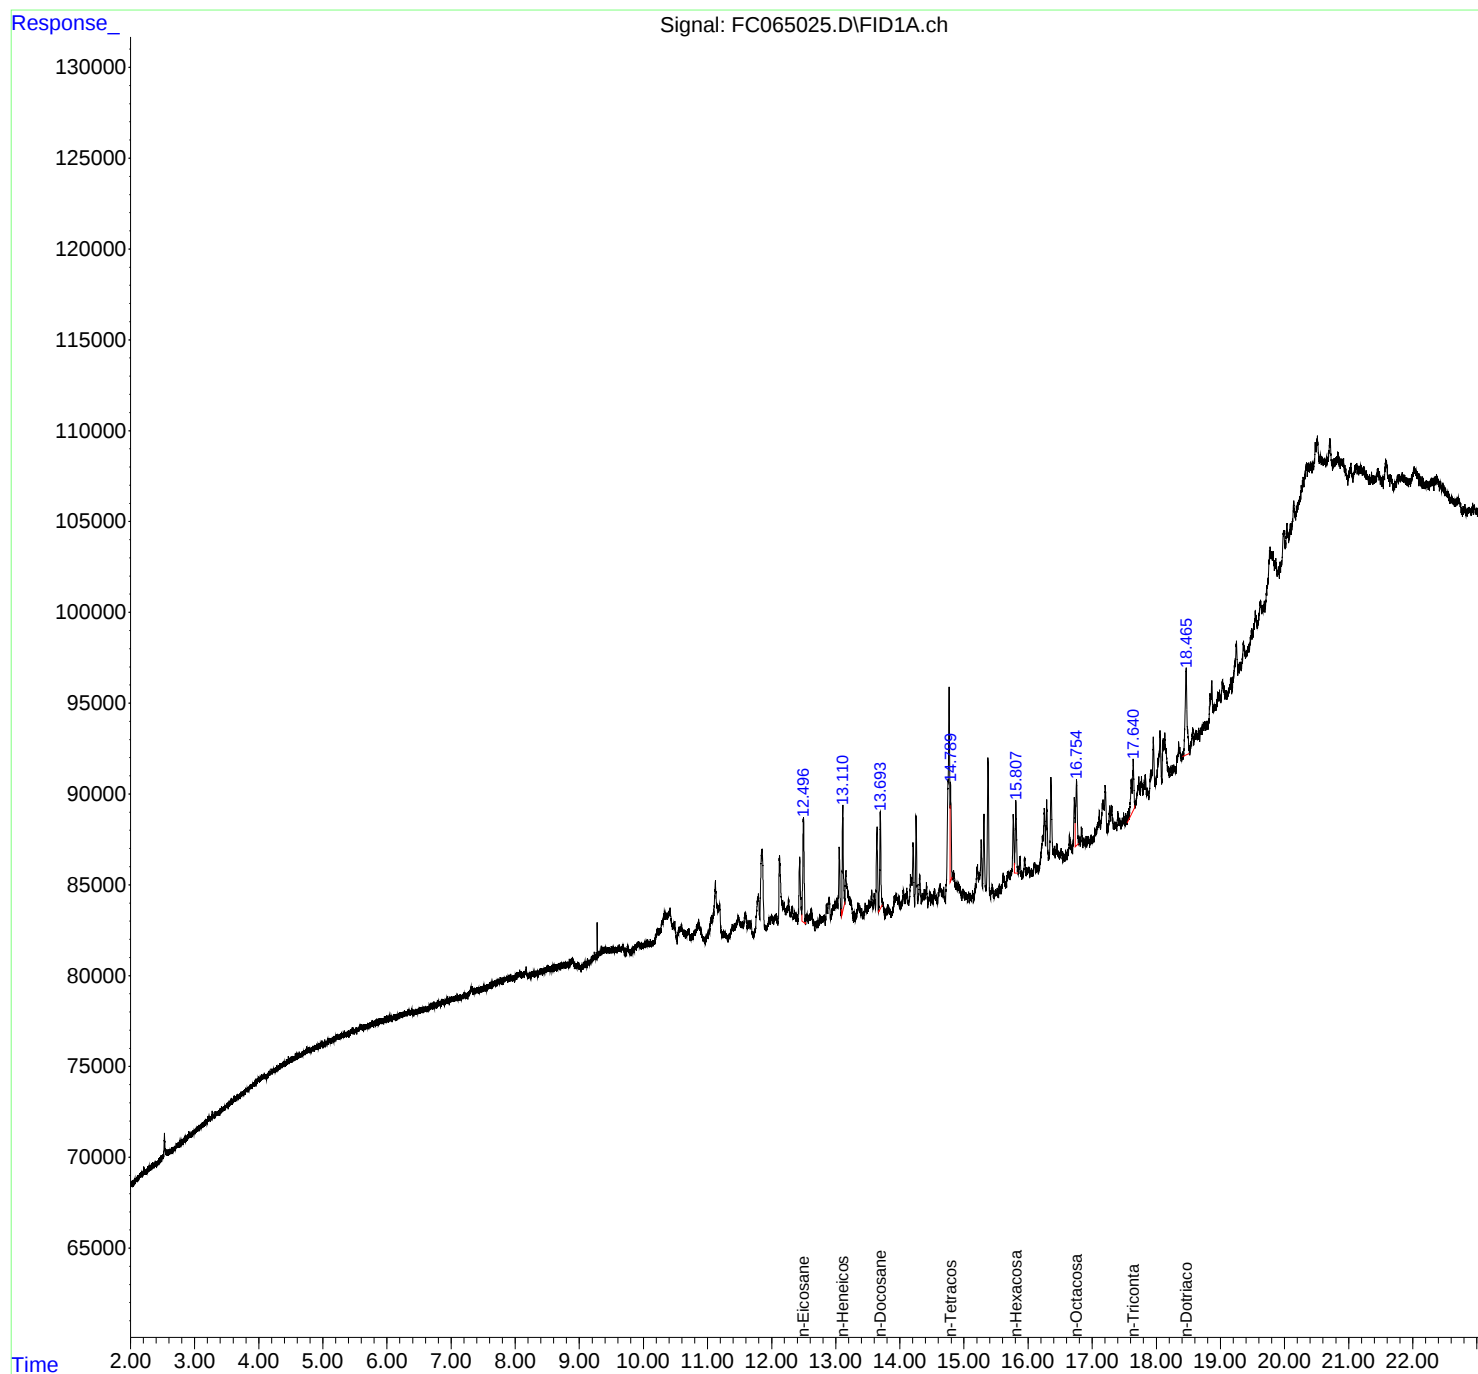


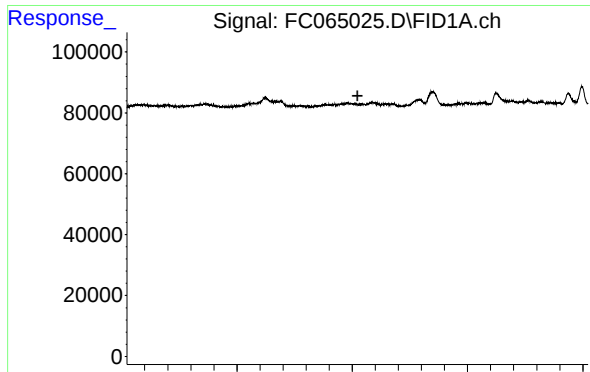

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

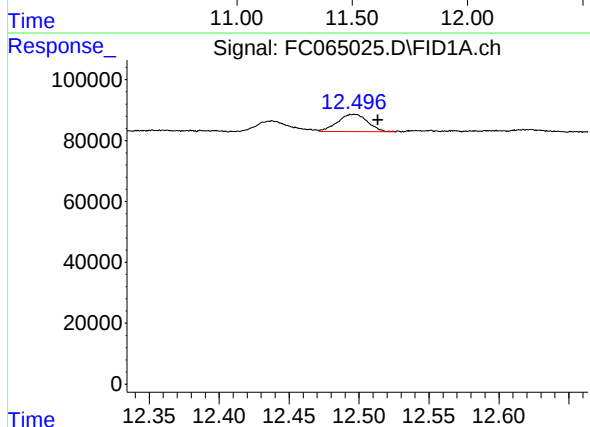


#10 n-Eicosane (C20)

R.T.: 12.497 min
Delta R.T.: -0.017 min
Response: 85724
Conc: 0.48 ug/ml

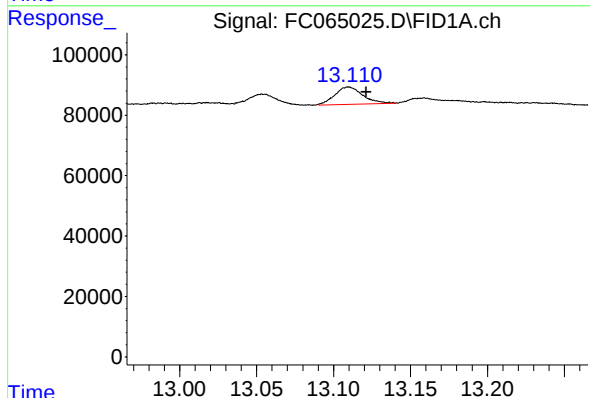


#11 n-Heneicosane (C21)

R.T.: 13.110 min
Delta R.T.: -0.012 min
Response: 72921
Conc: 0.42 ug/ml

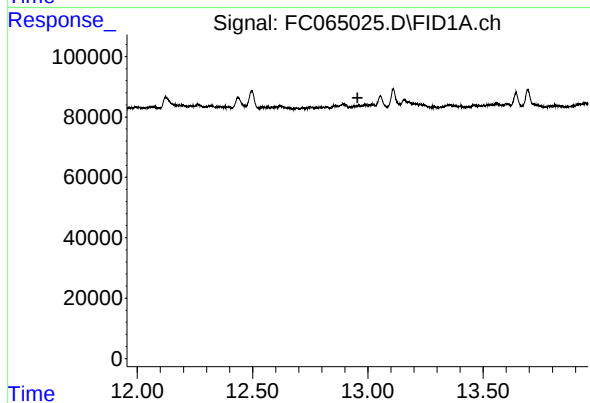

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

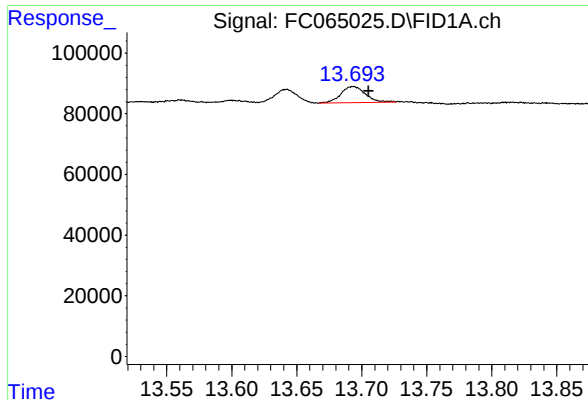

#13 n-Docosane (C22)


R.T.: 13.693 min
Delta R.T.: -0.012 min
Response: 70061
Conc: 0.41 ug/ml

Instrument :
FID_C
ClientSampleId :

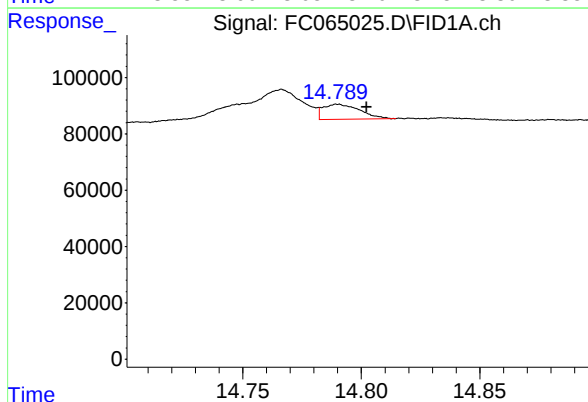


#14 n-Tetracosane (C24)

R.T.: 14.790 min
Delta R.T.: -0.012 min
Response: 57655
Conc: 0.35 ug/ml

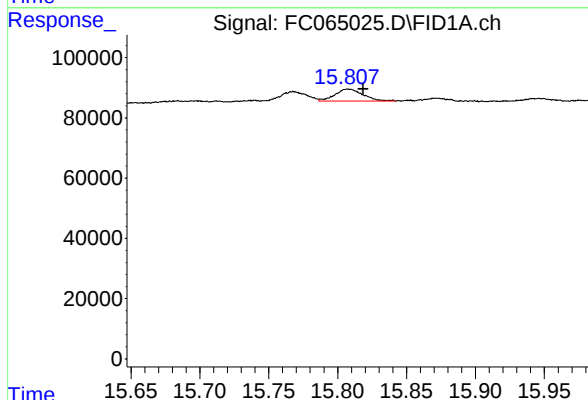


#15 n-Hexacosane (C26)

R.T.: 15.808 min
Delta R.T.: -0.011 min
Response: 54809
Conc: 0.34 ug/ml

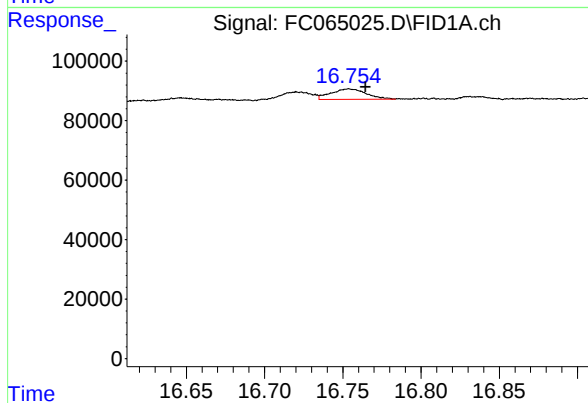

#16 n-Octacosane (C28)


R.T.: 16.754 min
Delta R.T.: -0.011 min
Response: 55336
Conc: 0.35 ug/ml

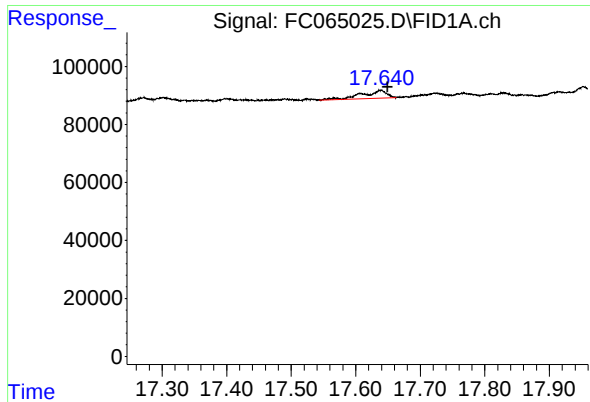

#17 n-Tricontane (C30)

R.T.: 17.639 min
Delta R.T.: -0.011 min
Response: 70884
Conc: 0.45 ug/ml

Instrument :
FID_C
ClientSampleId :

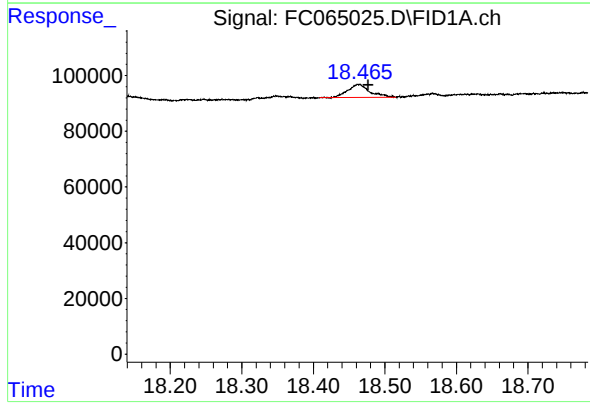

#18 n-Dotriacontane (C32)

R.T.: 18.464 min
Delta R.T.: -0.013 min
Response: 99876
Conc: 0.63 ug/ml