

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110923AL\
 Data File : FC065090.D
 Signal(s) : FID1A.ch
 Acq On : 10 Nov 2023 02:55
 Operator : YP/AJ
 Sample : 05394-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 10 04:29:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.942	7974473	50.444 ug/ml
Spiked Amount 50.000		Recovery =	100.89%
Target Compounds			
4) T n-Dodecane (C12)	6.380	68552	0.355 ug/ml
20) T n-Hexatriacontane (C36)	19.982	52312	0.347 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110923AL\
Data File : FC065090.D
Signal(s) : FID1A.ch
Acq On : 10 Nov 2023 02:55
Operator : YP/AJ
Sample : 05394-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 04:29:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

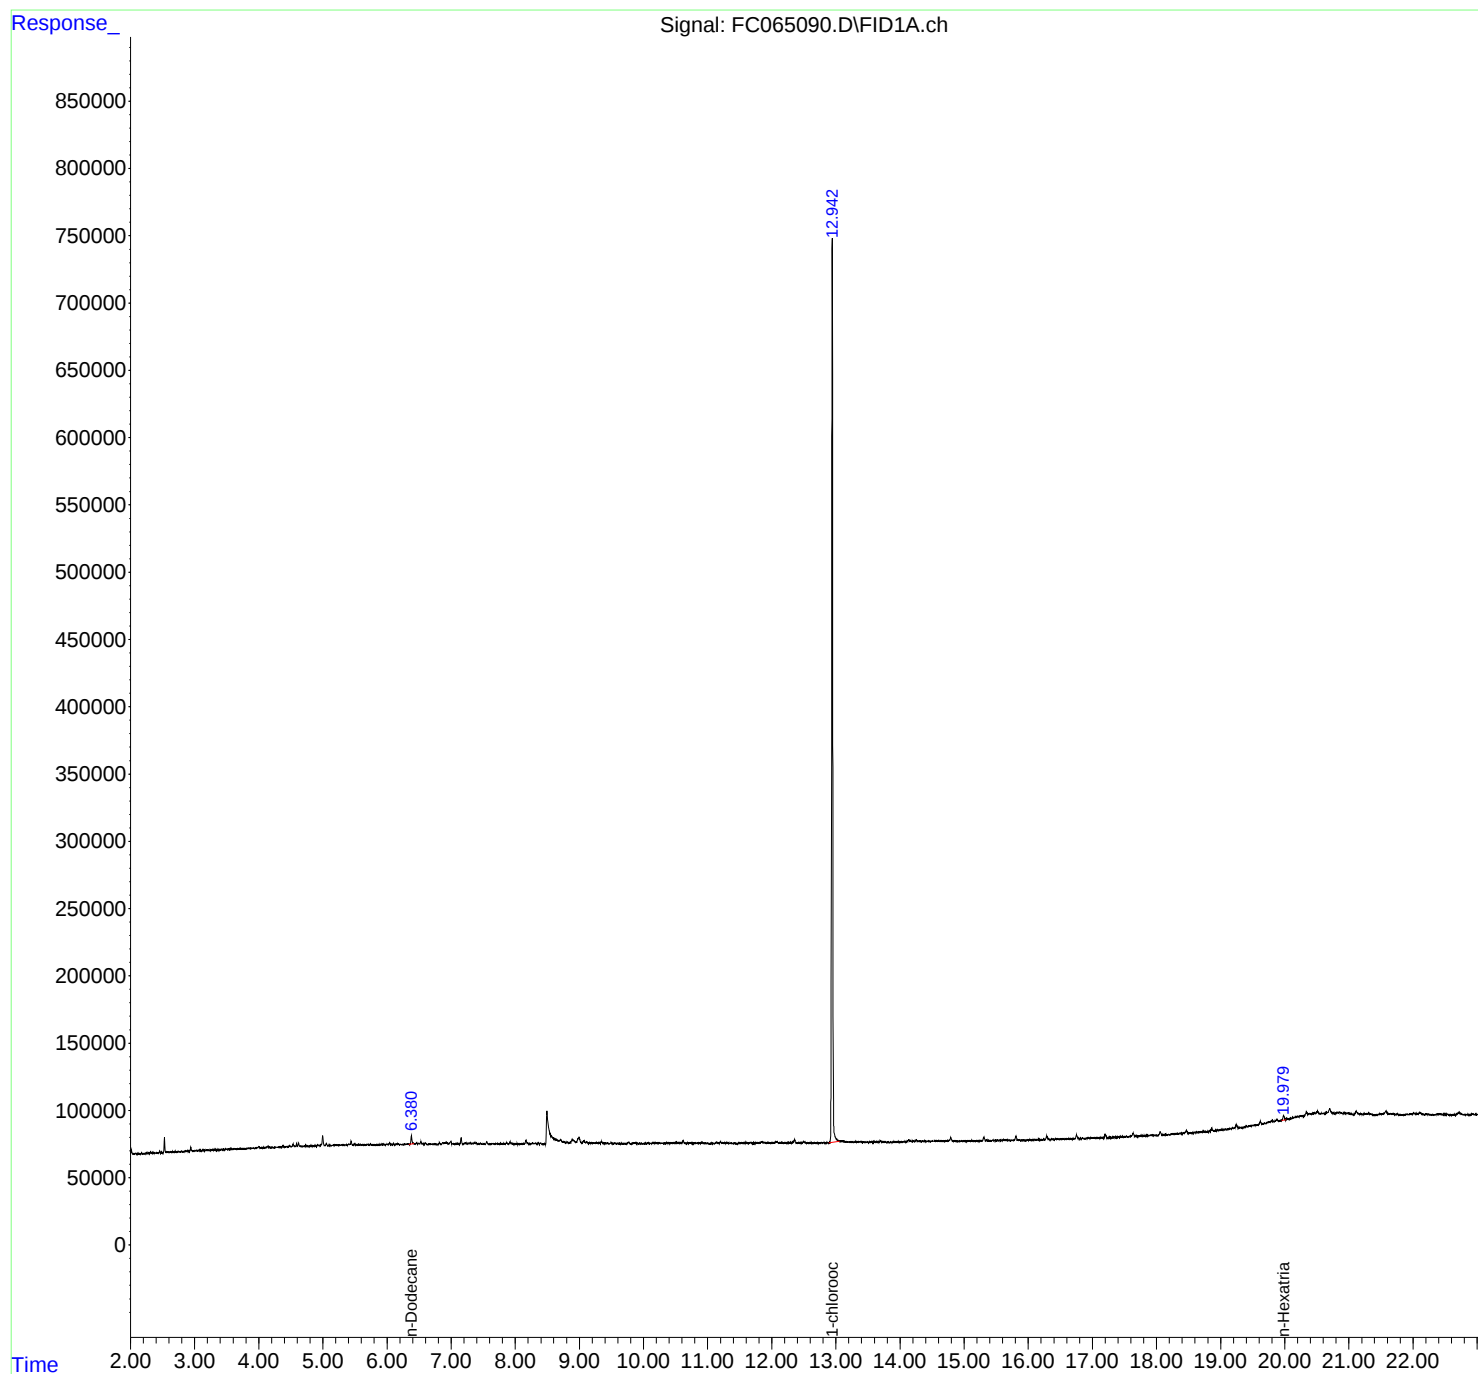


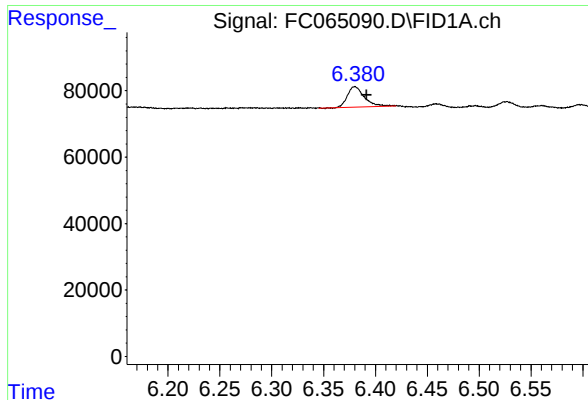

#4 n-Dodecane (C12)


R.T.: 6.380 min
Delta R.T.: -0.012 min
Response: 68552
Conc: 0.35 ug/ml

Instrument :
FID_C
ClientSampleId :

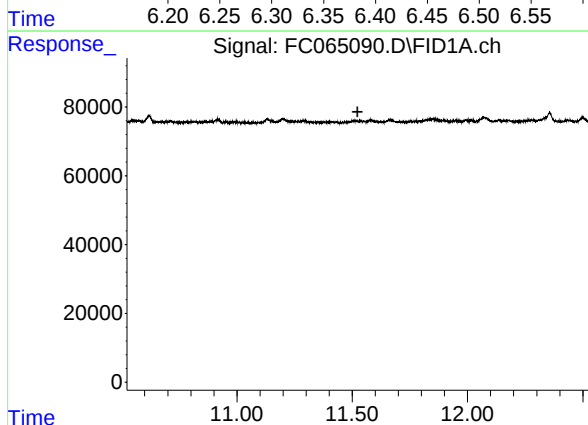


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

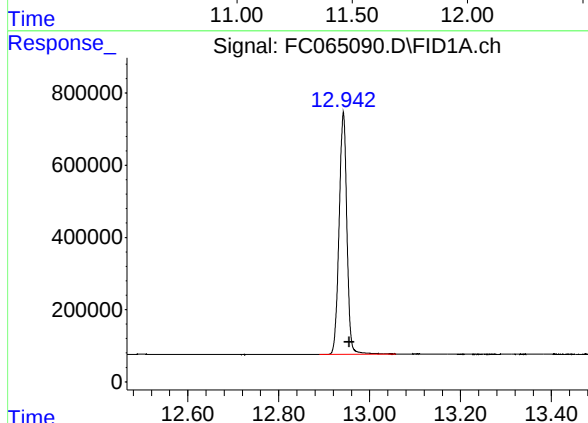

#12 1-chlorooctadecane (SURR)

R.T.: 12.942 min
Delta R.T.: -0.012 min
Response: 7974473
Conc: 50.44 ug/ml

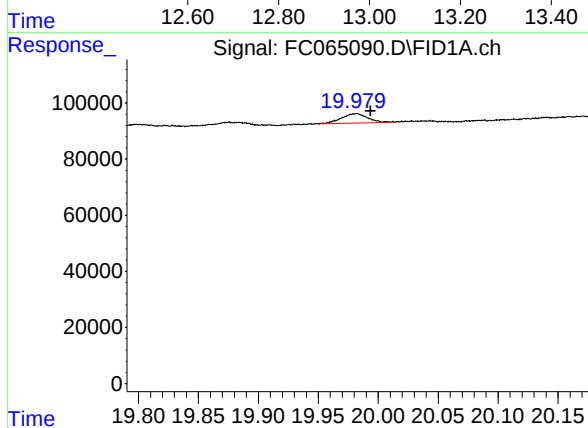

#20 n-Hexatriacontane (C36)

R.T.: 19.982 min
Delta R.T.: -0.012 min
Response: 52312
Conc: 0.35 ug/ml