

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110923AL\
 Data File : FC065091.D
 Signal(s) : FID1A.ch
 Acq On : 10 Nov 2023 03:33
 Operator : YP/AJ
 Sample : 05394-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 10 04:29:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.944	7841910	49.606 ug/ml
Spiked Amount 50.000		Recovery =	99.21%
Target Compounds			
4) T n-Dodecane (C12)	6.381	46490	0.241 ug/ml
16) T n-Octacosane (C28)	16.753	50517	0.323 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC110923AL\
Data File : FC065091.D
Signal(s) : FID1A.ch
Acq On : 10 Nov 2023 03:33
Operator : YP/AJ
Sample : 05394-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 04:29:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

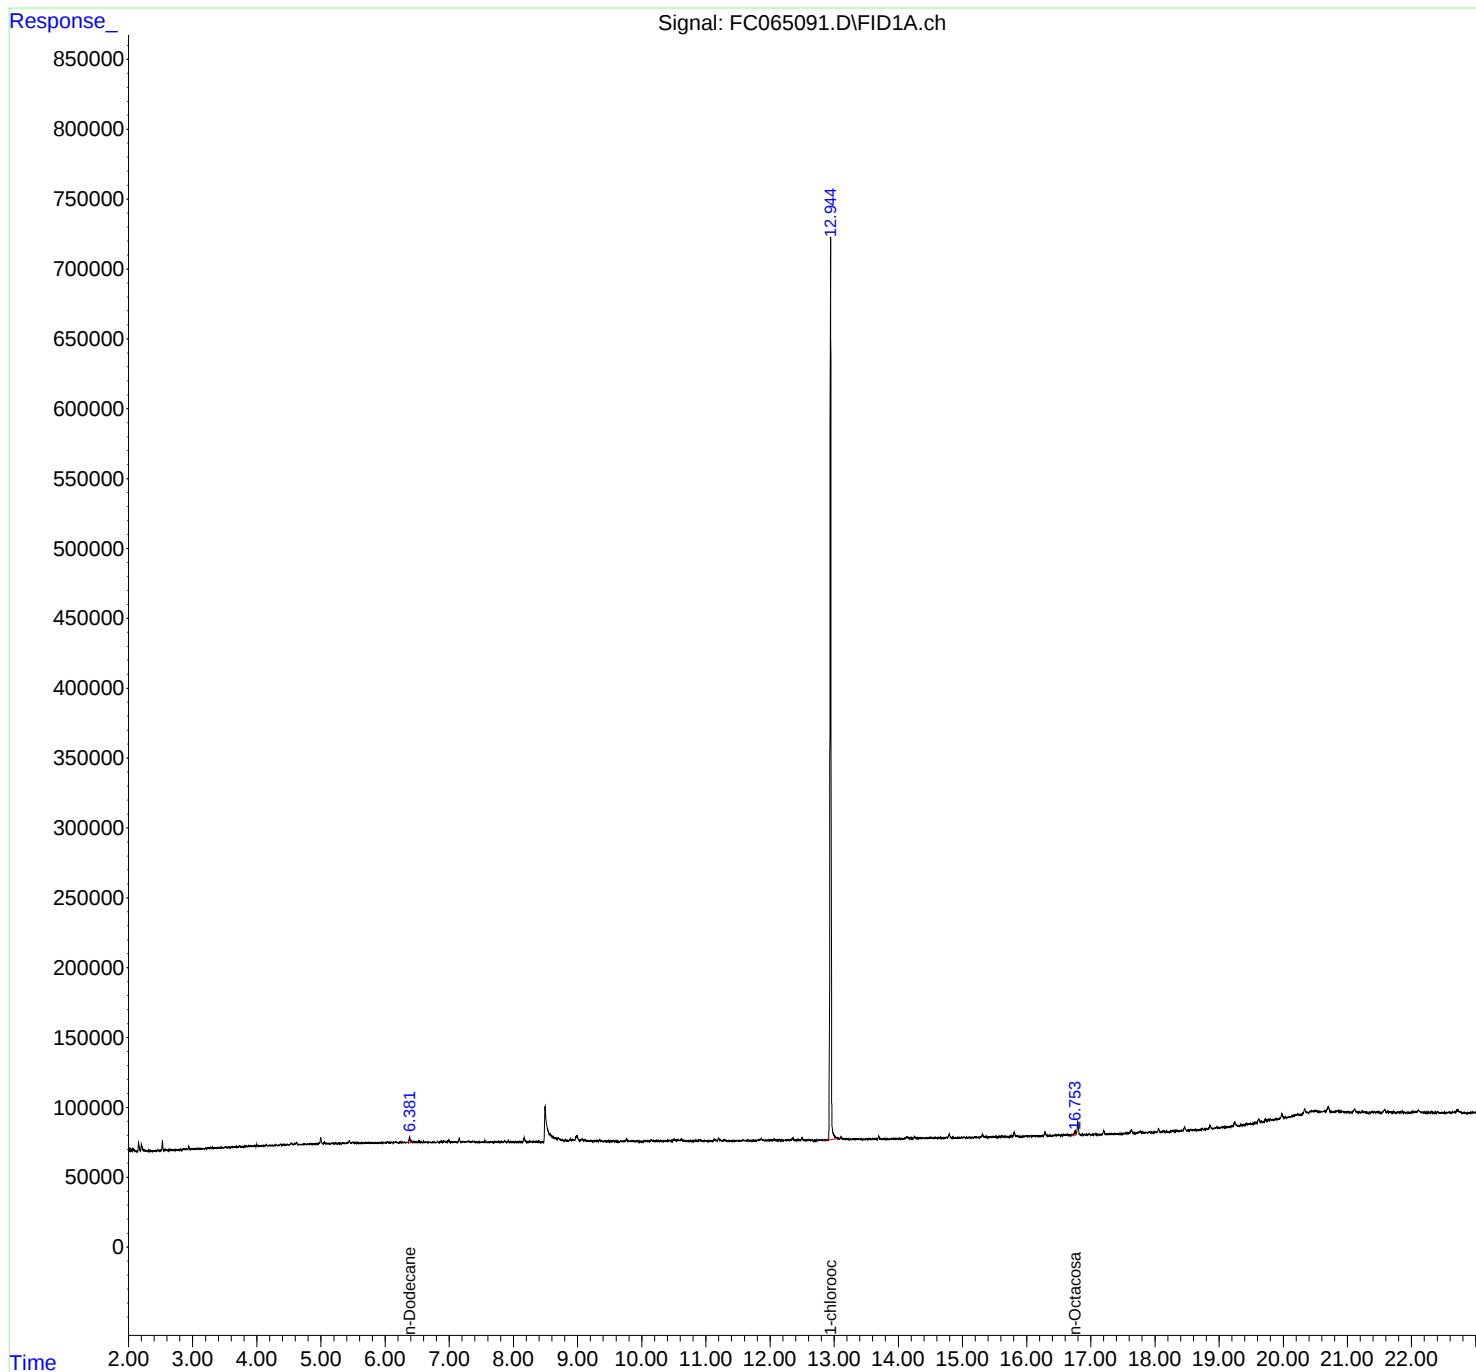

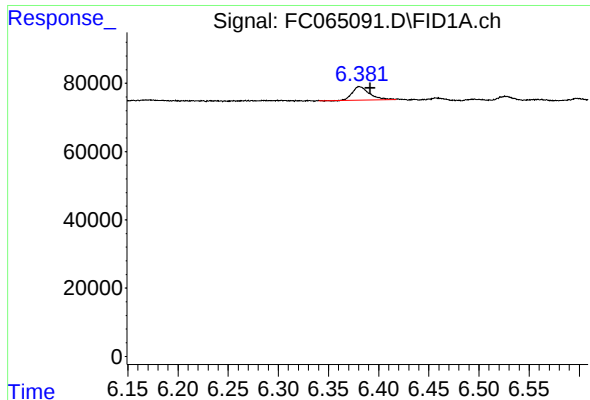


#4 n-Dodecane (C12)

R.T.: 6.381 min
Delta R.T.: -0.011 min
Response: 46490
Conc: 0.24 ug/ml

Instrument :


FID_C

ClientSampleId :

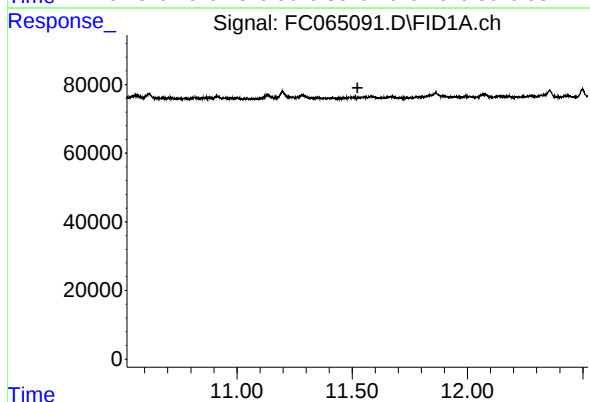


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

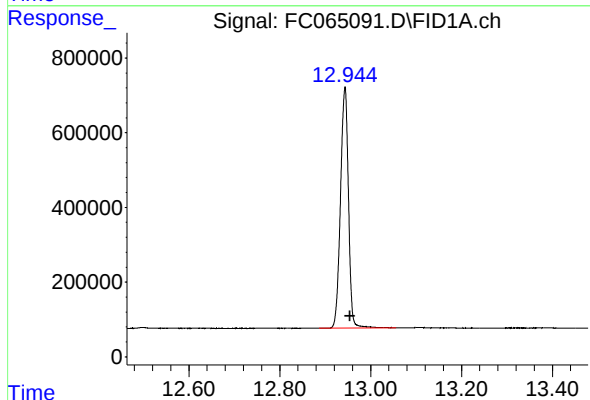

#12 1-chlorooctadecane (SURRE)

R.T.: 12.944 min
Delta R.T.: -0.011 min
Response: 7841910
Conc: 49.61 ug/ml

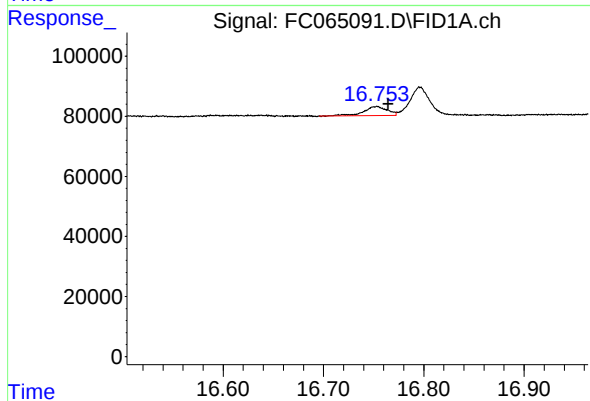

#16 n-Octacosane (C28)

R.T.: 16.753 min
Delta R.T.: -0.011 min
Response: 50517
Conc: 0.32 ug/ml