

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111323AL\
 Data File : FC065115.D
 Signal(s) : FID1A.ch
 Acq On : 13 Nov 2023 08:07
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 13 23:16:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.089	332545	1.894 ug/ml
13) T n-Docosane (C22)	13.681	327541	1.907 ug/ml
14) T n-Tetracosane (C24)	14.783	282848	1.698 ug/ml
15) T n-Hexacosane (C26)	15.800	211734	1.319 ug/ml
16) T n-Octacosane (C28)	16.746	170650	1.090 ug/ml
17) T n-Tricontane (C30)	17.629	106480	0.672 ug/ml
18) T n-Dotriacontane (C32)	18.456	237379	1.503 ug/ml
19) T n-Tetratriacontane (C34)	19.236	201179	1.318 ug/ml
20) T n-Hexatriacontane (C36)	19.976	59113	0.392 ug/ml
21) T n-Octatriacontane (C38)	20.692	95577	0.642 ug/ml
22) T n-Tetracontane (C40)	21.565	81757	0.556 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111323AL\
Data File : FC065115.D
Signal(s) : FID1A.ch
Acq On : 13 Nov 2023 08:07
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 13 23:16:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

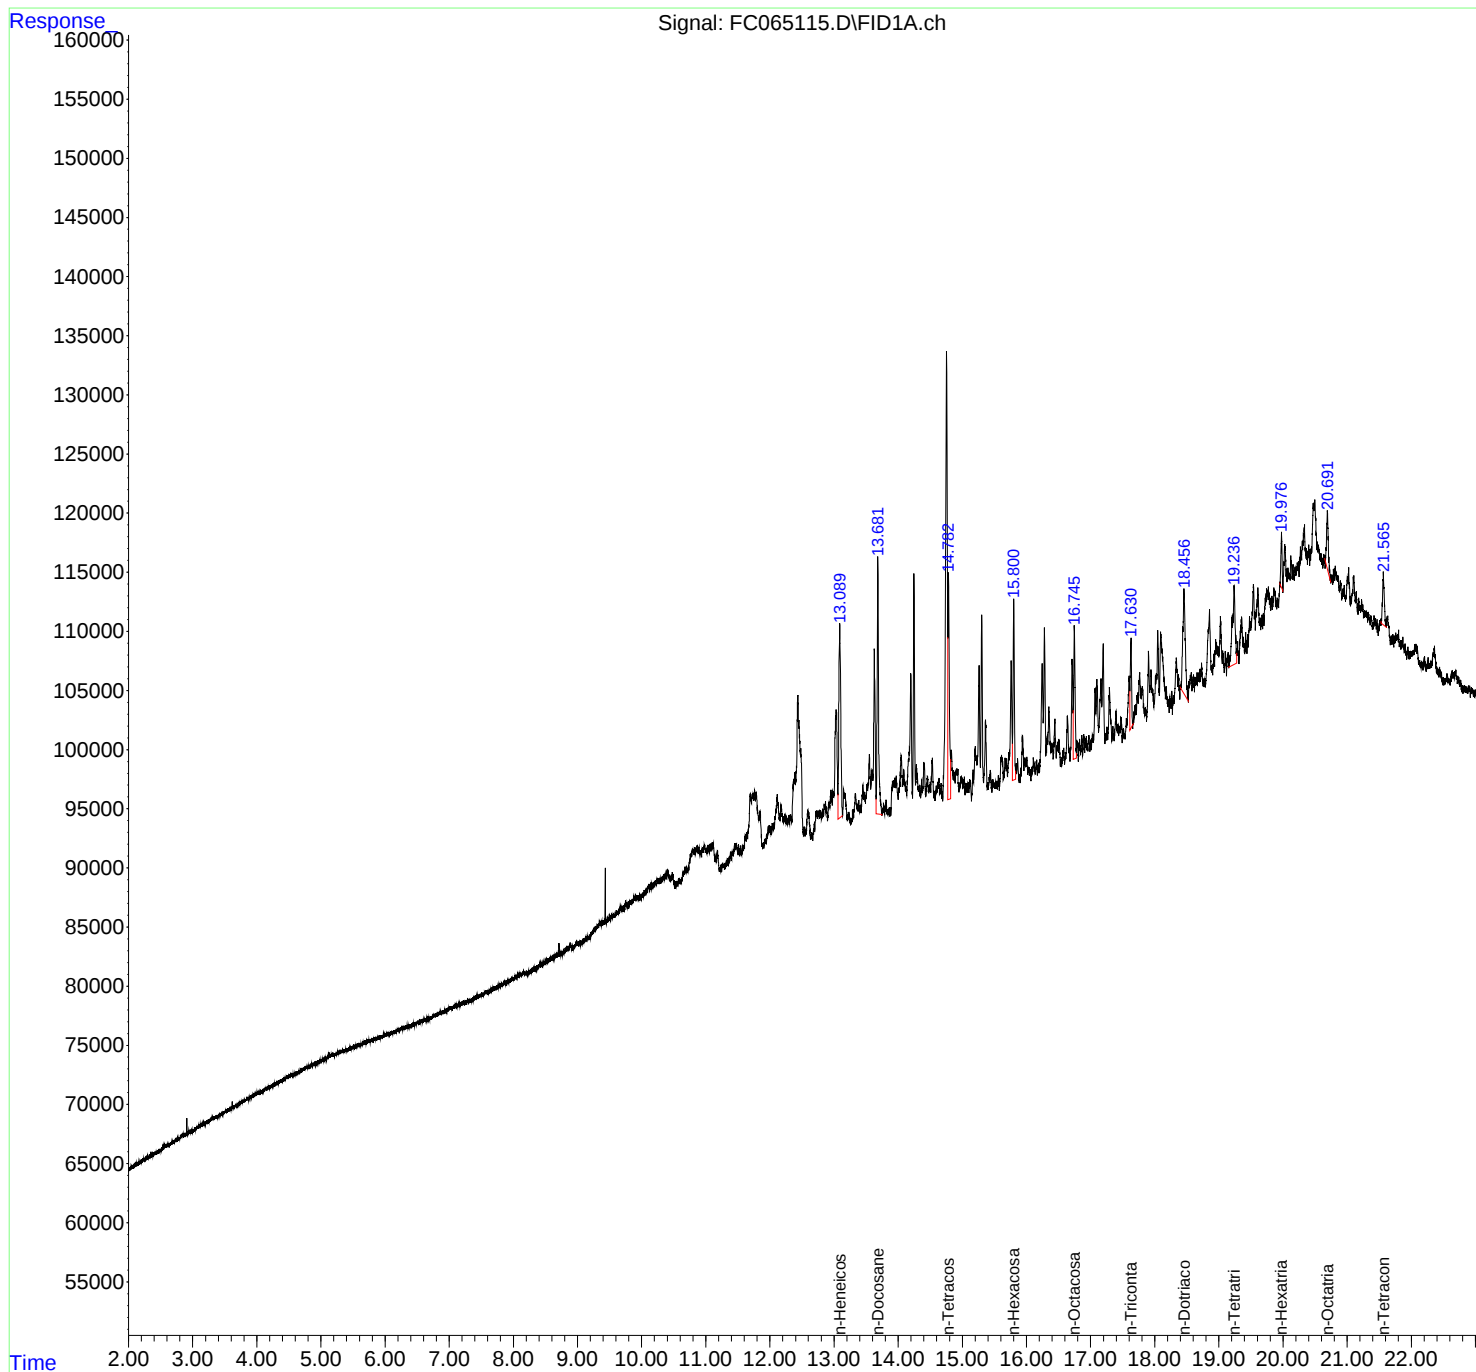


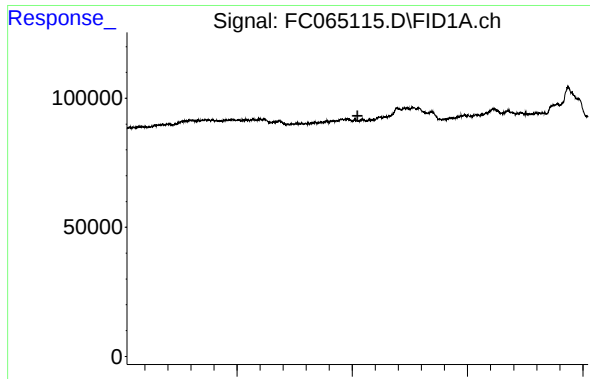

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

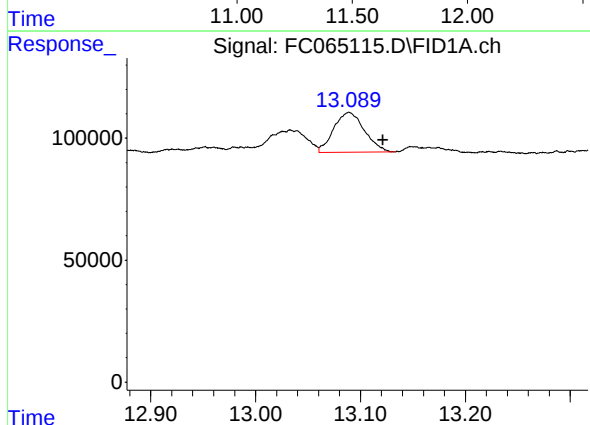


#11 n-Heneicosane (C21)

R.T.: 13.089 min
Delta R.T.: -0.032 min
Response: 332545
Conc: 1.89 ug/ml

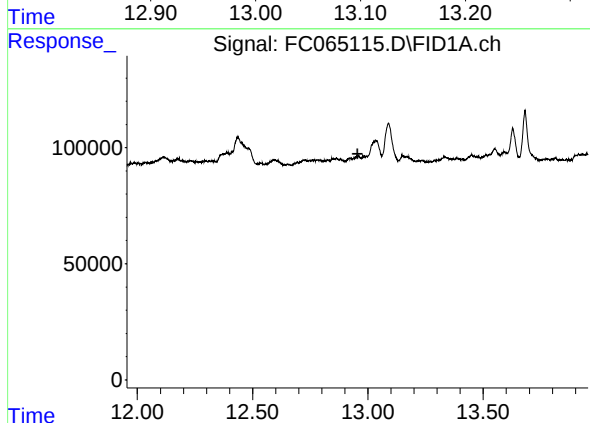


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

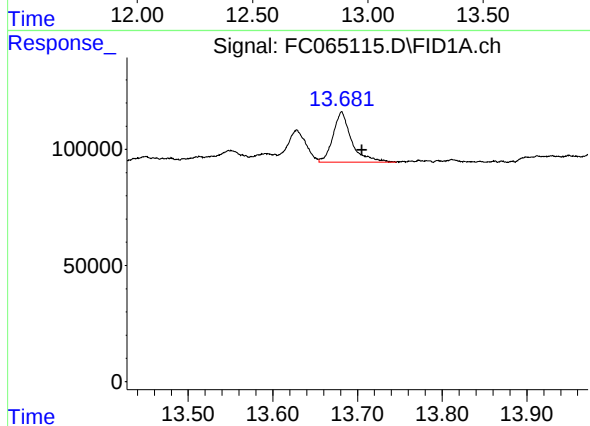

#13 n-Docosane (C22)


R.T.: 13.681 min
Delta R.T.: -0.024 min
Response: 327541
Conc: 1.91 ug/ml

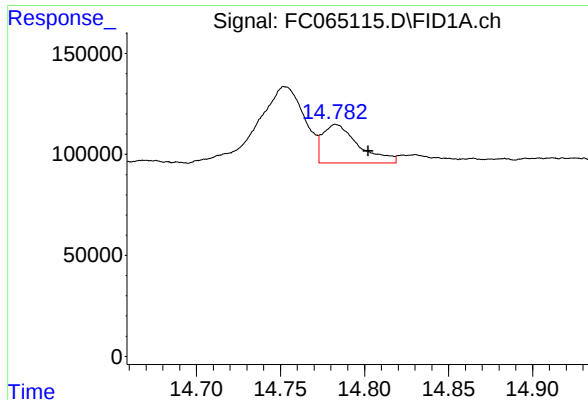

#14 n-Tetracosane (C24)


R.T.: 14.783 min
Delta R.T.: -0.019 min
Response: 282848
Conc: 1.70 ug/ml

Instrument :
FID_C
ClientSampleId :

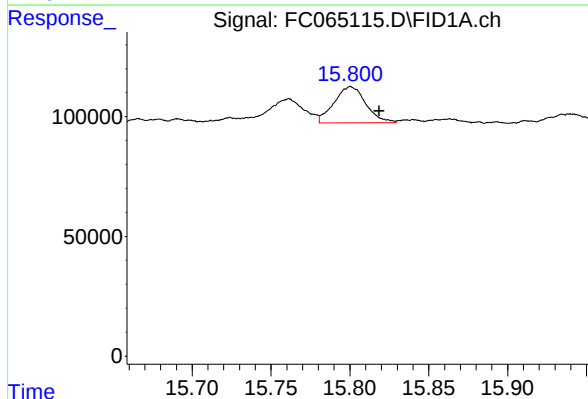


#15 n-Hexacosane (C26)

R.T.: 15.800 min
Delta R.T.: -0.018 min
Response: 211734
Conc: 1.32 ug/ml

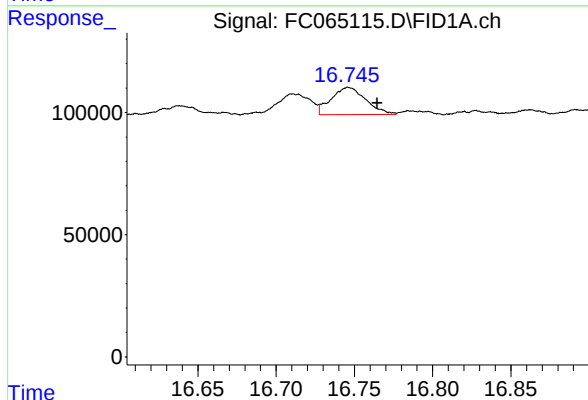


#16 n-Octacosane (C28)

R.T.: 16.746 min
Delta R.T.: -0.018 min
Response: 170650
Conc: 1.09 ug/ml

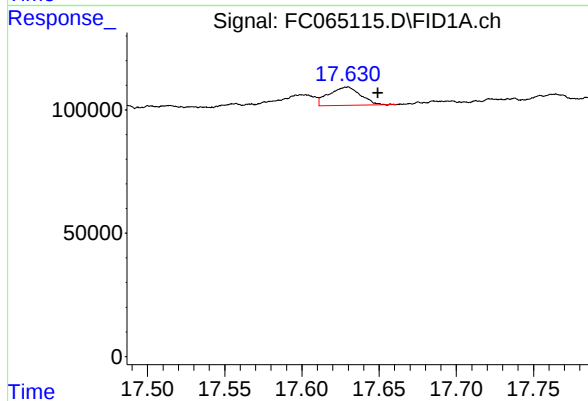

#17 n-Tricontane (C30)


R.T.: 17.629 min
Delta R.T.: -0.020 min
Response: 106480
Conc: 0.67 ug/ml

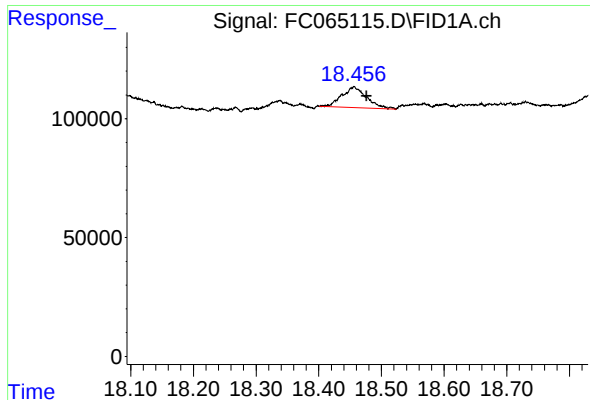

#18 n-Dotriacontane (C32)


R.T.: 18.456 min
Delta R.T.: -0.020 min
Response: 237379
Conc: 1.50 ug/ml

Instrument :
FID_C
ClientSampleId :

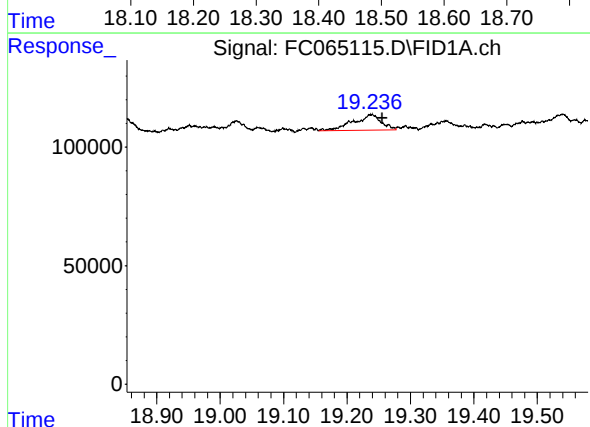


#19 n-Tetratriacontane (C34)

R.T.: 19.236 min
Delta R.T.: -0.020 min
Response: 201179
Conc: 1.32 ug/ml

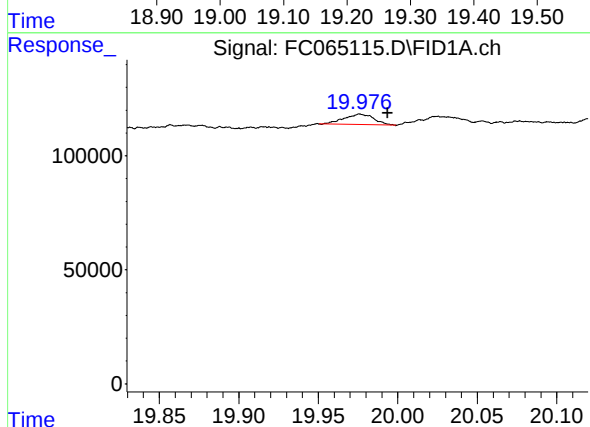


#20 n-Hexatriacontane (C36)

R.T.: 19.976 min
Delta R.T.: -0.017 min
Response: 59113
Conc: 0.39 ug/ml

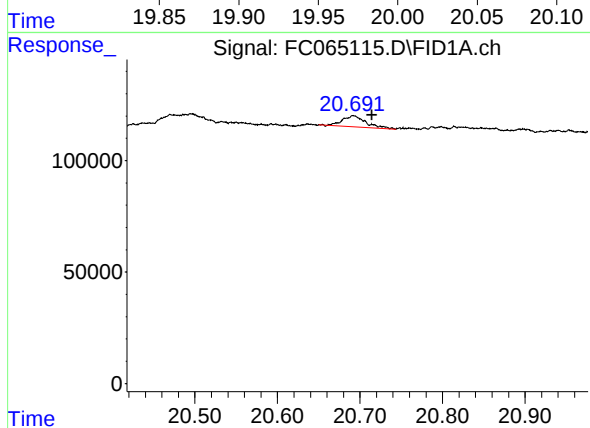

#21 n-Octatriacontane (C38)

R.T.: 20.692 min
Delta R.T.: -0.022 min
Response: 95577
Conc: 0.64 ug/ml

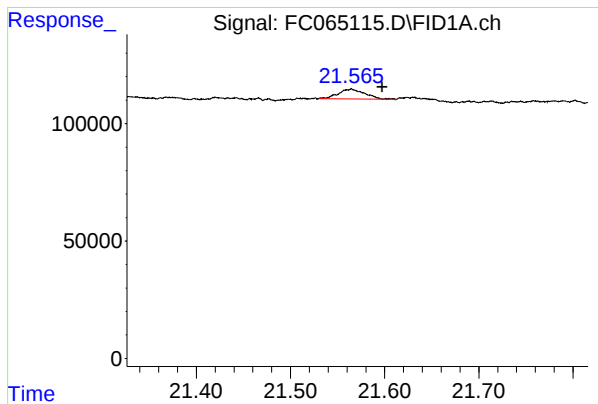

#22 n-Tetracontane (C40)

R.T.: 21.565 min
Delta R.T.: -0.033 min
Response: 81757
Conc: 0.56 ug/ml

Instrument :

FID_C

ClientSampleId :