

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC111423AL\  
 Data File : FC065142.D  
 Signal(s) : FID1A.ch  
 Acq On : 14 Nov 2023 17:02  
 Operator : YP/AJ  
 Sample : 05388-02D  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 TP-3-EPH

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 11/15/2023  
 Supervised By :Ankita Jodhani 11/15/2023

Integration File: autoint1.e  
 Quant Time: Nov 14 21:29:14 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 102823.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Oct 28 02:12:00 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 11.508 | 7339645    | 33.349 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 66.70%        |
| 12) S 1-chlorooctadecane (S... | 12.939 | 5519601    | 34.916 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 69.83%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC111423AL\  
Data File : FC065142.D  
Signal(s) : FID1A.ch  
Acq On : 14 Nov 2023 17:02  
Operator : YP/AJ  
Sample : 05388-02D  
Misc :  
ALS Vial : 15 Sample Multiplier: 1


Instrument :  
FID\_C  
ClientSampleId :  
TP-3-EPH


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/15/2023  
Supervised By :Ankita Jodhani 11/15/2023

Integration File: autoint1.e  
Quant Time: Nov 14 21:29:14 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 102823.M  
Quant Title : GC Extractables  
QLast Update : Sat Oct 28 02:12:00 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

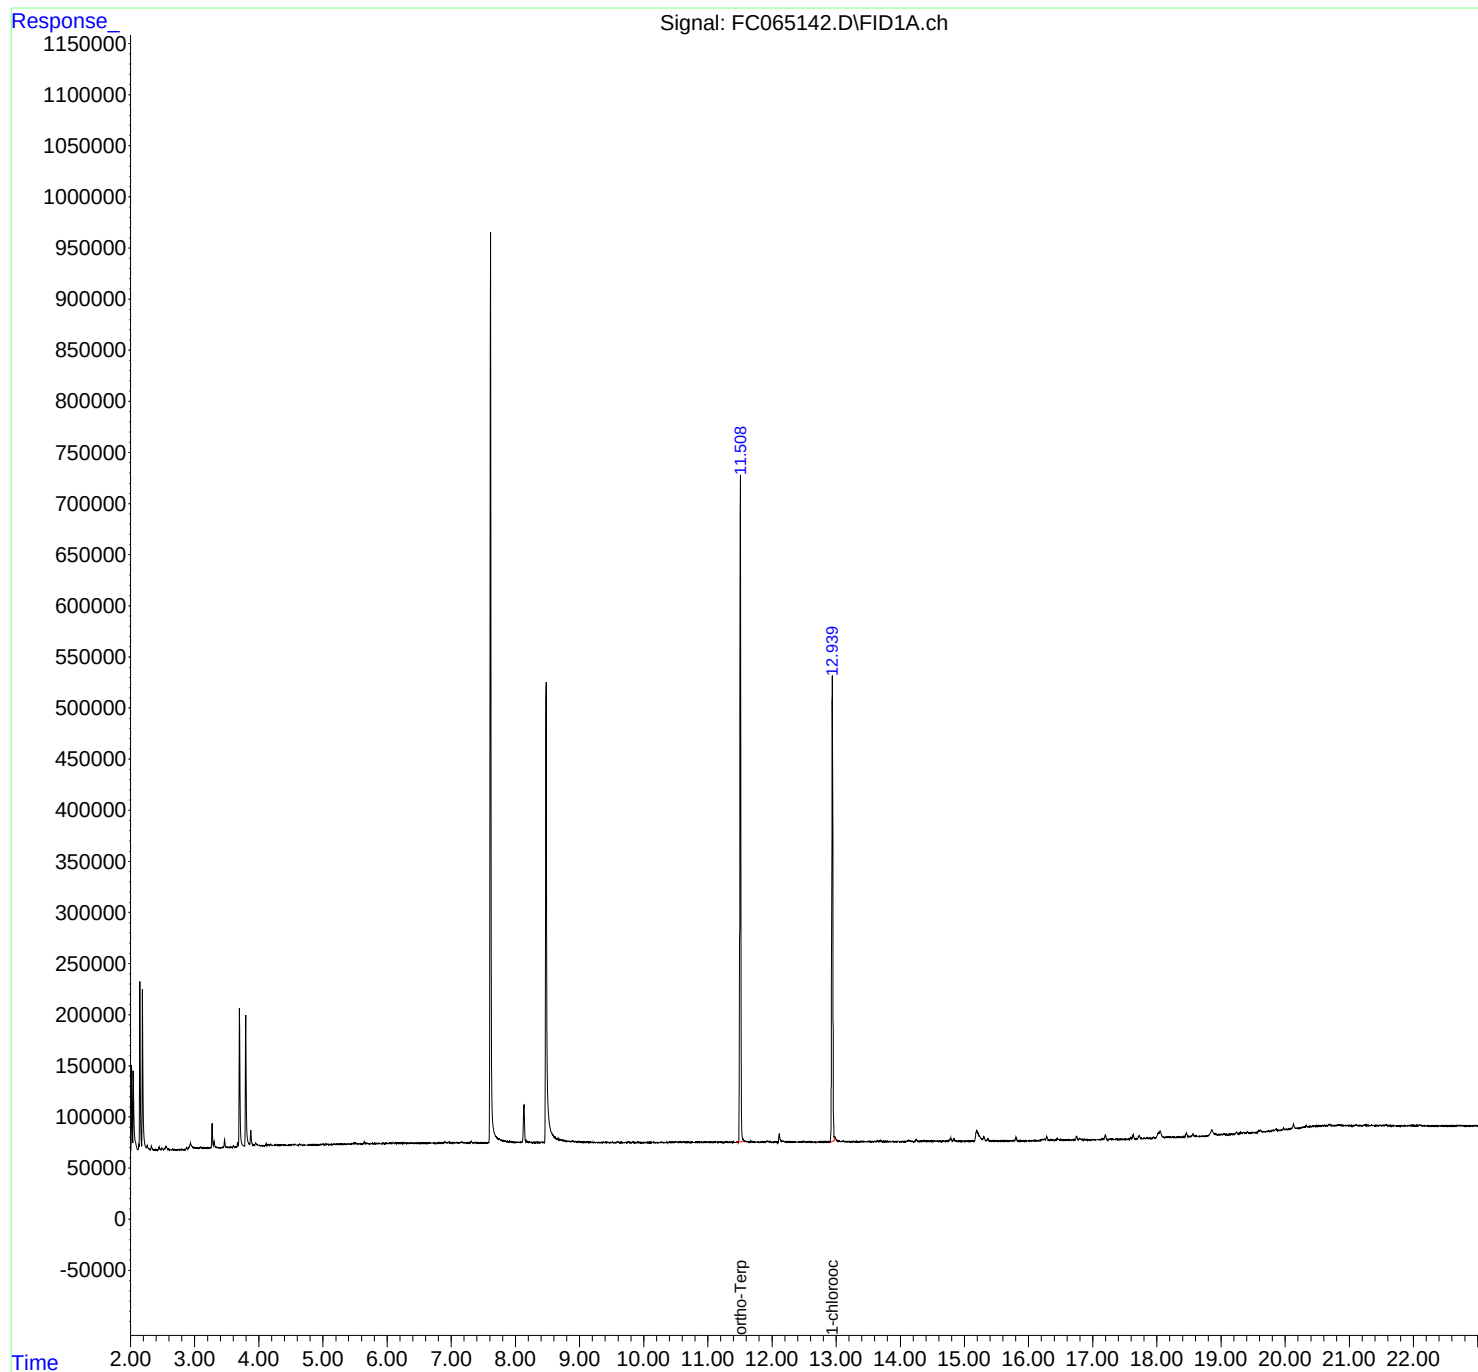

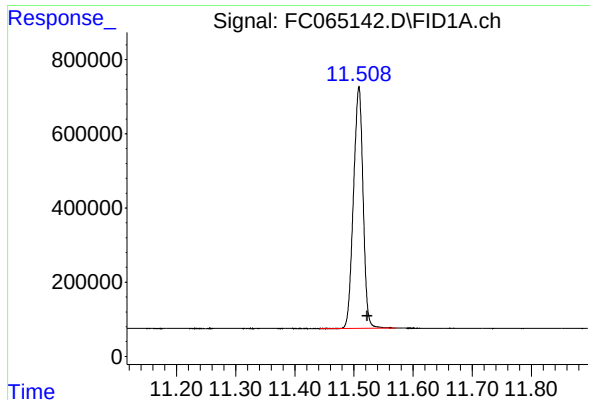


#9 ortho-Terphenyl (SURR)

R.T.: 11.508 min  
Delta R.T.: -0.015 min  
Response: 7339645  
Conc: 33.35 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
TP-3-EPH

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/15/2023  
Supervised By :Ankita Jodhani 11/15/2023

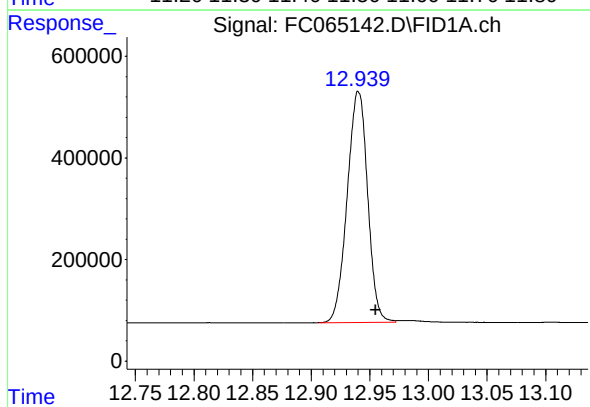

#12 1-chlorooctadecane (SURR)

R.T.: 12.939 min  
Delta R.T.: -0.016 min  
Response: 5519601  
Conc: 34.92 ug/ml m