

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111723AL\
Data File : FC065180.D
Signal(s) : FID1A.ch
Acq On : 17 Nov 2023 06:18
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 17 21:32:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	14.760	9956	0.060 ug/ml
18) T	n-Dotriacontane (C32)	18.454	66268	0.420 ug/ml
20) T	n-Hexatriacontane (C36)	19.976	100455	0.666 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111723AL\
Data File : FC065180.D
Signal(s) : FID1A.ch
Acq On : 17 Nov 2023 06:18
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 17 21:32:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

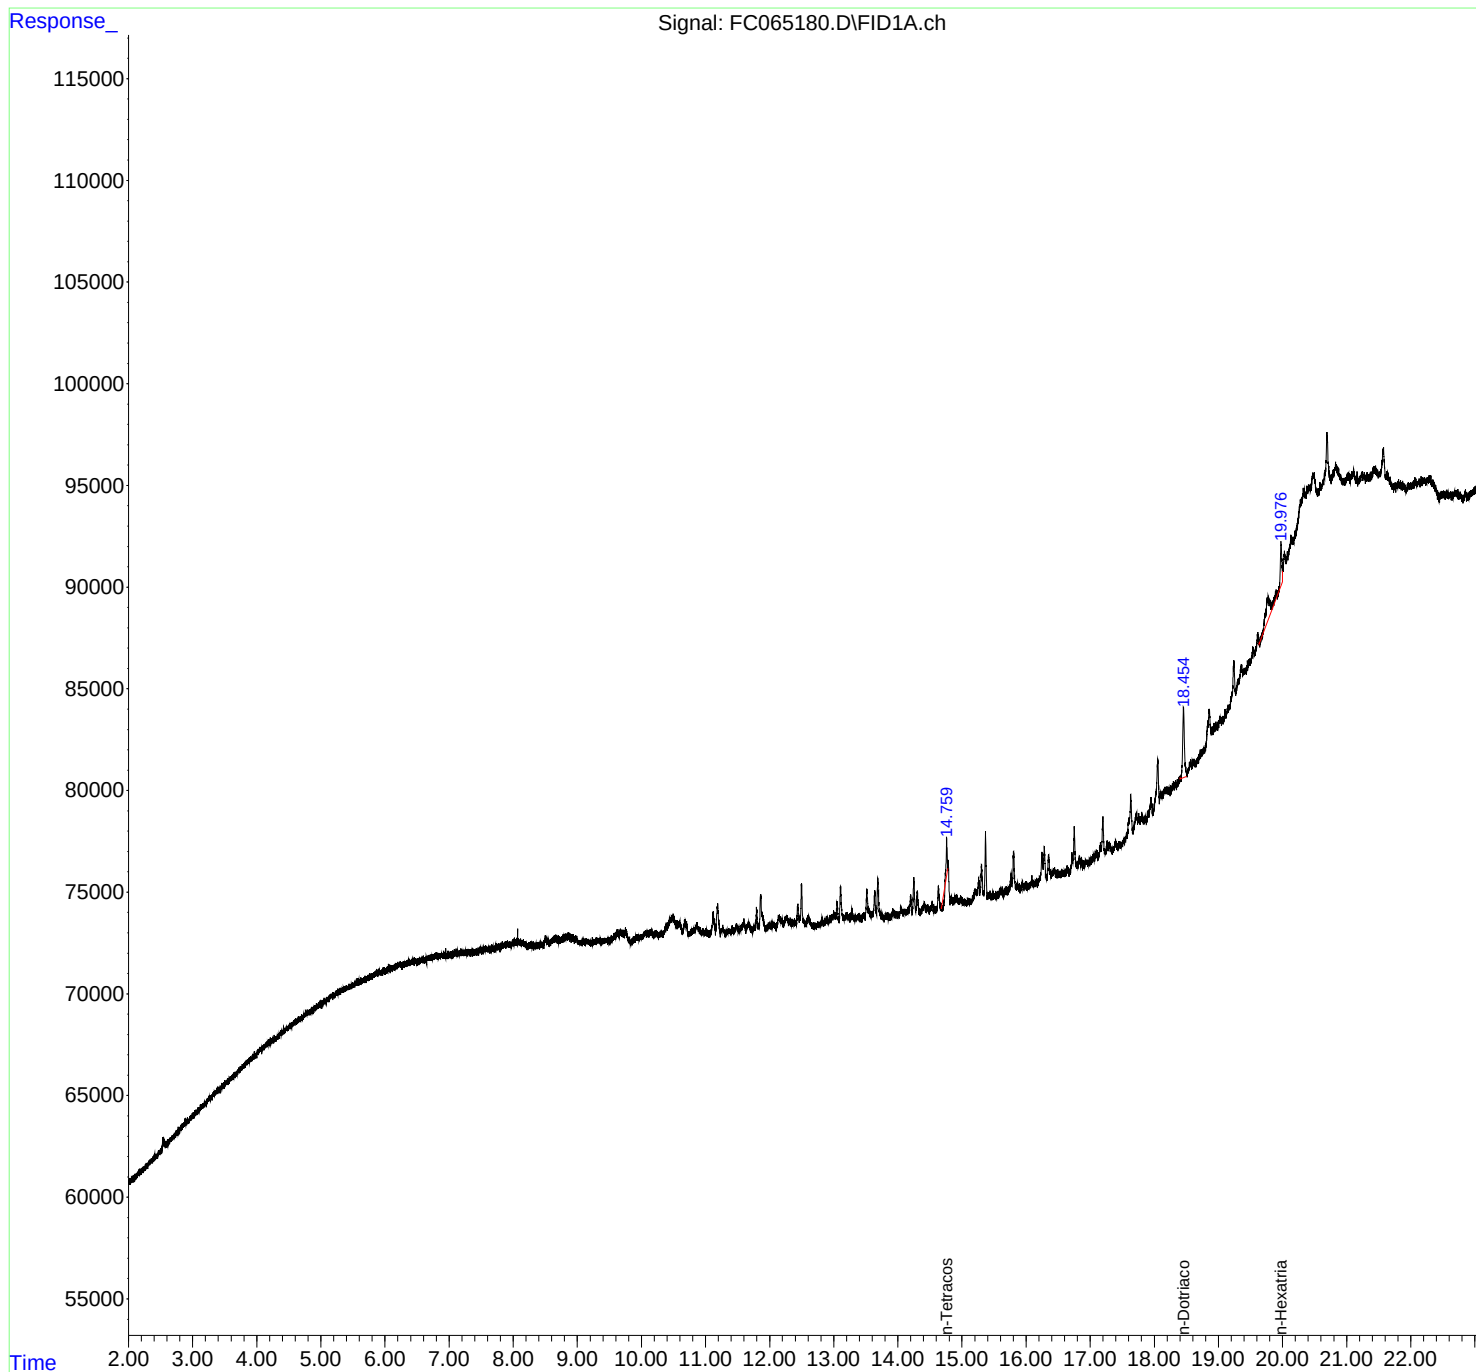


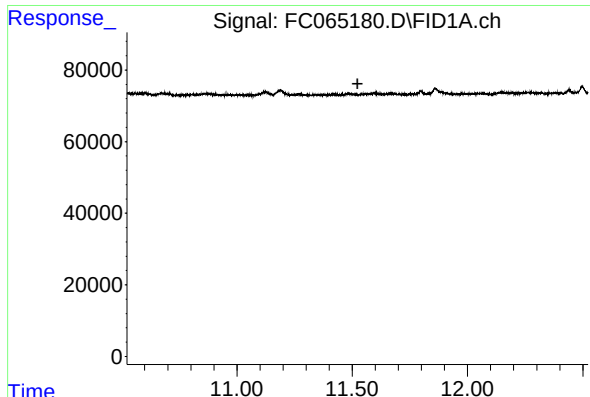

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

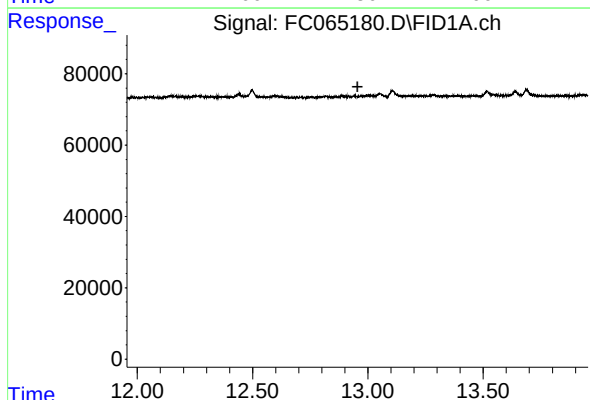


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

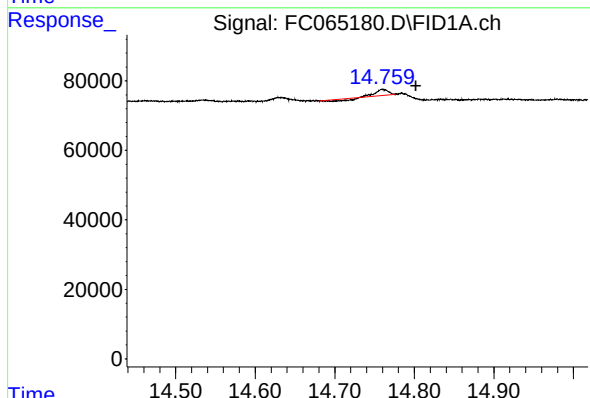


#14 n-Tetracosane (C24)

R.T.: 14.760 min
Delta R.T.: -0.042 min
Response: 9956
Conc: 0.06 ug/ml

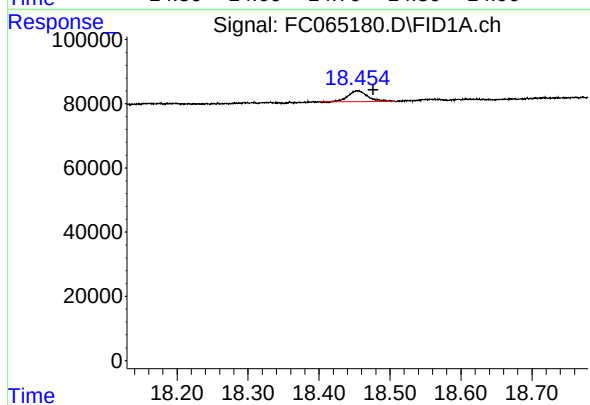

#18 n-Dotriacontane (C32)

R.T.: 18.454 min
Delta R.T.: -0.022 min
Response: 66268
Conc: 0.42 ug/ml

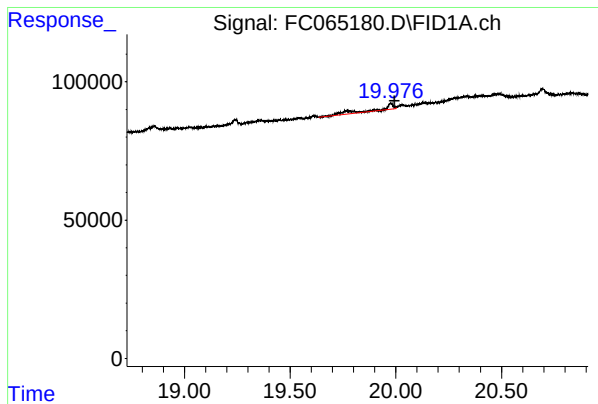

#20 n-Hexatriacontane (C36)

R.T.: 19.976 min
Delta R.T.: -0.018 min
Response: 100455
Conc: 0.67 ug/ml

Instrument :

FID_C

ClientSampleId :