

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111823AL\
 Data File : FC065211.D
 Signal(s) : FID1A.ch
 Acq On : 18 Nov 2023 09:05
 Operator : YP/AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 20 04:10:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.499	68170	0.379 ug/ml
11) T n-Heneicosane (C21)	13.109	57378	0.327 ug/ml
13) T n-Docosane (C22)	13.693	51699	0.301 ug/ml
14) T n-Tetracosane (C24)	14.789	41899	0.252 ug/ml
15) T n-Hexacosane (C26)	15.807	44518	0.277 ug/ml
16) T n-Octacosane (C28)	16.754	55897	0.357 ug/ml
17) T n-Tricontane (C30)	17.639	62136	0.392 ug/ml
18) T n-Dotriacontane (C32)	18.464	99111	0.628 ug/ml
19) T n-Tetratriacontane (C34)	19.248	69502	0.455 ug/ml
20) T n-Hexatriacontane (C36)	19.983	82627	0.548 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC111823AL\
Data File : FC065211.D
Signal(s) : FID1A.ch
Acq On : 18 Nov 2023 09:05
Operator : YP/AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 04:10:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

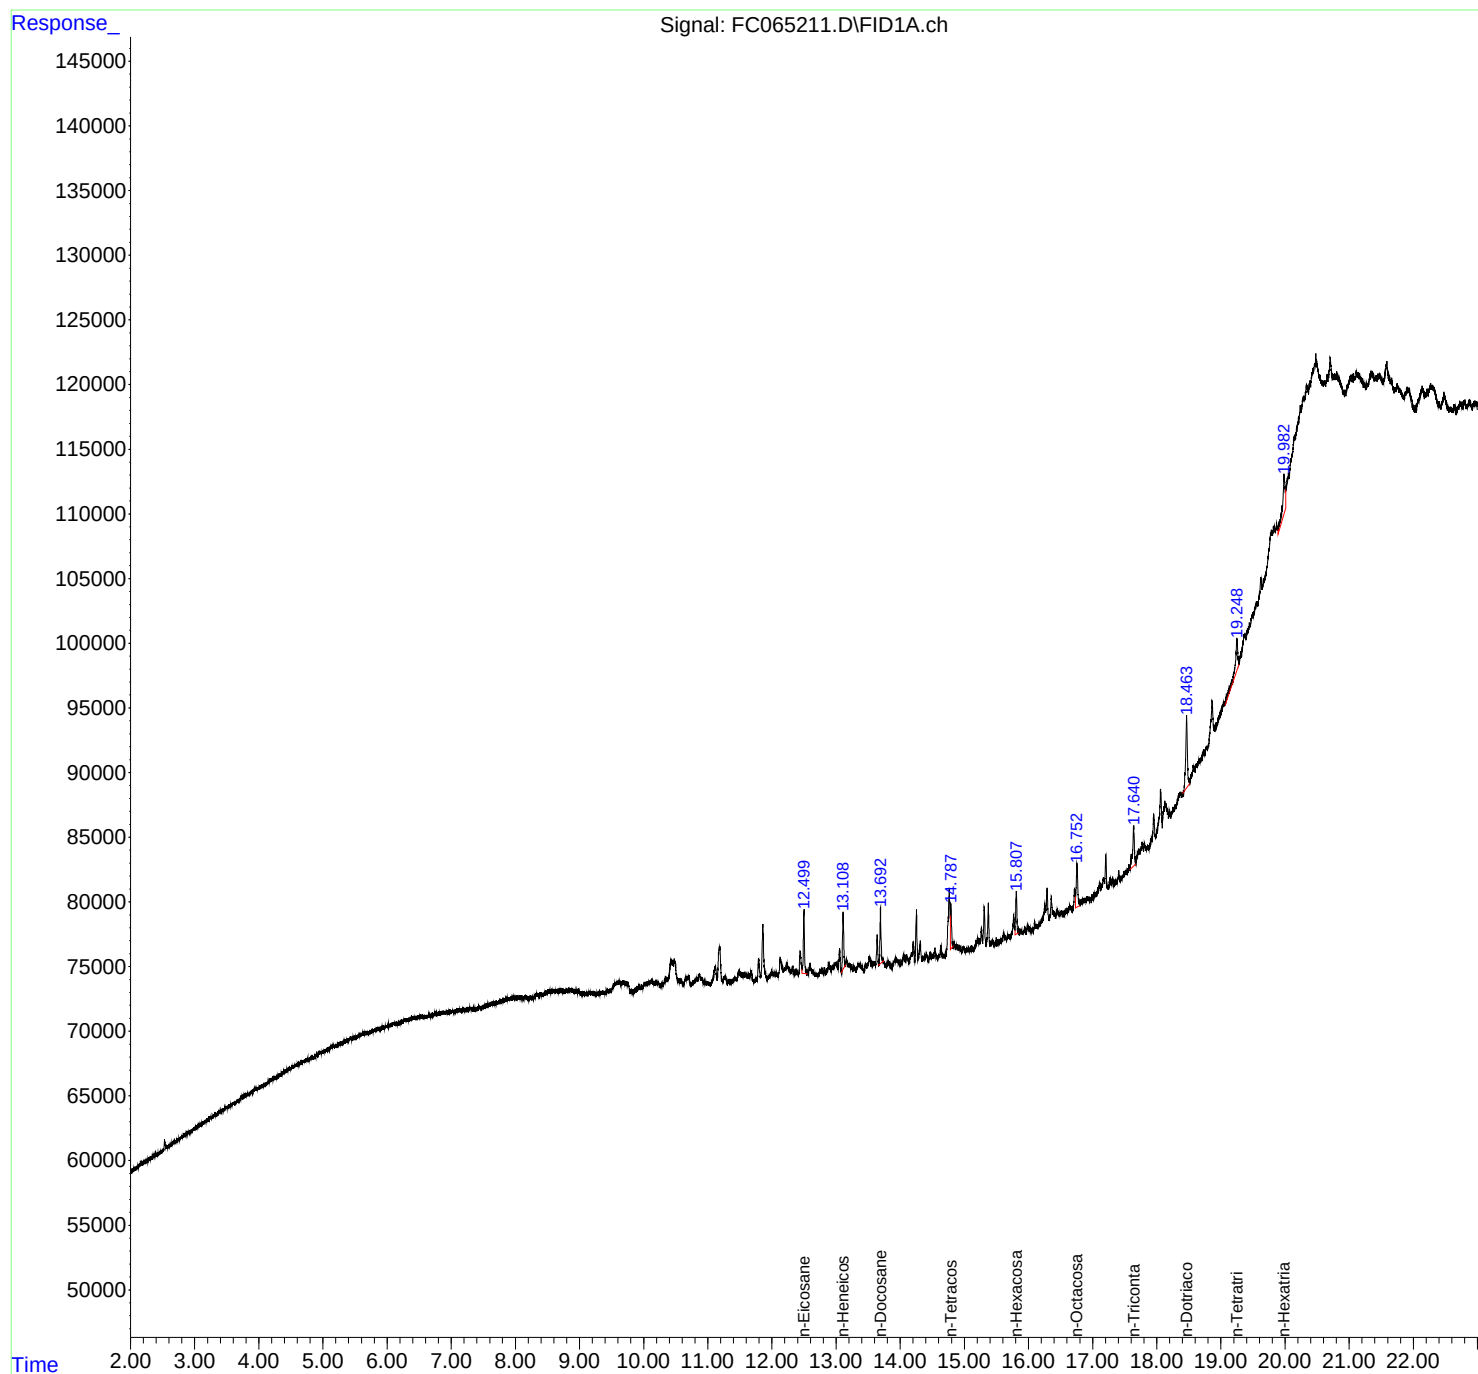


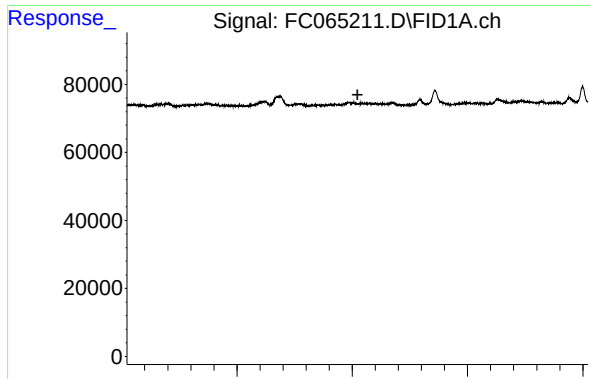

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

Instrument :
FID_C
ClientSampleId :

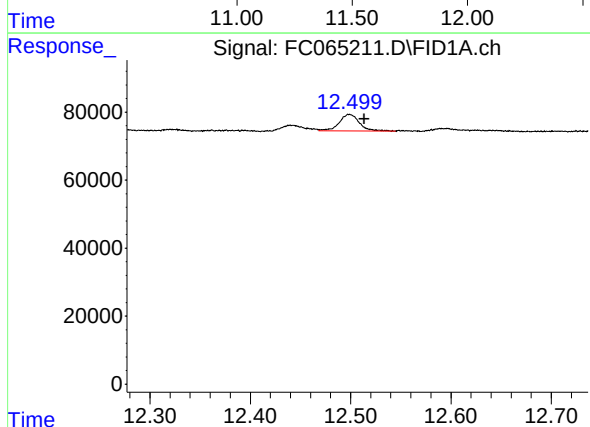


#10 n-Eicosane (C20)

R.T.: 12.499 min
Delta R.T.: -0.015 min
Response: 68170
Conc: 0.38 ug/ml

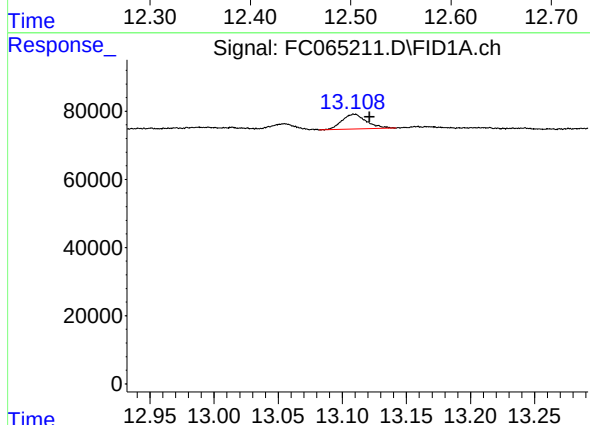


#11 n-Heneicosane (C21)

R.T.: 13.109 min
Delta R.T.: -0.012 min
Response: 57378
Conc: 0.33 ug/ml

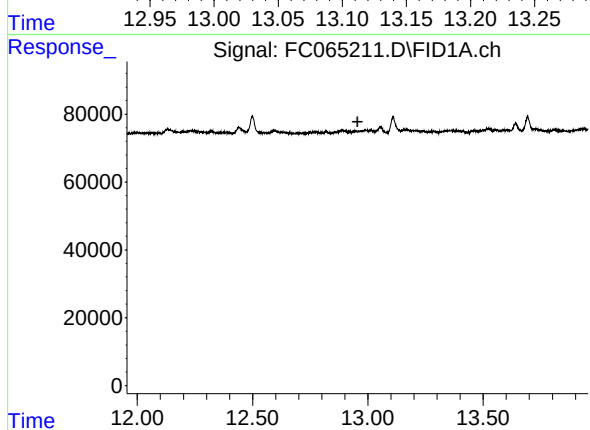

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 12.955 min
Response: 0
Conc: N.D.

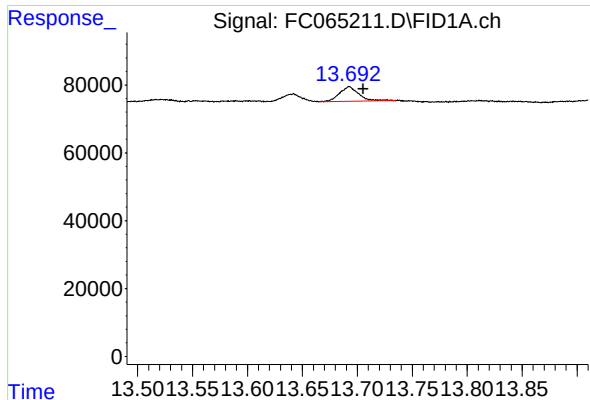

#13 n-Docosane (C22)


R.T.: 13.693 min
Delta R.T.: -0.013 min
Response: 51699
Conc: 0.30 ug/ml

Instrument :
FID_C
ClientSampleId :

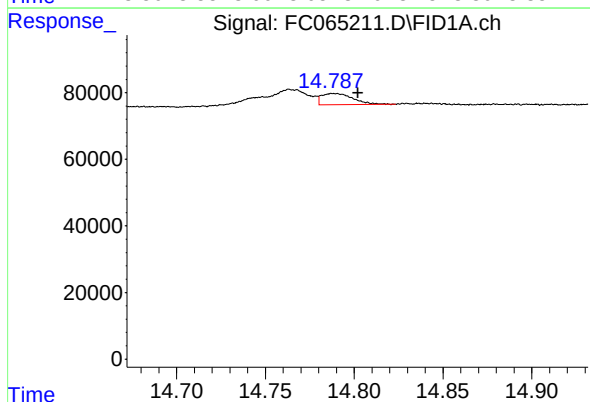


#14 n-Tetracosane (C24)

R.T.: 14.789 min
Delta R.T.: -0.014 min
Response: 41899
Conc: 0.25 ug/ml

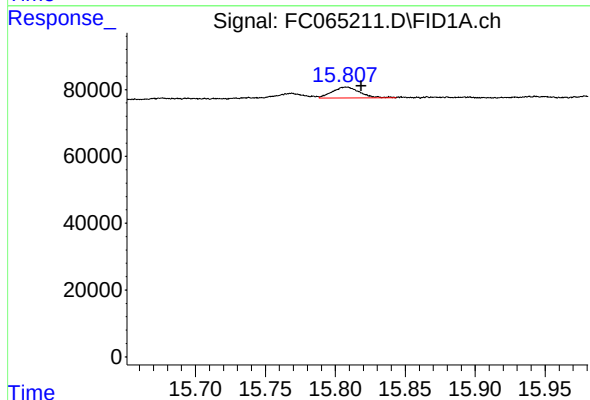


#15 n-Hexacosane (C26)

R.T.: 15.807 min
Delta R.T.: -0.011 min
Response: 44518
Conc: 0.28 ug/ml

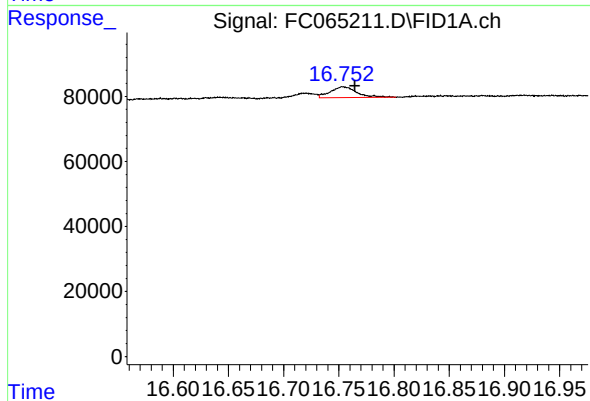

#16 n-Octacosane (C28)


R.T.: 16.754 min
Delta R.T.: -0.011 min
Response: 55897
Conc: 0.36 ug/ml

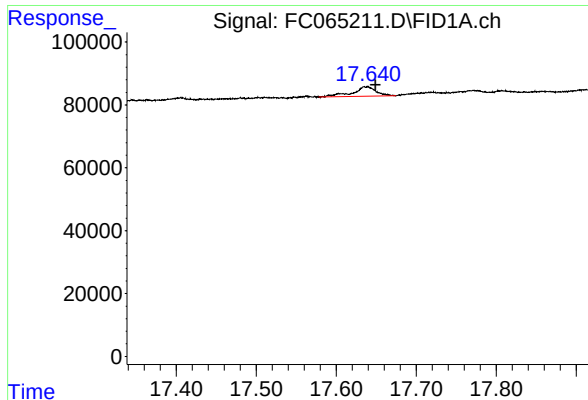

#17 n-Tricontane (C30)


R.T.: 17.639 min
Delta R.T.: -0.010 min
Response: 62136
Conc: 0.39 ug/ml

Instrument :
FID_C
ClientSampleId :

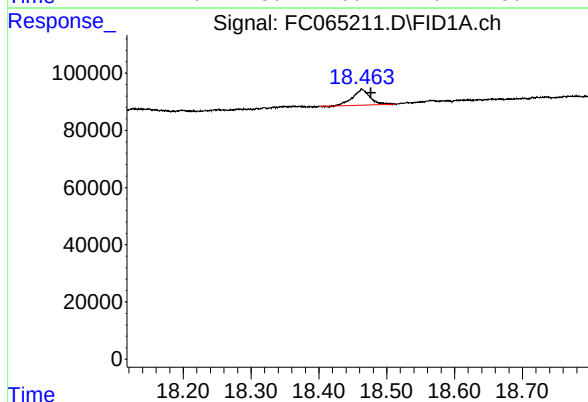


#18 n-Dotriacontane (C32)

R.T.: 18.464 min
Delta R.T.: -0.013 min
Response: 99111
Conc: 0.63 ug/ml

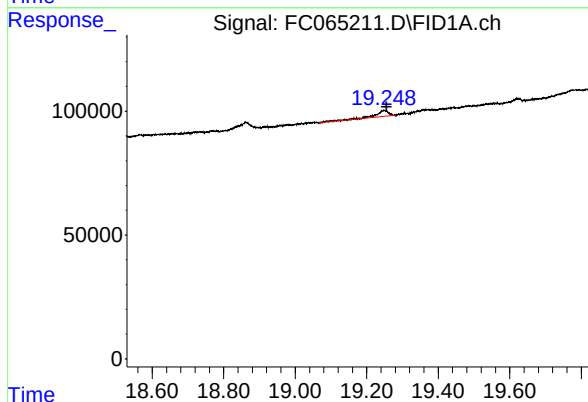

#19 n-Tetratriacontane (C34)

R.T.: 19.248 min
Delta R.T.: -0.007 min
Response: 69502
Conc: 0.46 ug/ml

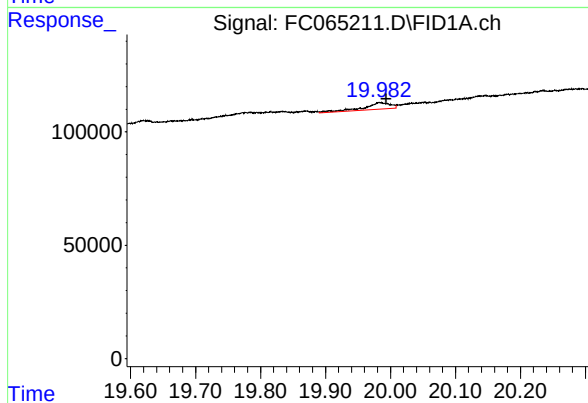

#20 n-Hexatriacontane (C36)

R.T.: 19.983 min
Delta R.T.: -0.011 min
Response: 82627
Conc: 0.55 ug/ml