

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112023AL\
 Data File : FC065241.D
 Signal(s) : FID1A.ch
 Acq On : 20 Nov 2023 21:49
 Operator : YP/AJ
 Sample : 05449-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 21 00:13:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.937	3101196	19.617 ug/ml
Spiked Amount 50.000		Recovery =	39.23%
Target Compounds			
4) T n-Dodecane (C12)	6.378	114179	0.591 ug/ml
14) T n-Tetracosane (C24)	14.784	53188	0.319 ug/ml
15) T n-Hexacosane (C26)	15.800	47092	0.293 ug/ml
16) T n-Octacosane (C28)	16.744	49131	0.314 ug/ml
17) T n-Tricontane (C30)	17.627	44209	0.279 ug/ml
19) T n-Tetratriacontane (C34)	19.263	70580	0.462 ug/ml
20) T n-Hexatriacontane (C36)	19.983	80292	0.532 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112023AL\
Data File : FC065241.D
Signal(s) : FID1A.ch
Acq On : 20 Nov 2023 21:49
Operator : YP/AJ
Sample : 05449-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 21 00:13:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

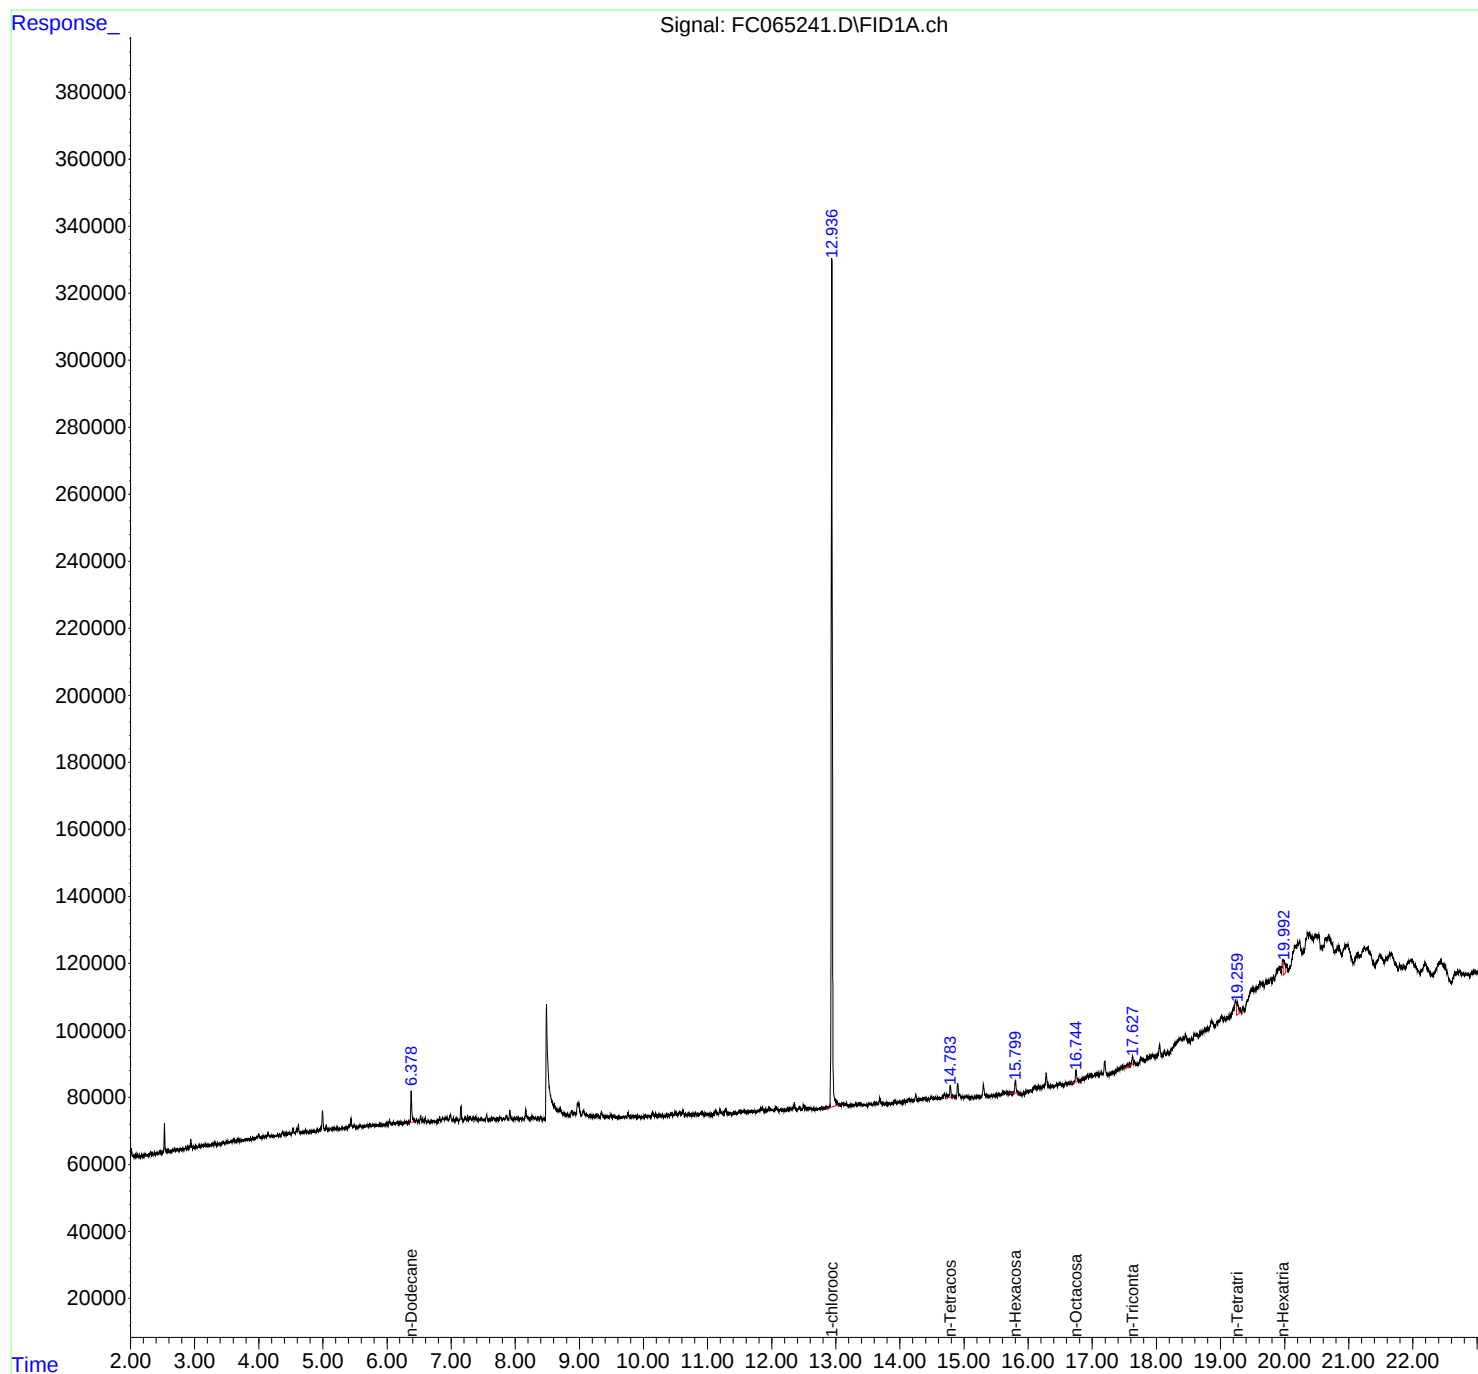


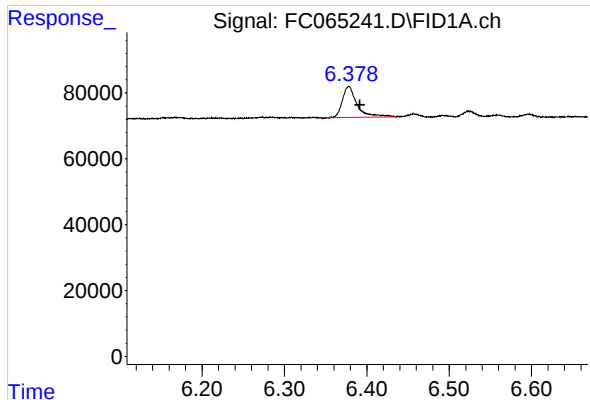

#4 n-Dodecane (C12)


R.T.: 6.378 min
Delta R.T.: -0.013 min
Response: 114179
Conc: 0.59 ug/ml

Instrument :
FID_C
ClientSampleId :

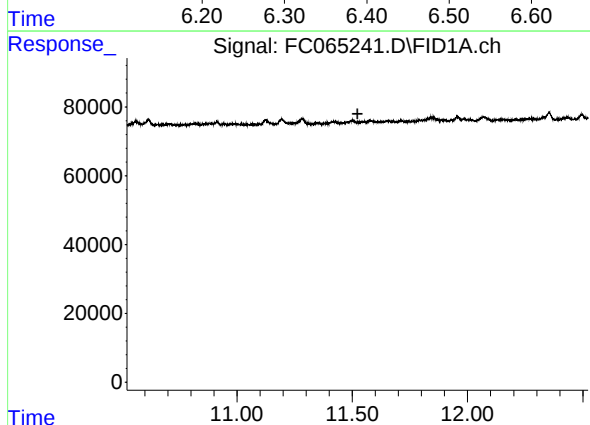


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

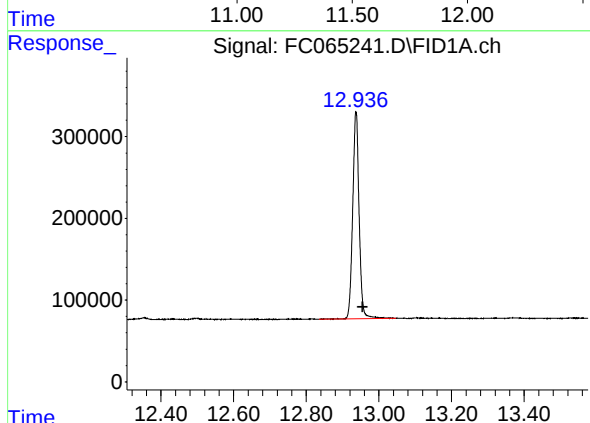


#12 1-chlorooctadecane (SURRE)

R.T.: 12.937 min
Delta R.T.: -0.018 min
Response: 3101196
Conc: 19.62 ug/ml

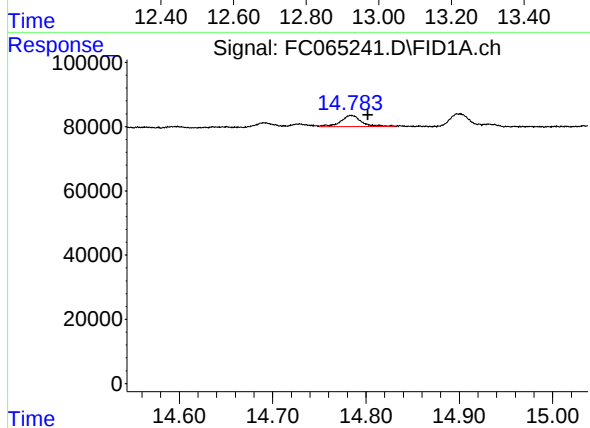

#14 n-Tetracosane (C24)


R.T.: 14.784 min
Delta R.T.: -0.018 min
Response: 53188
Conc: 0.32 ug/ml

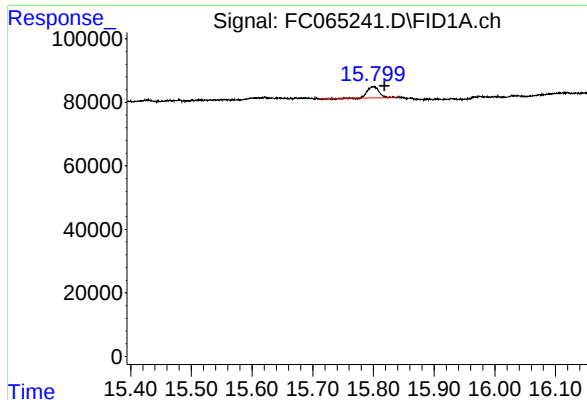

#15 n-Hexacosane (C26)


R.T.: 15.800 min
Delta R.T.: -0.018 min
Response: 47092
Conc: 0.29 ug/ml

Instrument :
FID_C
ClientSampleId :

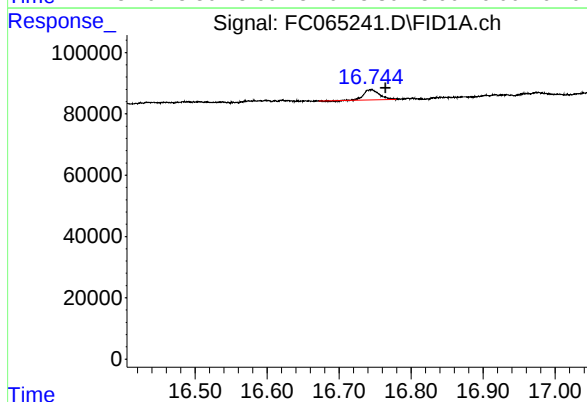


#16 n-Octacosane (C28)

R.T.: 16.744 min
Delta R.T.: -0.020 min
Response: 49131
Conc: 0.31 ug/ml

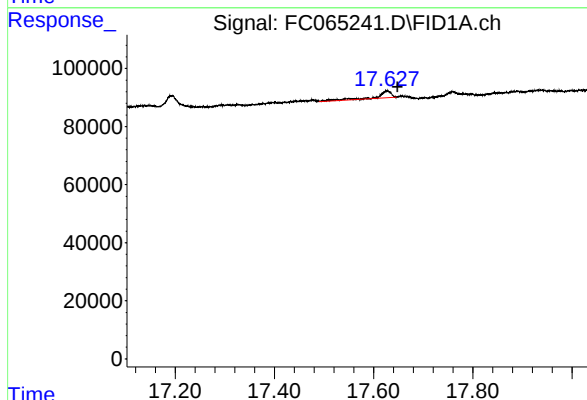


#17 n-Tricontane (C30)

R.T.: 17.627 min
Delta R.T.: -0.022 min
Response: 44209
Conc: 0.28 ug/ml

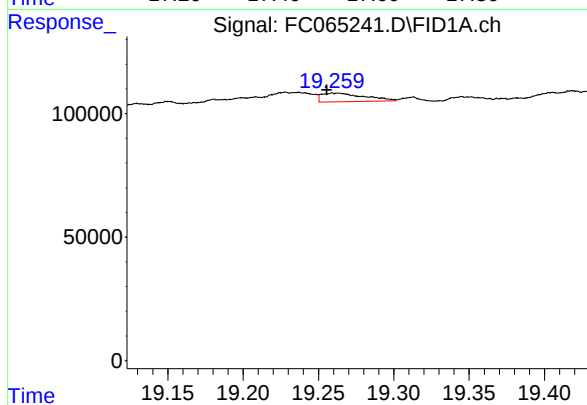

#19 n-Tetratriacontane (C34)

R.T.: 19.263 min
Delta R.T.: 0.007 min
Response: 70580
Conc: 0.46 ug/ml

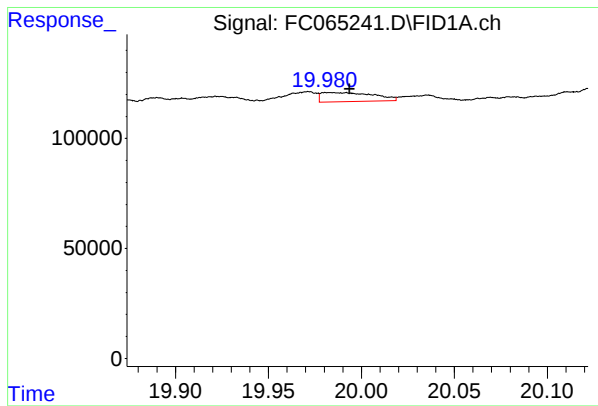

#20 n-Hexatriacontane (C36)

R.T.: 19.983 min
Delta R.T.: -0.011 min
Response: 80292
Conc: 0.53 ug/ml

Instrument :
FID_C
ClientSampleId :