

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112023AL\
 Data File : FC065244.D
 Signal(s) : FID1A.ch
 Acq On : 20 Nov 2023 23:44
 Operator : YP/AJ
 Sample : 05449-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 21 03:03:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.938	4795212	30.333 ug/ml
Spiked Amount 50.000		Recovery =	60.67%
Target Compounds			
4) T n-Dodecane (C12)	6.378	104533	0.541 ug/ml
14) T n-Tetracosane (C24)	14.784	60254	0.362 ug/ml
15) T n-Hexacosane (C26)	15.800	65507	0.408 ug/ml
16) T n-Octacosane (C28)	16.745	65278	0.417 ug/ml
17) T n-Tricontane (C30)	17.626	90831	0.573 ug/ml
19) T n-Tetratriacontane (C34)	19.239	31902	0.209 ug/ml
20) T n-Hexatriacontane (C36)	19.971	167368	1.109 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112023AL\
Data File : FC065244.D
Signal(s) : FID1A.ch
Acq On : 20 Nov 2023 23:44
Operator : YP/AJ
Sample : 05449-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 21 03:03:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

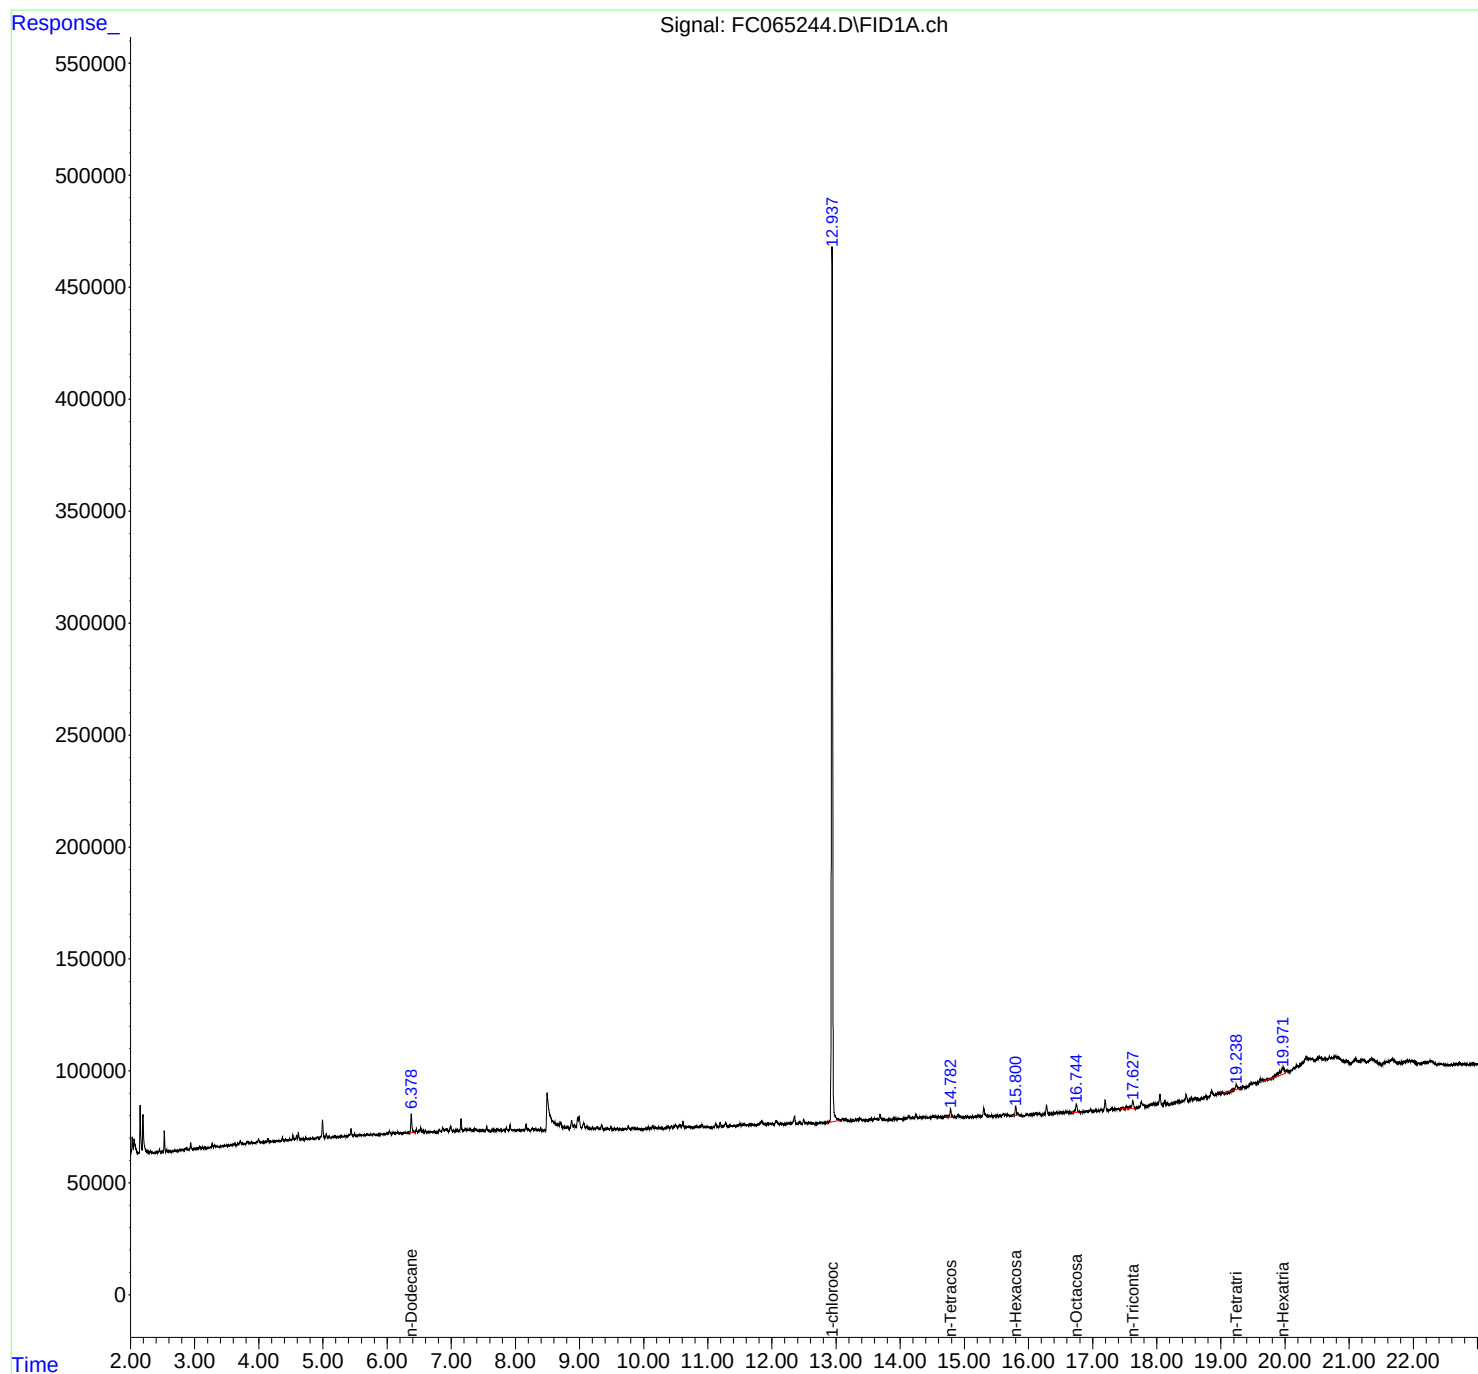


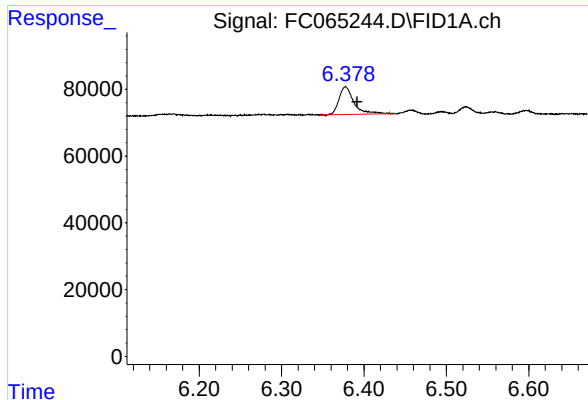

#4 n-Dodecane (C12)


R.T.: 6.378 min
Delta R.T.: -0.014 min
Response: 104533
Conc: 0.54 ug/ml

Instrument :
FID_C
ClientSampleId :

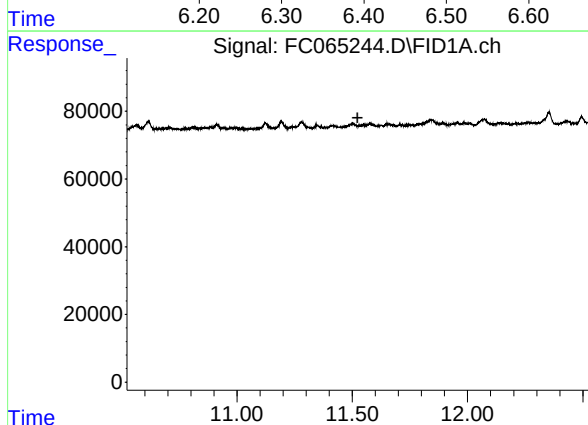


#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

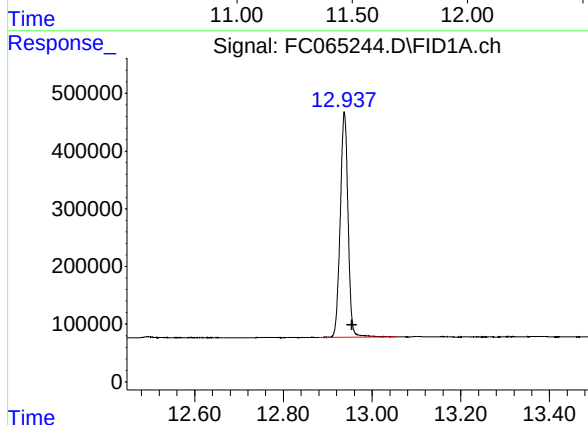


#12 1-chlorooctadecane (SURRE)

R.T.: 12.938 min
Delta R.T.: -0.017 min
Response: 4795212
Conc: 30.33 ug/ml

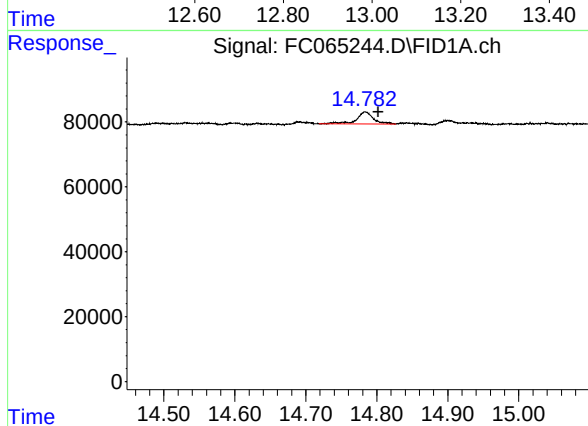

#14 n-Tetracosane (C24)

R.T.: 14.784 min
Delta R.T.: -0.019 min
Response: 60254
Conc: 0.36 ug/ml

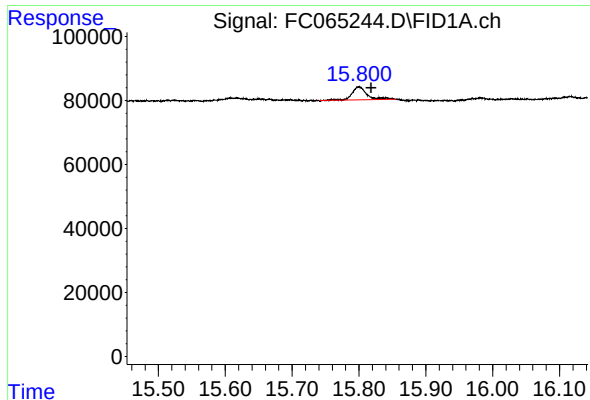


#15 n-Hexacosane (C26)

R.T.: 15.800 min
Delta R.T.: -0.019 min
Response: 65507
Conc: 0.41 ug/ml

Instrument :


FID_C

ClientSampleId :

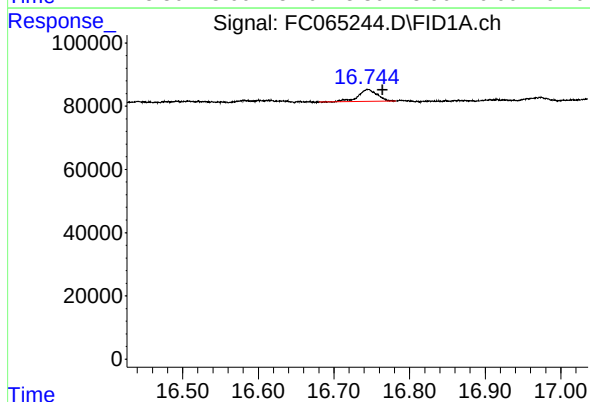


#16 n-Octacosane (C28)

R.T.: 16.745 min
Delta R.T.: -0.020 min
Response: 65278
Conc: 0.42 ug/ml

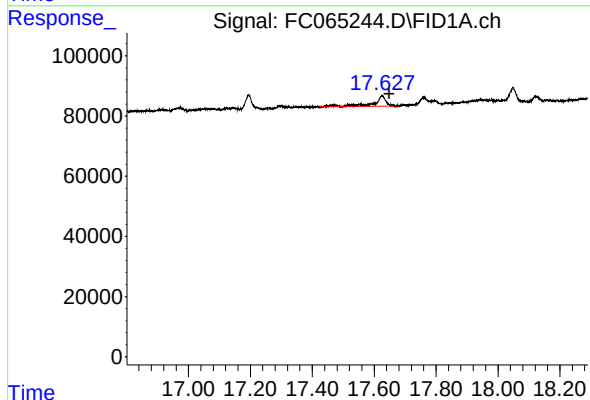


#17 n-Tricontane (C30)

R.T.: 17.626 min
Delta R.T.: -0.024 min
Response: 90831
Conc: 0.57 ug/ml

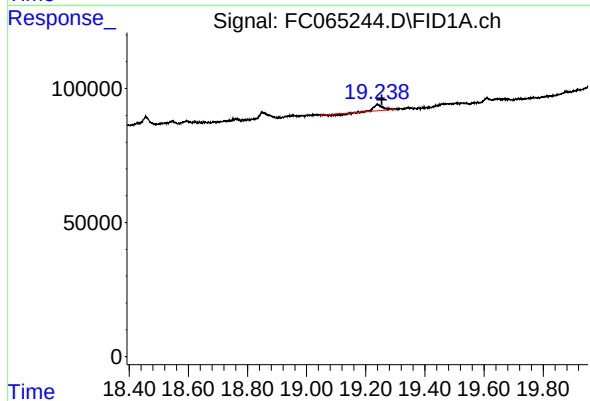

#19 n-Tetratriacontane (C34)

R.T.: 19.239 min
Delta R.T.: -0.017 min
Response: 31902
Conc: 0.21 ug/ml

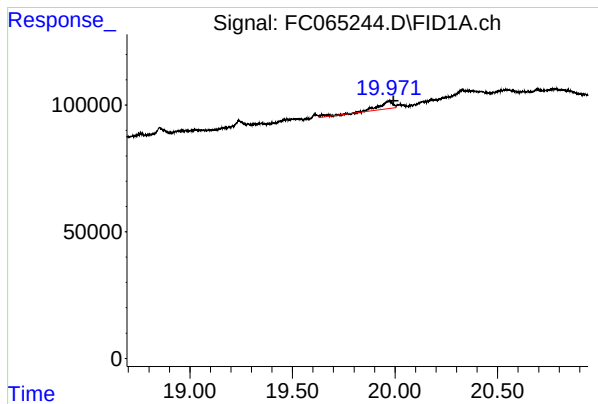

#20 n-Hexatriacontane (C36)

R.T.: 19.971 min
Delta R.T.: -0.023 min
Response: 167368
Conc: 1.11 ug/ml

Instrument :

FID_C

ClientSampleId :