

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC112122AL\  
 Data File : FC062230.D  
 Signal(s) : FID1A.ch  
 Acq On : 22 Nov 2022 04:03  
 Operator : YP/AJ  
 Sample : N5691-01DL 2X  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 FID\_C  
 ClientSampleId :  
 ETGI-358DL

Integration File: autoint1.e  
 Quant Time: Nov 22 04:50:54 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 111422.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Nov 21 12:12:05 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.605 | 2173138    | 15.921 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 31.84%       |
| 12) S 1-chlorooctadecane (S... | 13.043 | 1741009    | 17.127 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 34.25%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_C\Data\FC112122AL\  
Data File : FC062230.D  
Signal(s) : FID1A.ch  
Acq On : 22 Nov 2022 04:03  
Operator : YP/AJ  
Sample : N5691-01DL 2X  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
FID\_C  
ClientSampleId :  
ETGI-358DL

Integration File: autoint1.e  
Quant Time: Nov 22 04:50:54 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_C\Method\Aliphatic EPH 111422.M  
Quant Title : GC Extractables  
QLast Update : Mon Nov 21 12:12:05 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

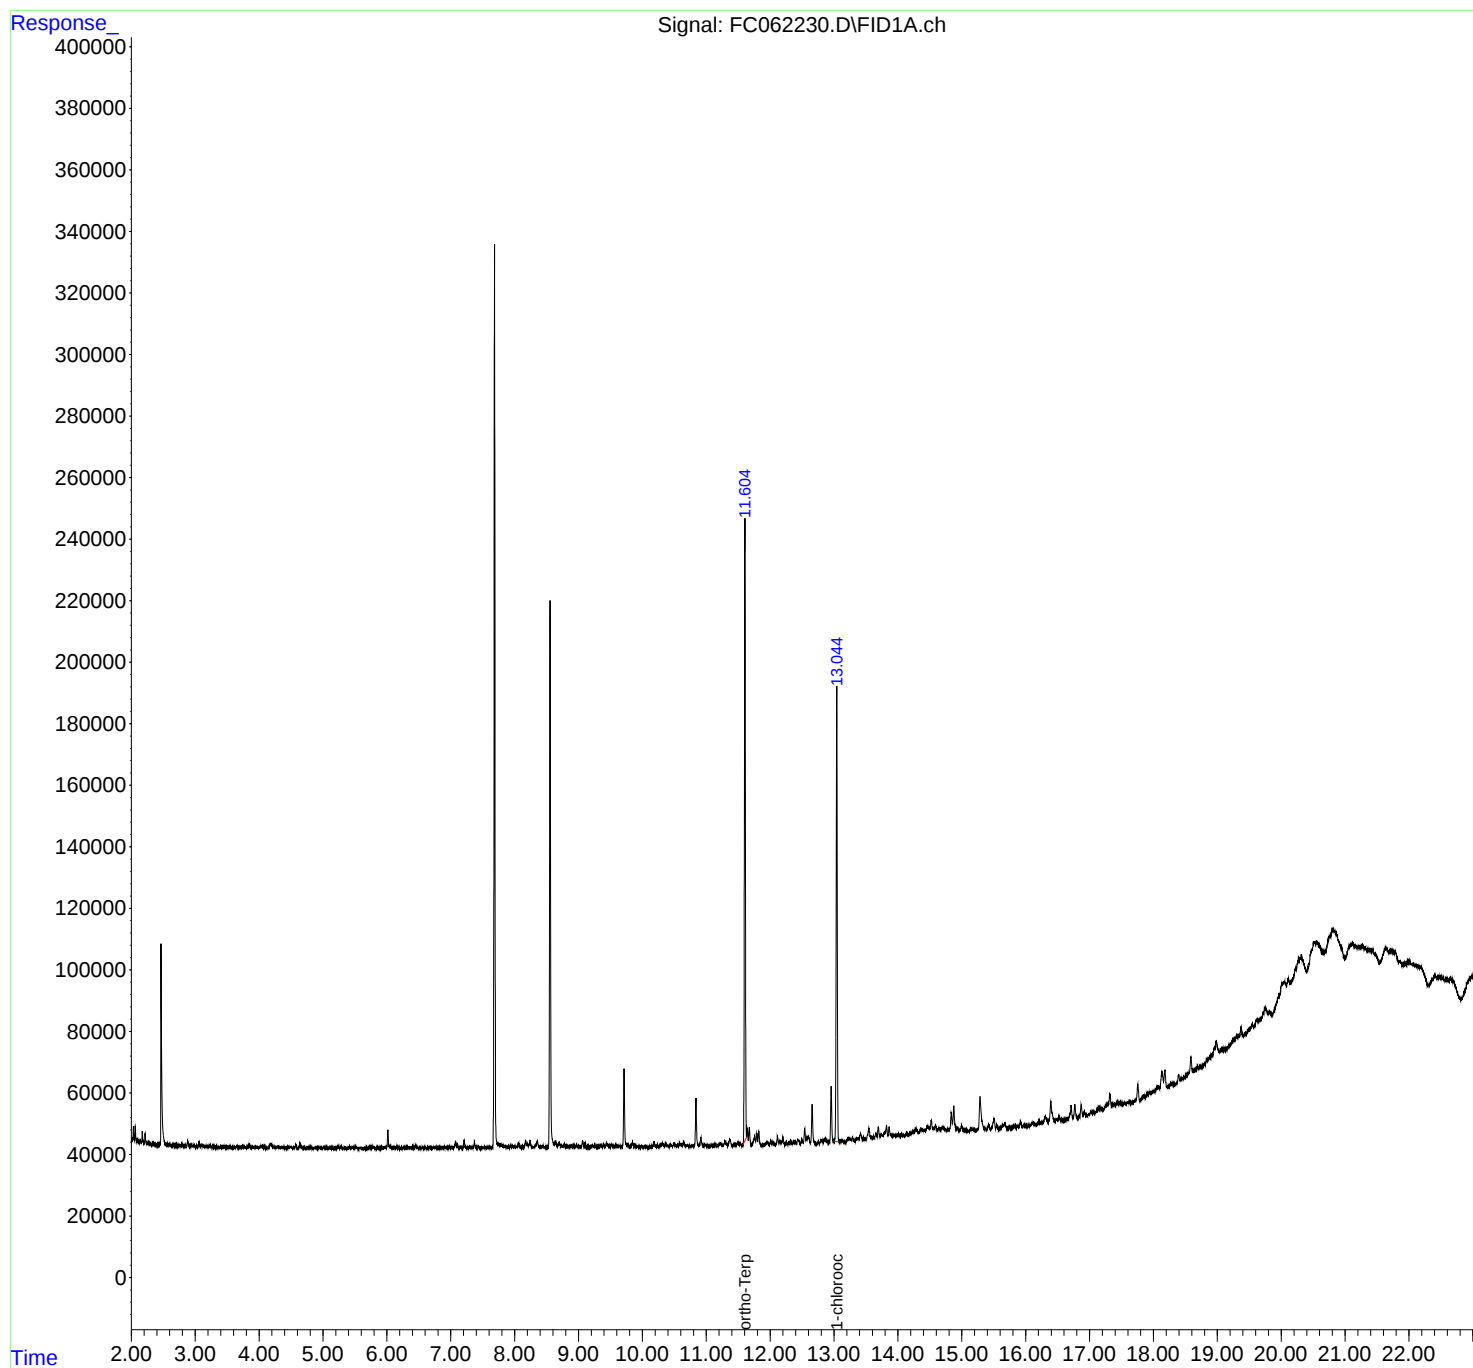


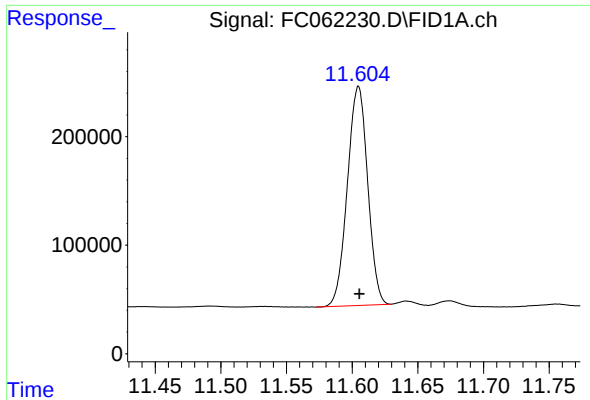

#9 ortho-Terphenyl (SURR)

R.T.: 11.605 min  
Delta R.T.: 0.000 min  
Response: 2173138  
Conc: 15.92 ug/ml

Instrument :  
FID\_C  
ClientSampleId :  
ETGI-358DL

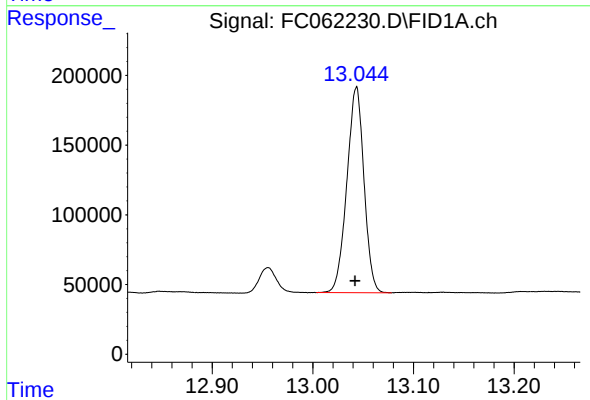

#12 1-chlorooctadecane (SURR)

R.T.: 13.043 min  
Delta R.T.: 0.001 min  
Response: 1741009  
Conc: 17.13 ug/ml