

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112123AL\
 Data File : FC065258.D
 Signal(s) : FID1A.ch
 Acq On : 21 Nov 2023 10:02
 Operator : YP/AJ
 Sample : 05449-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_C
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 21 22:49:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 28 02:12:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.936	3985244	25.210 ug/ml
Spiked Amount 50.000		Recovery =	50.42%
Target Compounds			
4) T n-Dodecane (C12)	6.378	103034	0.533 ug/ml
14) T n-Tetracosane (C24)	14.783	56923	0.342 ug/ml
15) T n-Hexacosane (C26)	15.799	95861	0.597 ug/ml
16) T n-Octacosane (C28)	16.743	91581	0.585 ug/ml
17) T n-Tricontane (C30)	17.628	84629	0.534 ug/ml
18) T n-Dotriacontane (C32)	18.455	60658	0.384 ug/ml
20) T n-Hexatriacontane (C36)	19.971	32312	0.214 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC112123AL\
Data File : FC065258.D
Signal(s) : FID1A.ch
Acq On : 21 Nov 2023 10:02
Operator : YP/AJ
Sample : 05449-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_C
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 21 22:49:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 102823.M
Quant Title : GC Extractables
QLast Update : Sat Oct 28 02:12:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

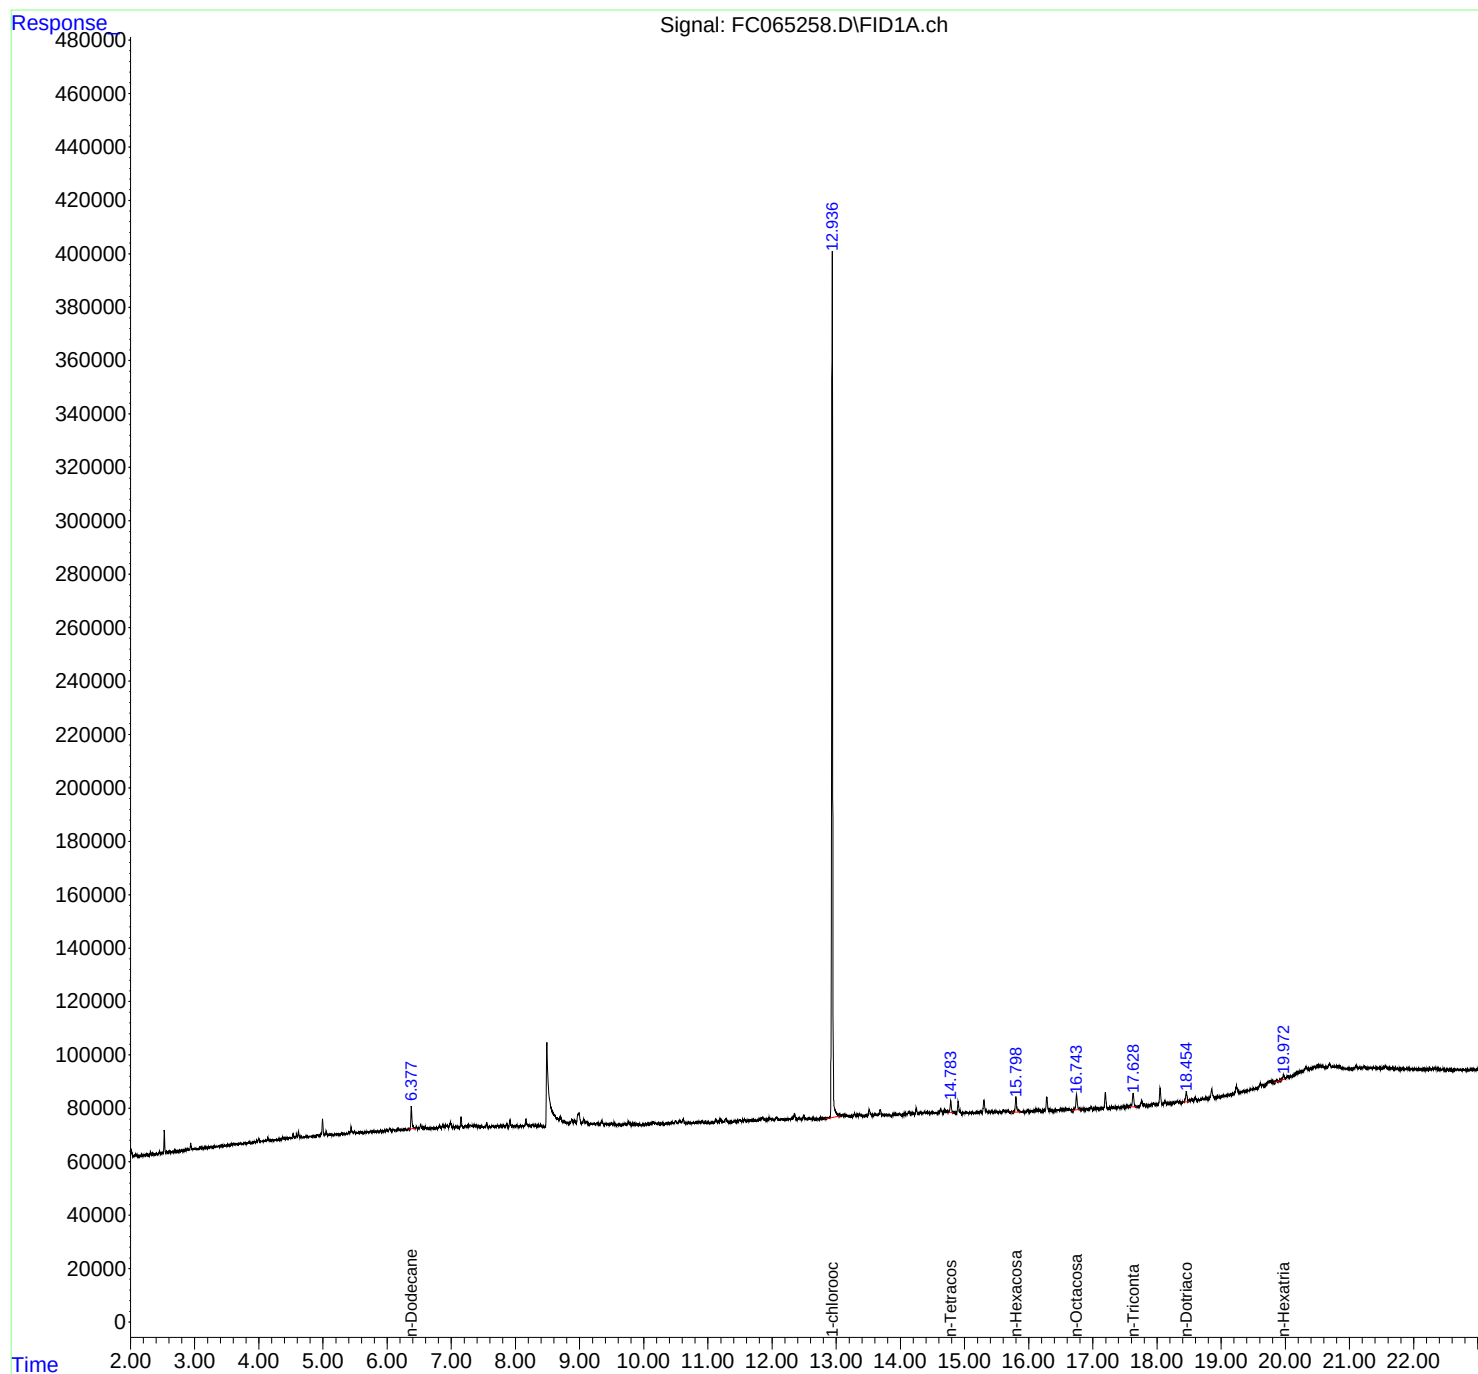


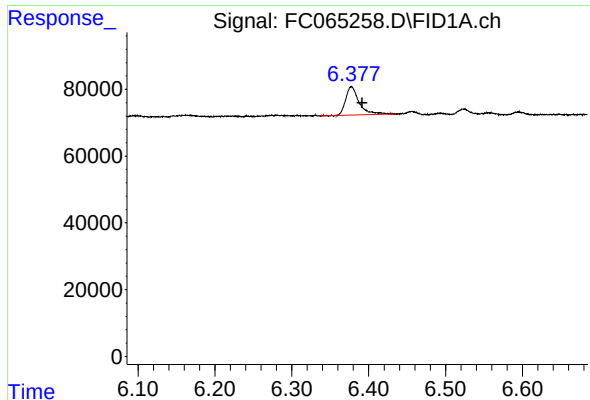

#4 n-Dodecane (C12)


R.T.: 6.378 min
Delta R.T.: -0.014 min
Response: 103034
Conc: 0.53 ug/ml

Instrument :
FID_C
ClientSampleId :

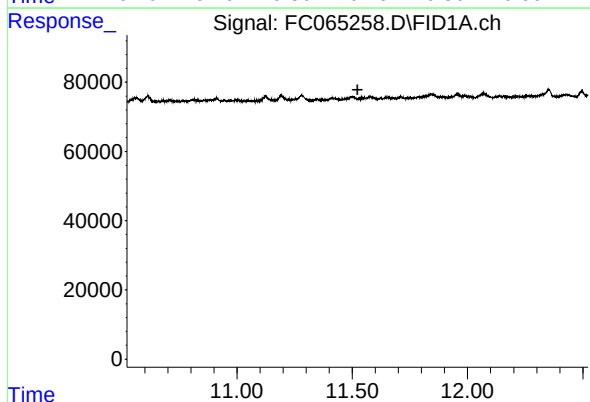


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.523 min
Response: 0
Conc: N.D.

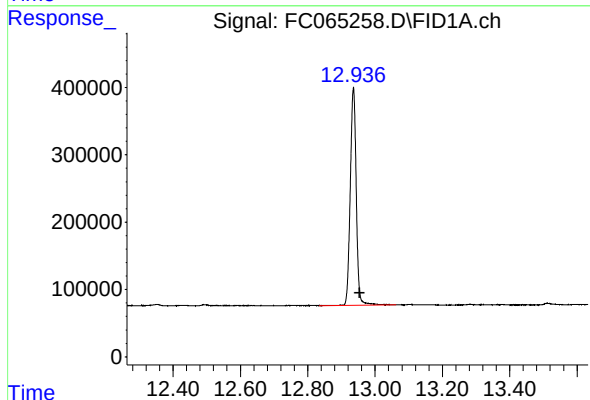


#12 1-chlorooctadecane (SURR)

R.T.: 12.936 min
Delta R.T.: -0.019 min
Response: 3985244
Conc: 25.21 ug/ml

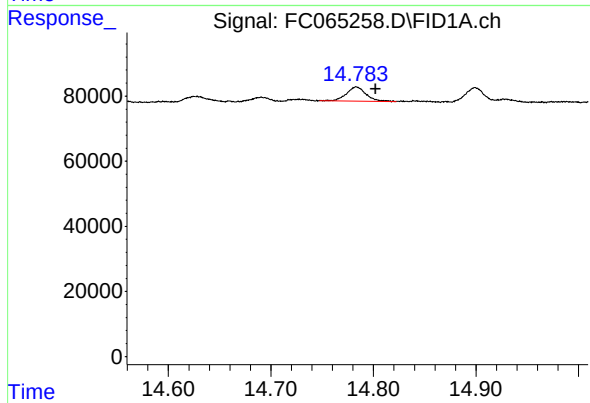

#14 n-Tetracosane (C24)


R.T.: 14.783 min
Delta R.T.: -0.019 min
Response: 56923
Conc: 0.34 ug/ml

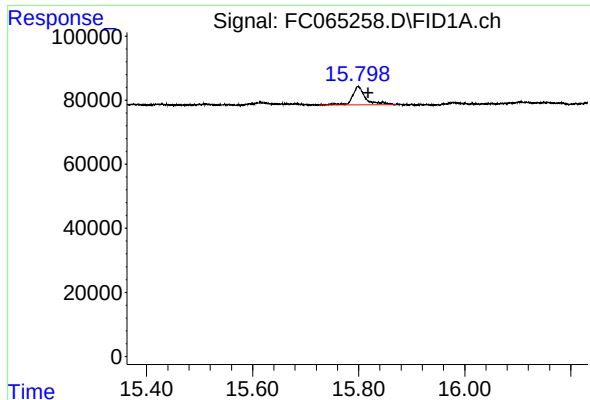

#15 n-Hexacosane (C26)


R.T.: 15.799 min
Delta R.T.: -0.020 min
Response: 95861
Conc: 0.60 ug/ml

Instrument :
FID_C
ClientSampleId :

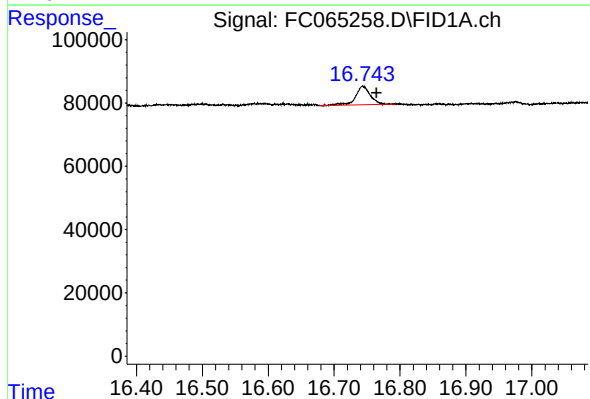


#16 n-Octacosane (C28)

R.T.: 16.743 min
Delta R.T.: -0.021 min
Response: 91581
Conc: 0.59 ug/ml

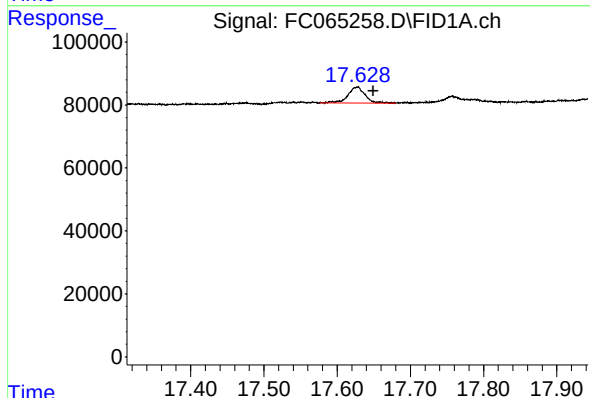


#17 n-Tricontane (C30)

R.T.: 17.628 min
Delta R.T.: -0.021 min
Response: 84629
Conc: 0.53 ug/ml

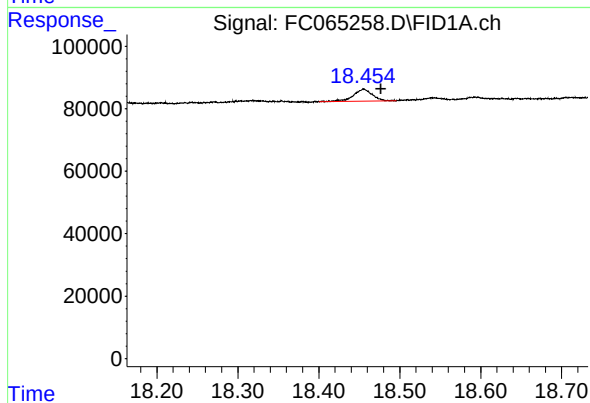

#18 n-Dotriacontane (C32)

R.T.: 18.455 min
Delta R.T.: -0.021 min
Response: 60658
Conc: 0.38 ug/ml

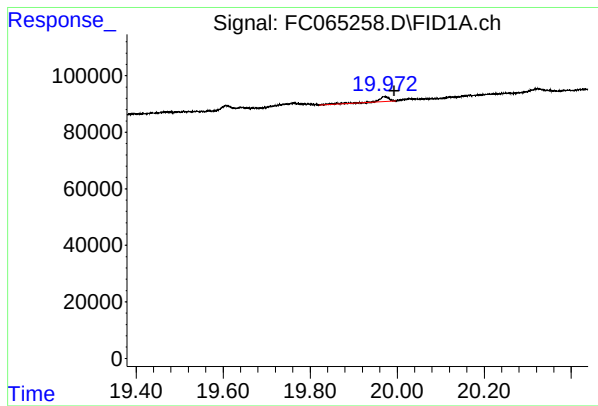

#20 n-Hexatriacontane (C36)

R.T.: 19.971 min
Delta R.T.: -0.023 min
Response: 32312
Conc: 0.21 ug/ml

Instrument :

FID_C

ClientSampleId :